

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031022\
 Data File : P0085284.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2022 20:03
 Operator : YP\AJ
 Sample : N1645-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:21:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.496	3.590	2893423	915156	16.851	20.055
2) SA Decachlor...	10.402	8.608	1435892	855670	21.928m	22.475
Target Compounds						
8) L2 AR-1221-1	4.708	3.806	80478	24158	43.553	43.825
9) L2 AR-1221-2	4.799	3.890	88991	28768	66.901	67.664
10) L2 AR-1221-3	4.873	3.967	203519	65934	52.170	50.618



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031022\
Data File : P0085284.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2022 20:03
Operator : YP\AJ
Sample : N1645-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:21:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

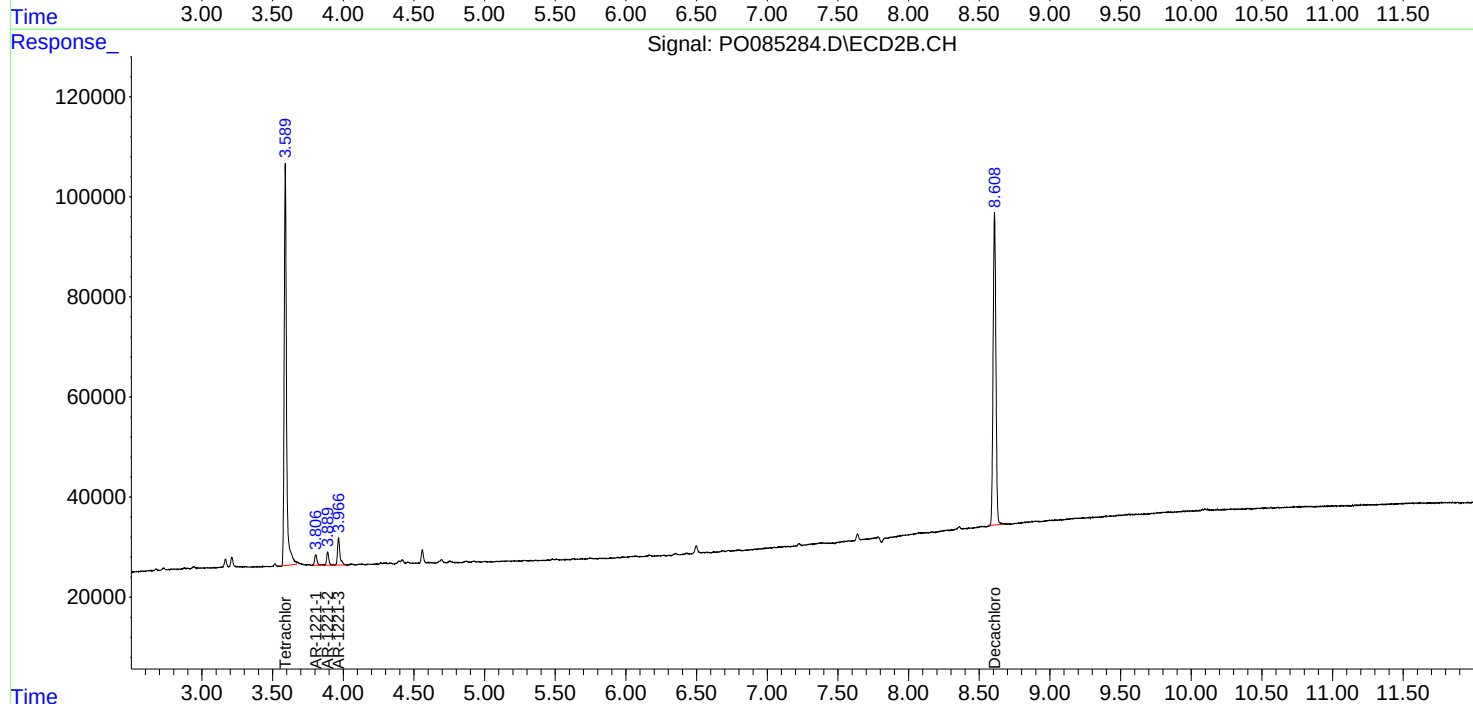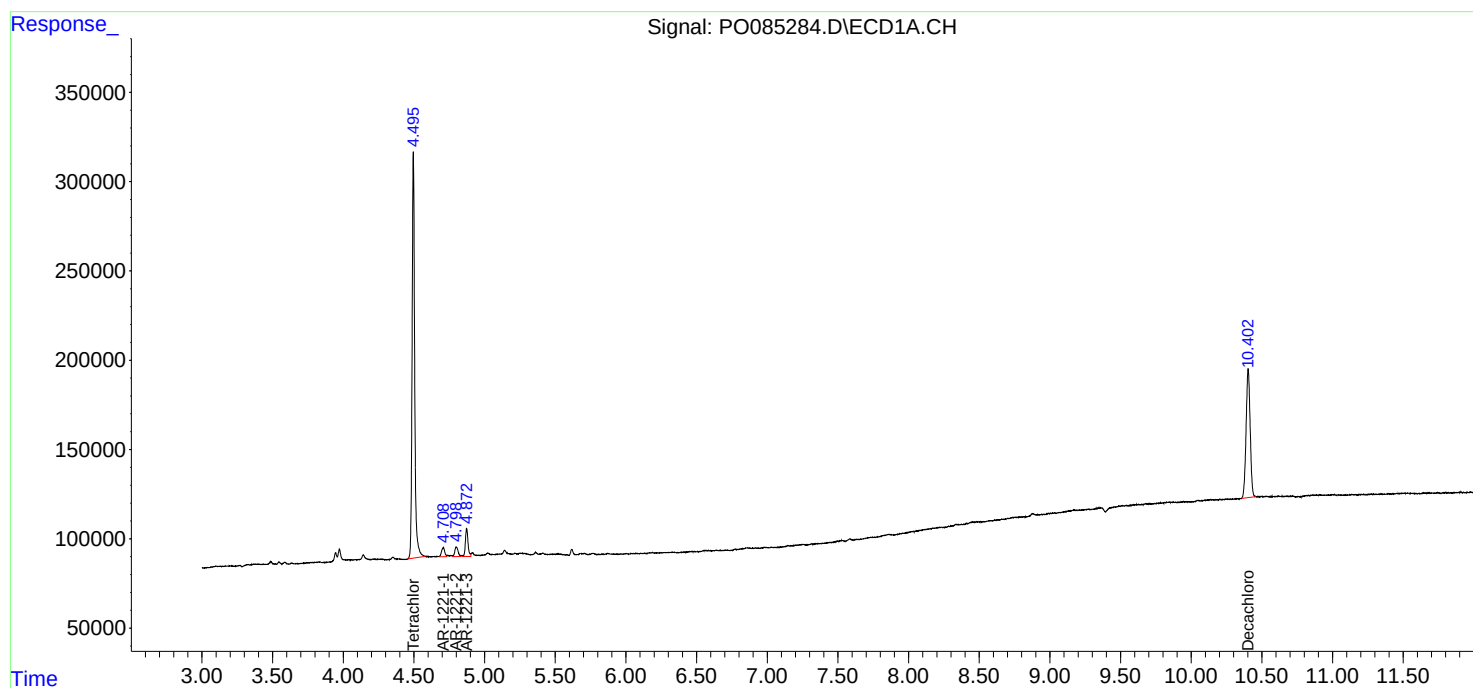


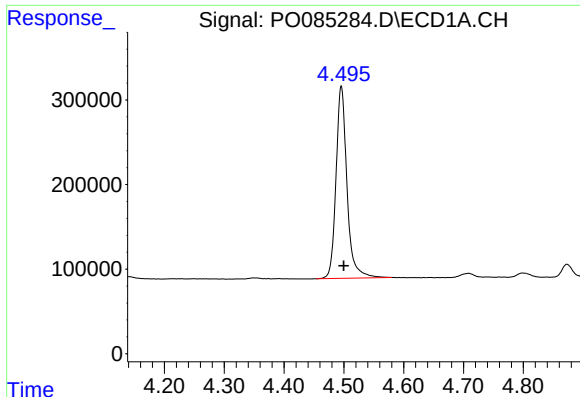

#1 Tetrachloro-m-xylene


R.T.: 4.496 min
Delta R.T.: -0.004 min
Response: 2893423
Conc: 16.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

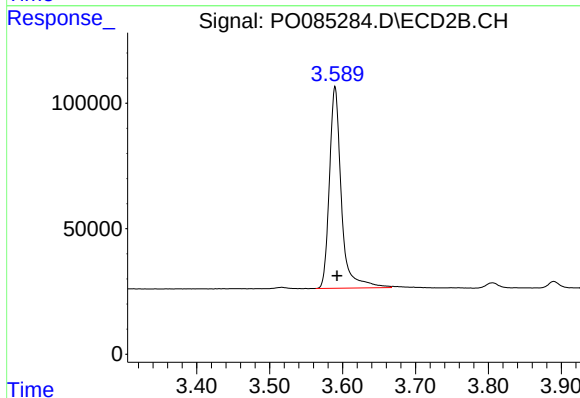


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.002 min
Response: 915156
Conc: 20.06 ng/ml

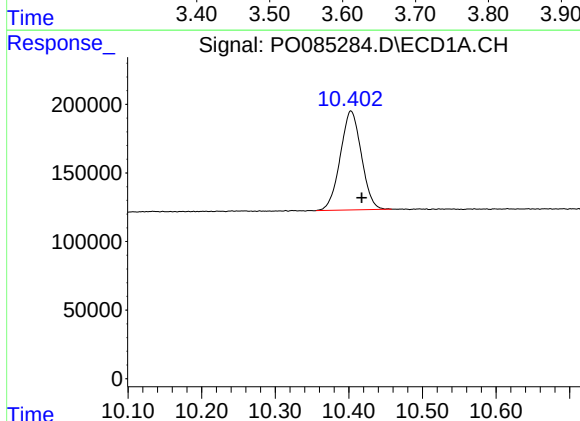


#2 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.015 min
Response: 1435892
Conc: 21.93 ng/ml m

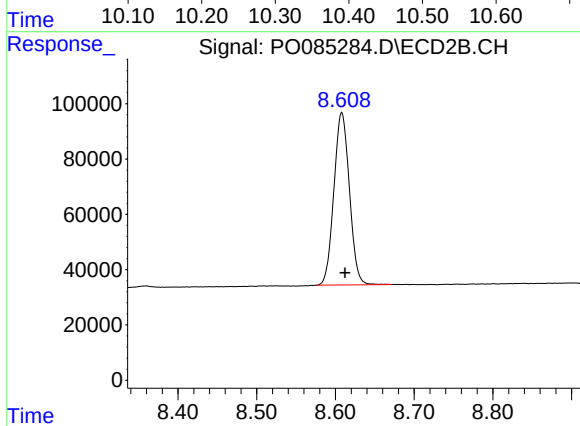

#2 Decachlorobiphenyl


R.T.: 8.608 min
Delta R.T.: -0.004 min
Response: 855670
Conc: 22.48 ng/ml

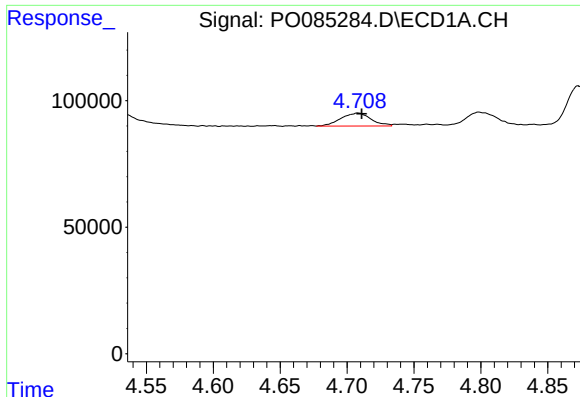

#8 AR-1221-1


R.T.: 4.708 min
Delta R.T.: -0.003 min
Response: 80478
Conc: 43.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

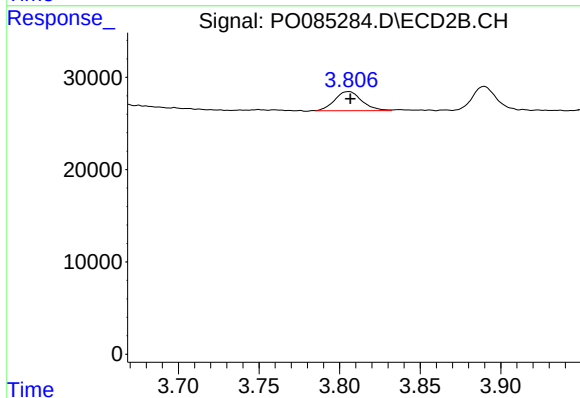


#8 AR-1221-1

R.T.: 3.806 min
Delta R.T.: -0.001 min
Response: 24158
Conc: 43.82 ng/ml

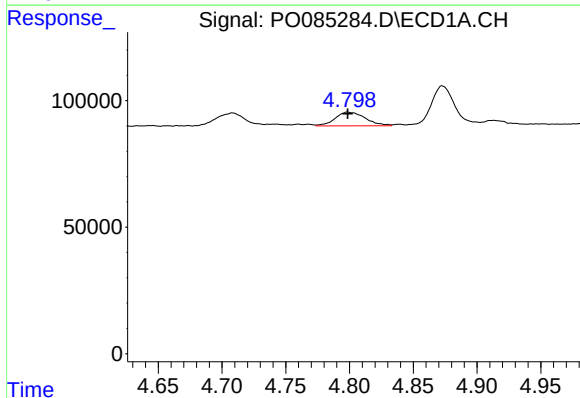


#9 AR-1221-2

R.T.: 4.799 min
Delta R.T.: 0.000 min
Response: 88991
Conc: 66.90 ng/ml

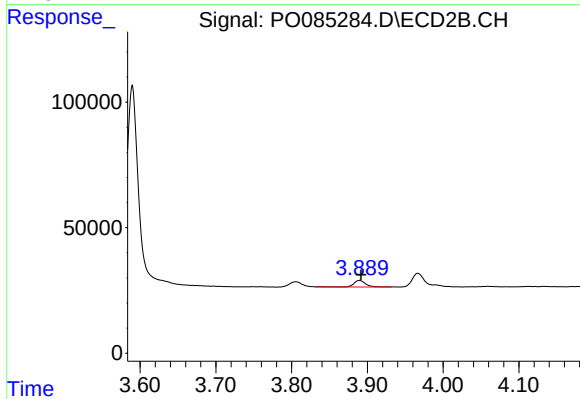

#9 AR-1221-2


R.T.: 3.890 min
Delta R.T.: -0.002 min
Response: 28768
Conc: 67.66 ng/ml

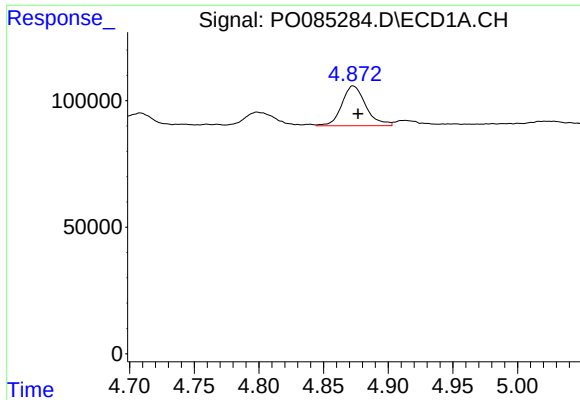

#10 AR-1221-3

R.T.: 4.873 min
Delta R.T.: -0.004 min
Response: 203519
Conc: 52.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

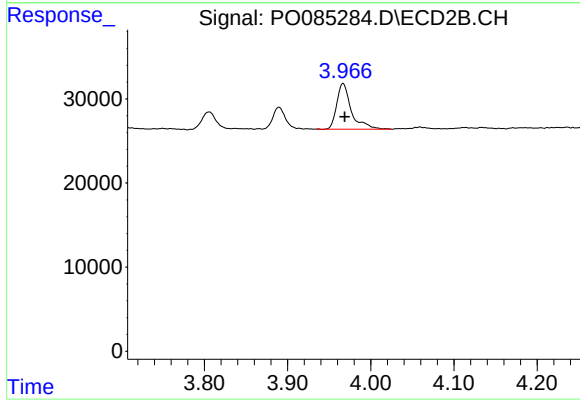

#10 AR-1221-3

R.T.: 3.967 min
Delta R.T.: -0.002 min
Response: 65934
Conc: 50.62 ng/ml