

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031022\
 Data File : P0085289.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2022 21:23
 Operator : YP\AJ
 Sample : N1645-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:23:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 09 04:29:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.496	3.590	3235830	1038013	18.845	22.748
2) SA Decachlor...	10.402	8.609	1840812	1073652	28.111m	28.201
Target Compounds						
41) L9 AR-1268-1	8.823	7.512	436152	317781	46.531	48.442
42) L9 AR-1268-2	8.921	7.576	404110	278189	47.615	47.558
43) L9 AR-1268-3	9.161	7.783	348667	246292	48.620	49.670
44) L9 AR-1268-4	9.607	8.071	145840	101057	47.646	47.620
45) L9 AR-1268-5	10.043	8.358	1109177	681285	46.514	47.468



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031022\
Data File : P0085289.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2022 21:23
Operator : YP\AJ
Sample : N1645-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:23:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0030822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 09 04:29:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

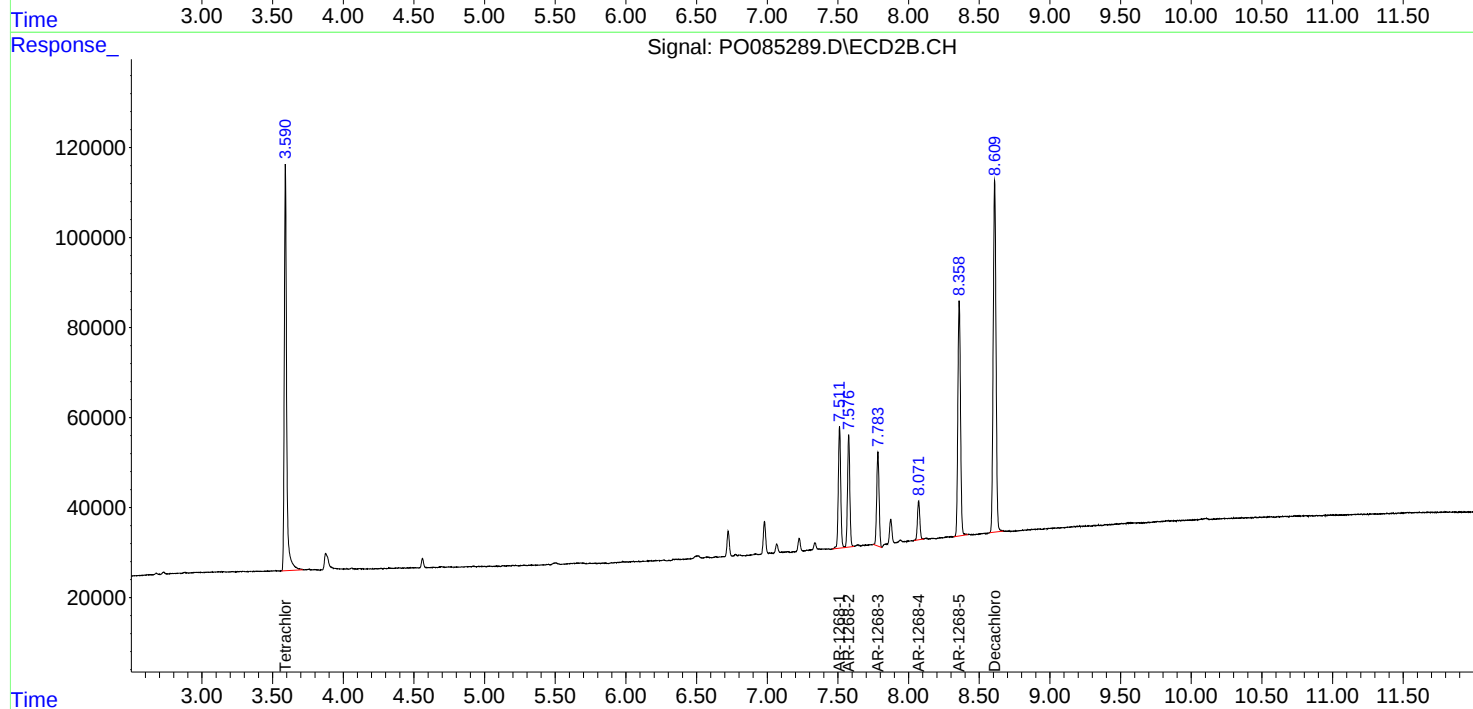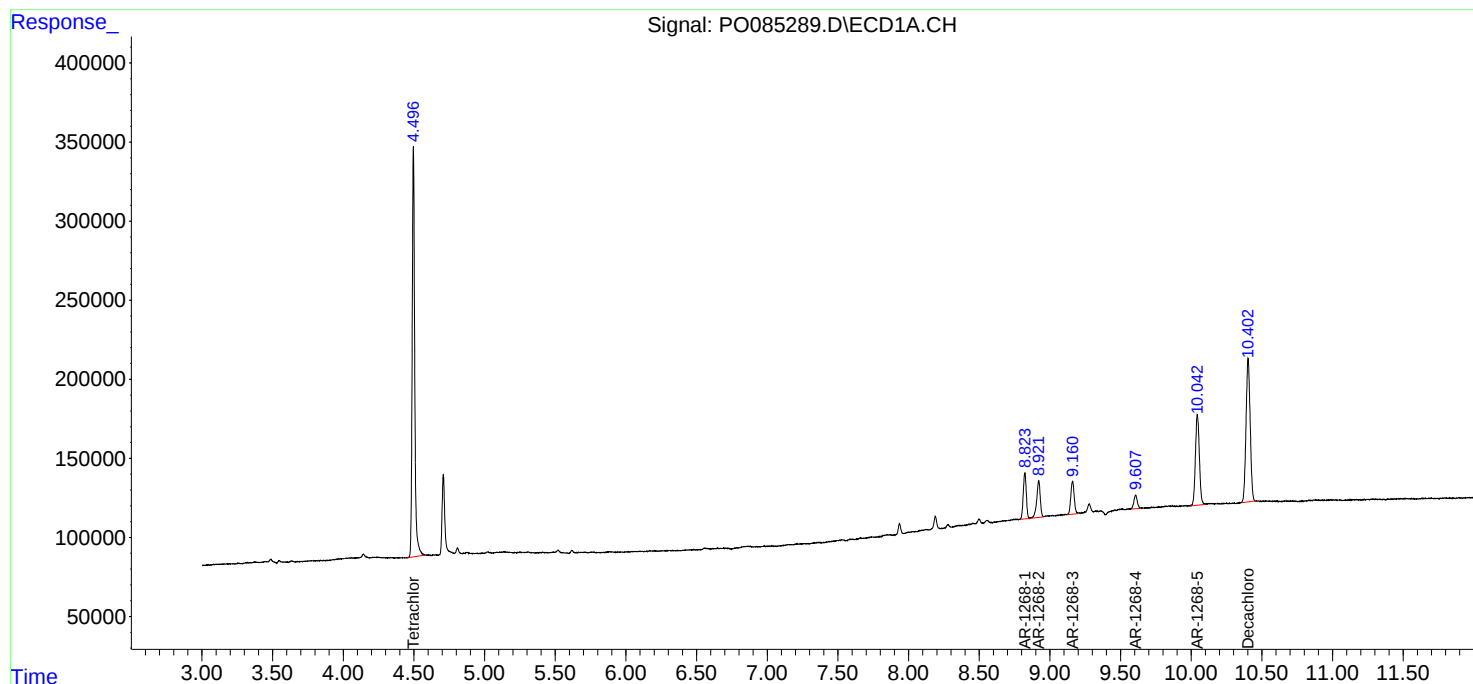


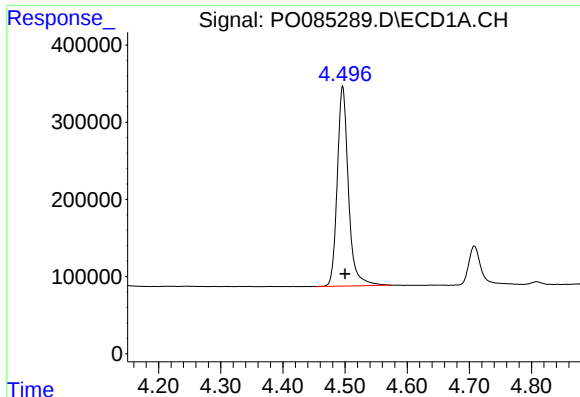

#1 Tetrachloro-m-xylene


R.T.: 4.496 min
Delta R.T.: -0.004 min
Response: 3235830
Conc: 18.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

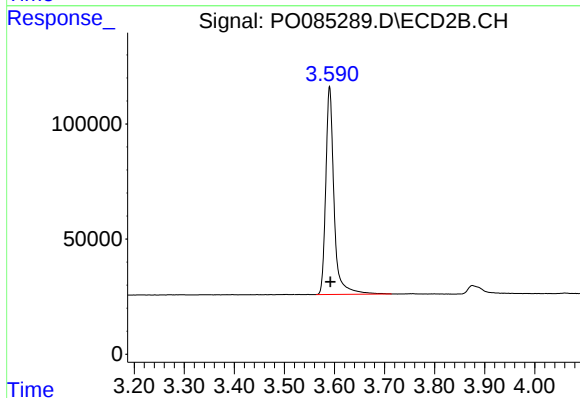


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: -0.002 min
Response: 1038013
Conc: 22.75 ng/ml

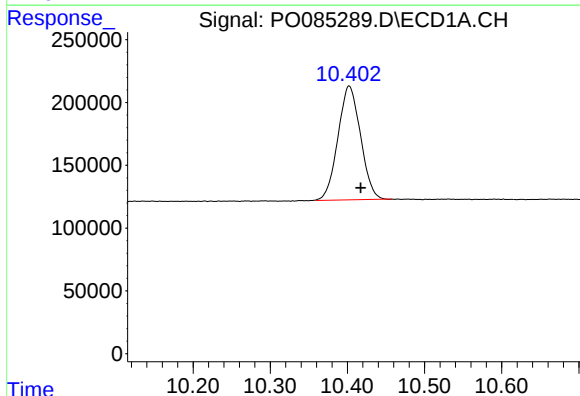


#2 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.016 min
Response: 1840812
Conc: 28.11 ng/ml m

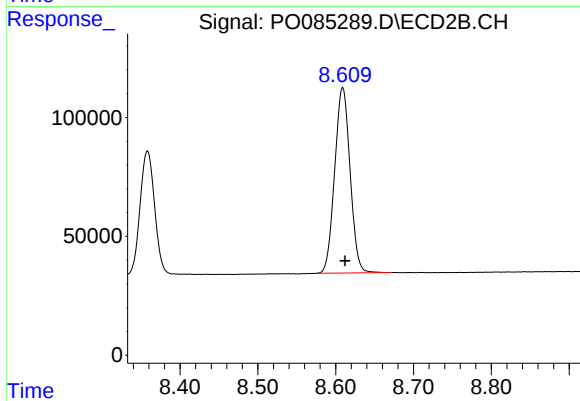

#2 Decachlorobiphenyl


R.T.: 8.609 min
Delta R.T.: -0.003 min
Response: 1073652
Conc: 28.20 ng/ml

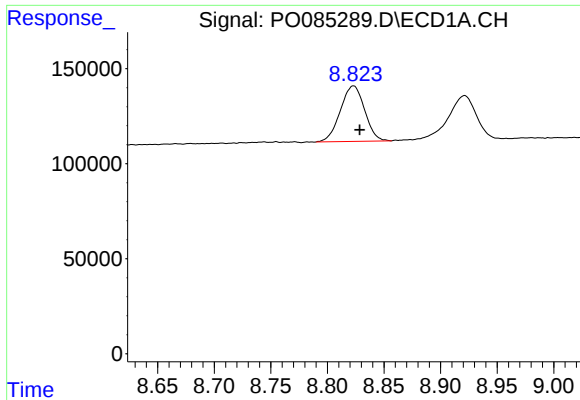

#41 AR-1268-1


R.T.: 8.823 min
Delta R.T.: -0.005 min
Response: 436152
Conc: 46.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

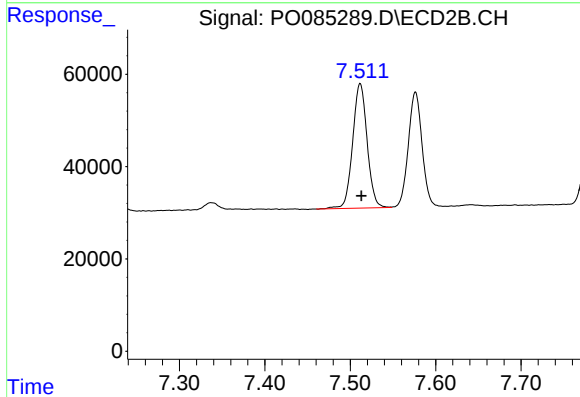


#41 AR-1268-1

R.T.: 7.512 min
Delta R.T.: -0.001 min
Response: 317781
Conc: 48.44 ng/ml

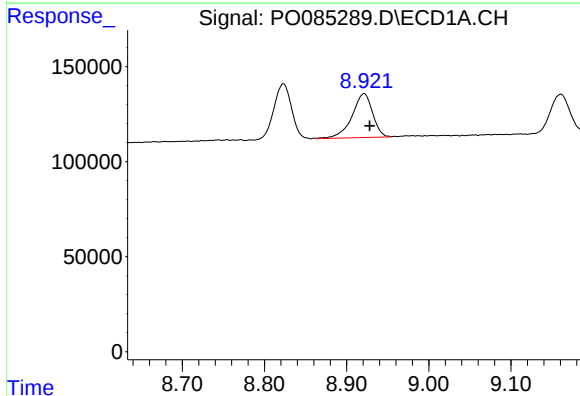


#42 AR-1268-2

R.T.: 8.921 min
Delta R.T.: -0.007 min
Response: 404110
Conc: 47.62 ng/ml

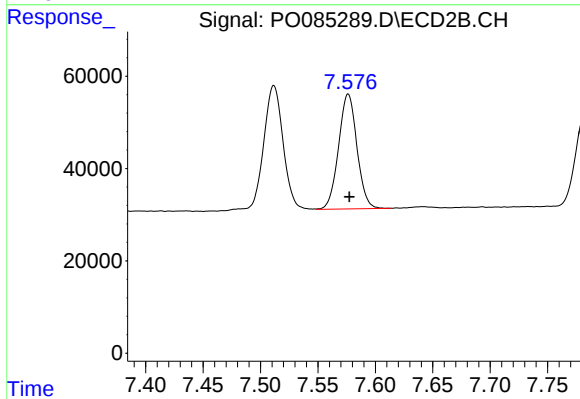

#42 AR-1268-2


R.T.: 7.576 min
Delta R.T.: -0.001 min
Response: 278189
Conc: 47.56 ng/ml

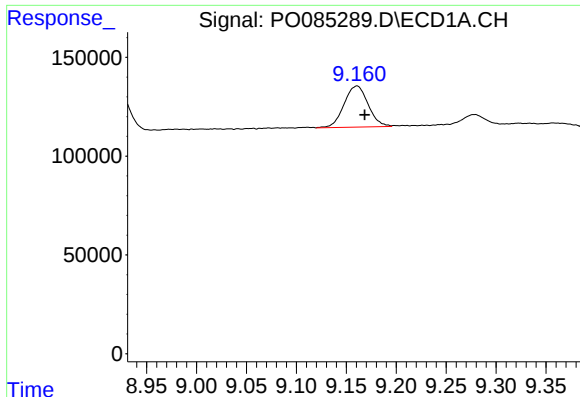

#43 AR-1268-3


R.T.: 9.161 min
Delta R.T.: -0.007 min
Response: 348667
Conc: 48.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

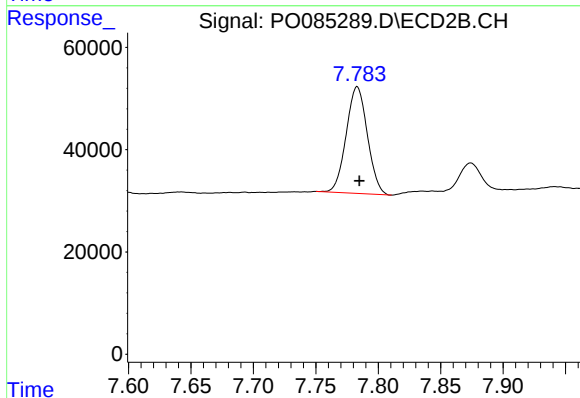


#43 AR-1268-3

R.T.: 7.783 min
Delta R.T.: -0.002 min
Response: 246292
Conc: 49.67 ng/ml

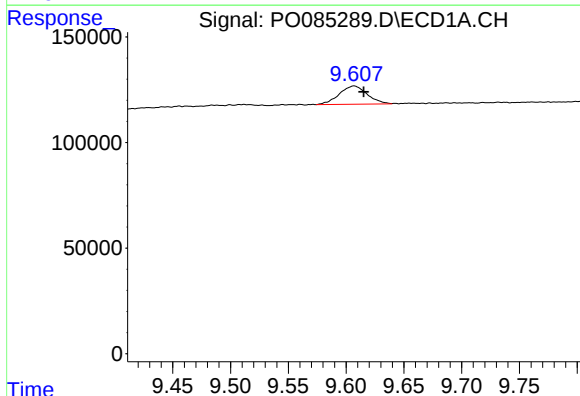


#44 AR-1268-4

R.T.: 9.607 min
Delta R.T.: -0.008 min
Response: 145840
Conc: 47.65 ng/ml

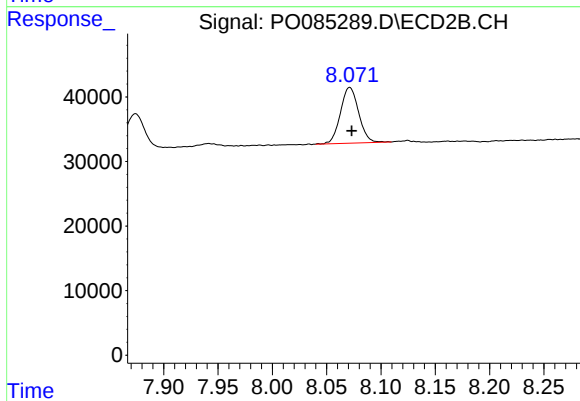

#44 AR-1268-4


R.T.: 8.071 min
Delta R.T.: -0.002 min
Response: 101057
Conc: 47.62 ng/ml

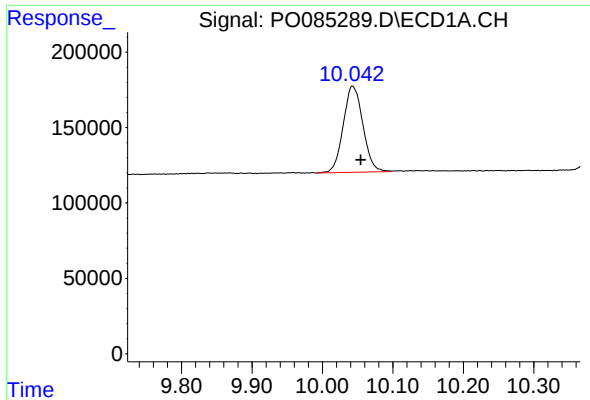

#45 AR-1268-5

R.T.: 10.043 min
Delta R.T.: -0.012 min
Response: 1109177
Conc: 46.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

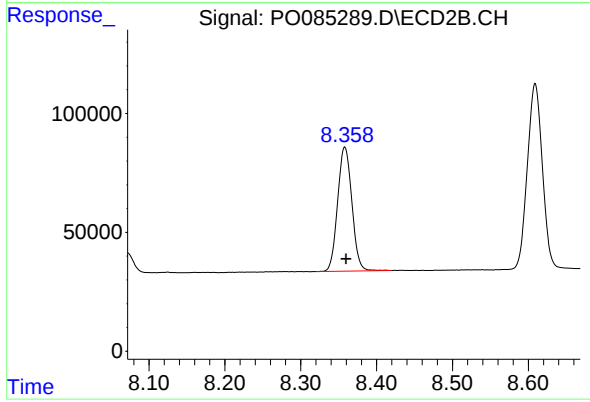

#45 AR-1268-5

R.T.: 8.358 min
Delta R.T.: -0.002 min
Response: 681285
Conc: 47.47 ng/ml