

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 12:55
 Operator : YP/AJ
 Sample : Q1527-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 022825-SEALPOT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 14:15:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	119.1E6	74677980	12.578	14.267
2) SA Decachlor...	8.752	8.702	130.8E6	57635690	15.206	18.100

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 12:55
Operator : YP/AJ
Sample : Q1527-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
022825-SEALPOT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 14:15:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

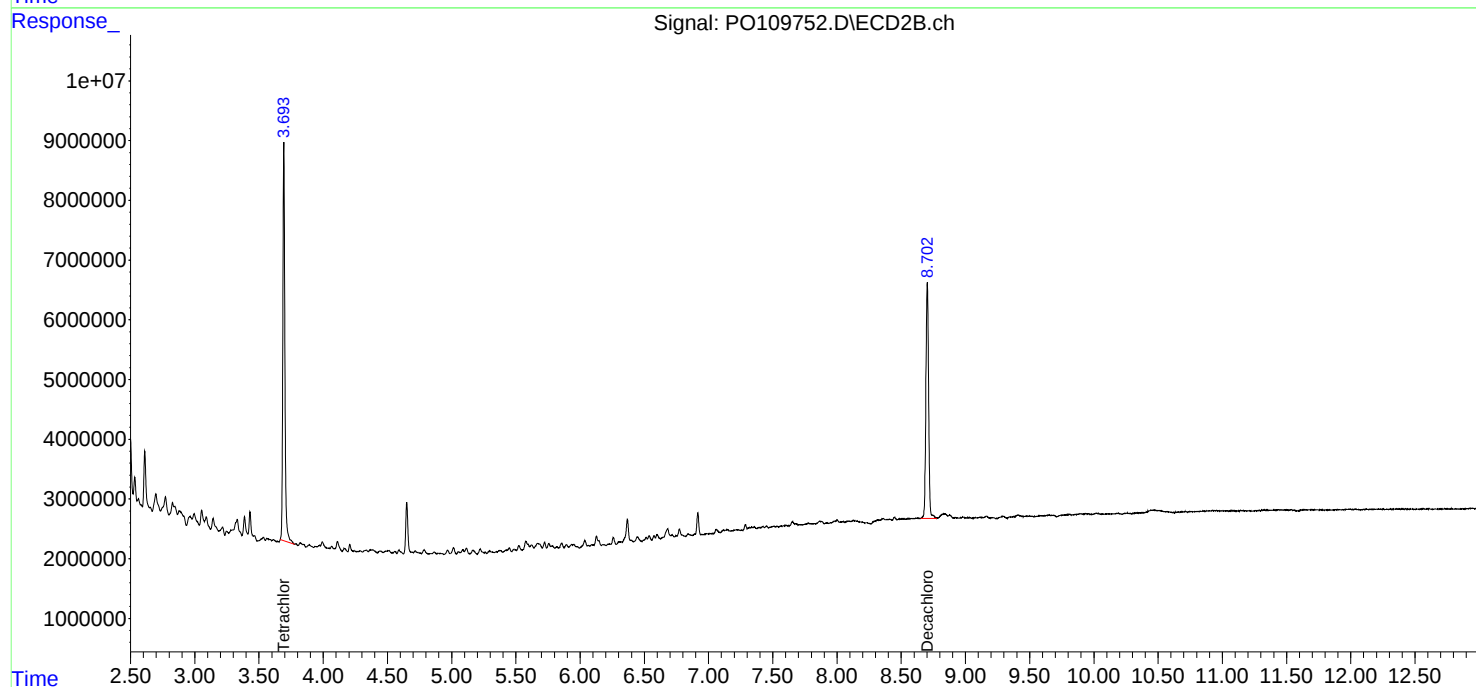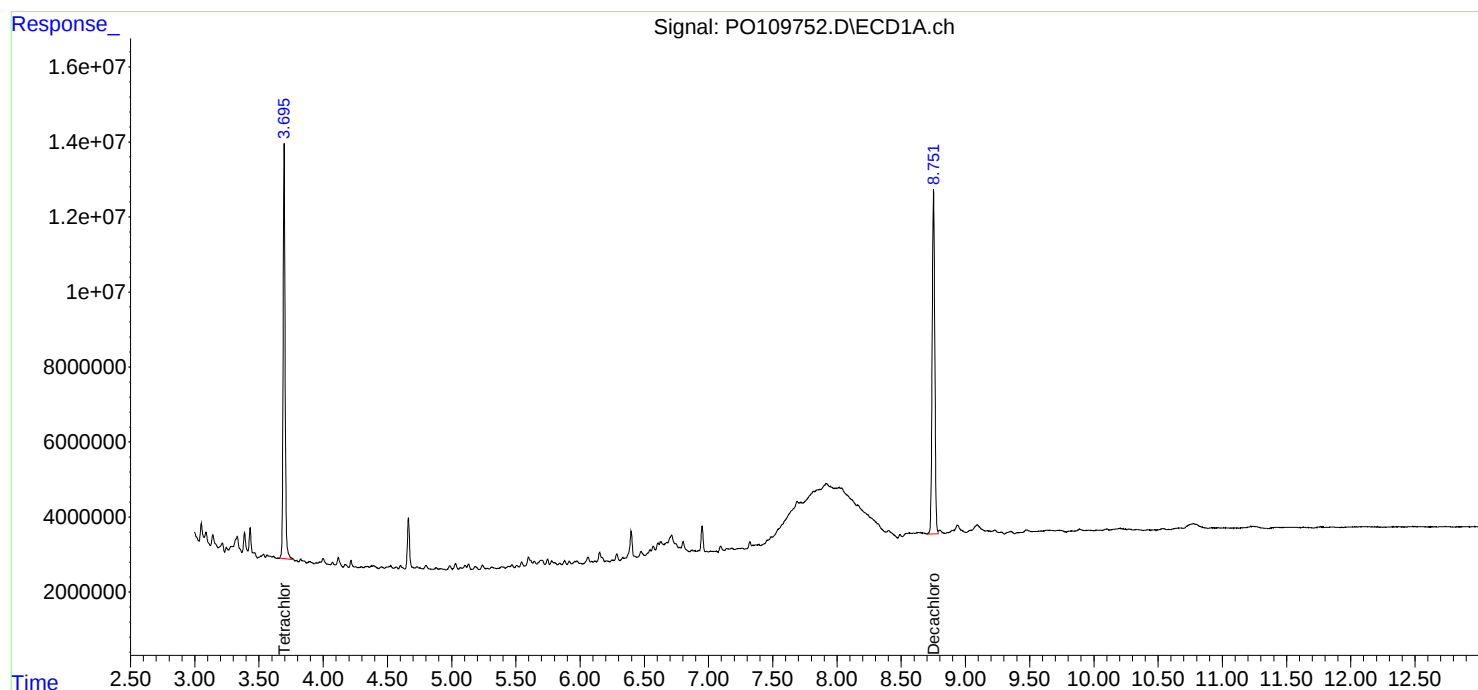


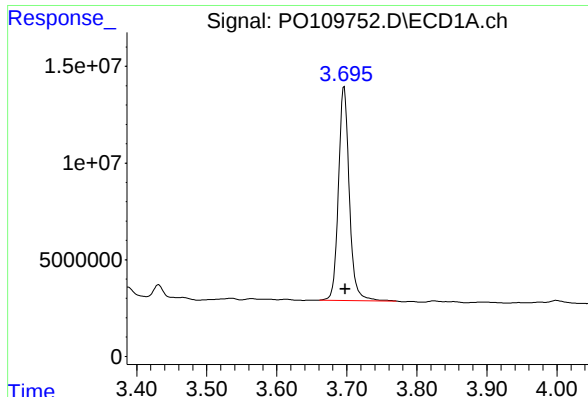

#1 Tetrachloro-m-xylene


R.T.: 3.696 min
Delta R.T.: -0.002 min
Response: 119055578
Conc: 12.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
022825-SEALPOT

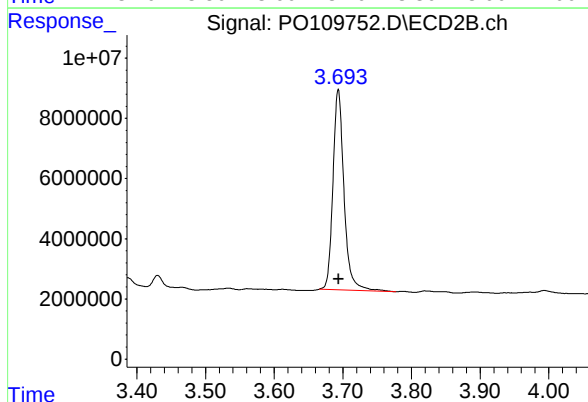


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.000 min
Response: 74677980
Conc: 14.27 ng/ml

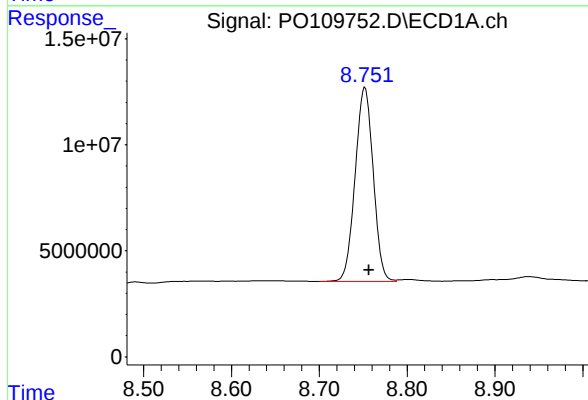

#2 Decachlorobiphenyl

R.T.: 8.752 min
Delta R.T.: -0.005 min
Response: 130803088
Conc: 15.21 ng/ml

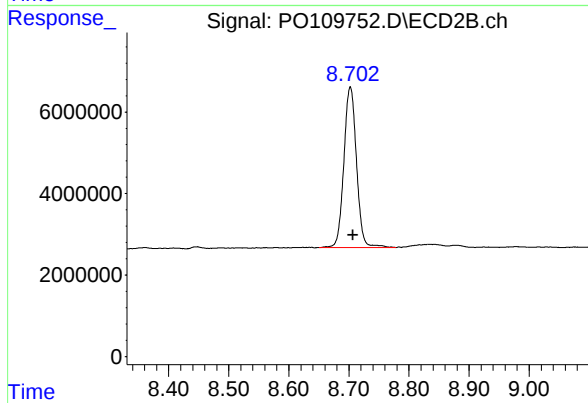

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.004 min
Response: 57635690
Conc: 18.10 ng/ml