

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 18:16
 Operator : YP/AJ
 Sample : Q1529-06 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 60299

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/11/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 01:00:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.693	26276373	15643315	2.776	2.989
2) SA Decachlor...	8.750	8.698	11924428	5564950	1.386m	1.748m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 18:16
Operator : YP/AJ
Sample : Q1529-06 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
60299


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/11/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 01:00:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

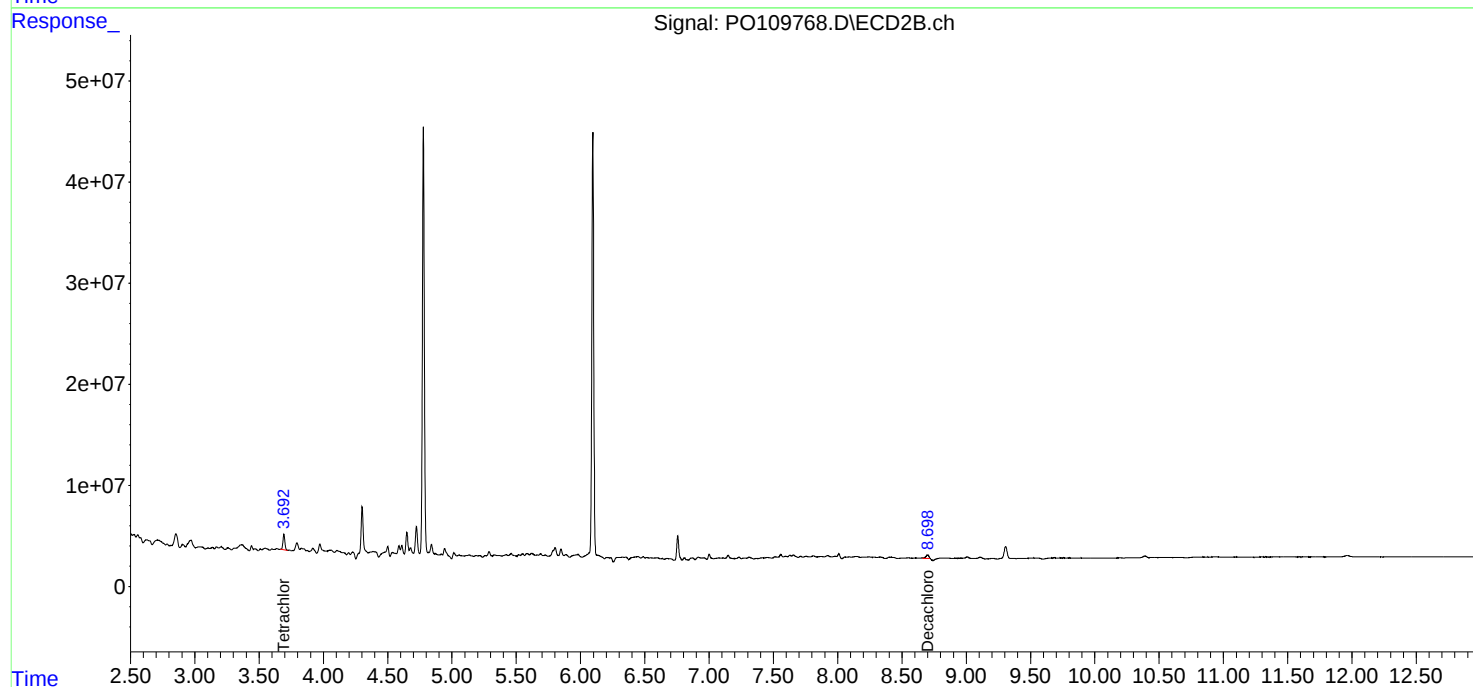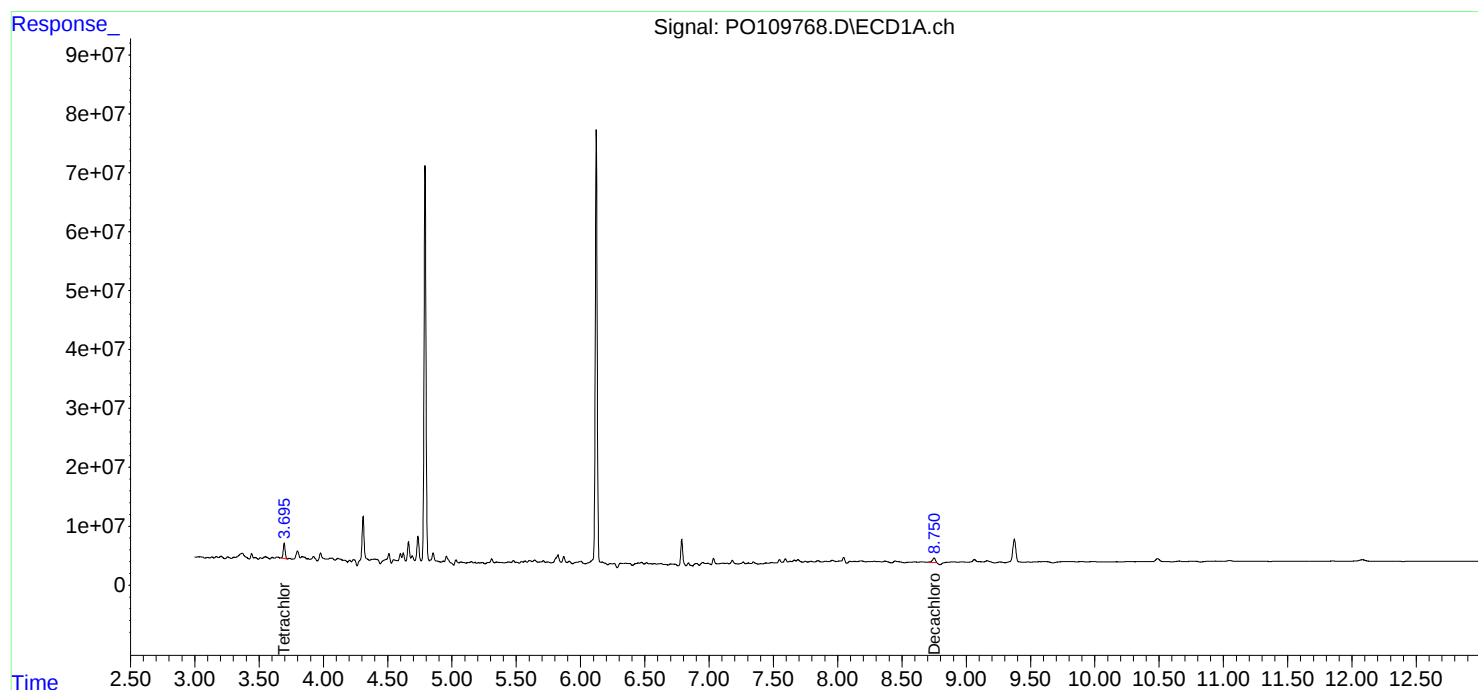

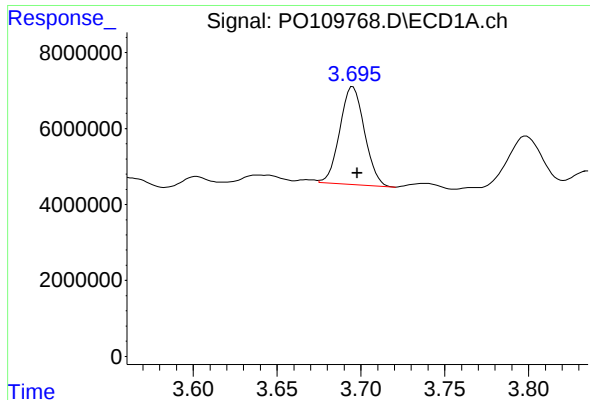


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: -0.003 min
Response: 26276373
Conc: 2.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
60299


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/11/2025
Supervised By :Ankita Jodhani 03/12/2025

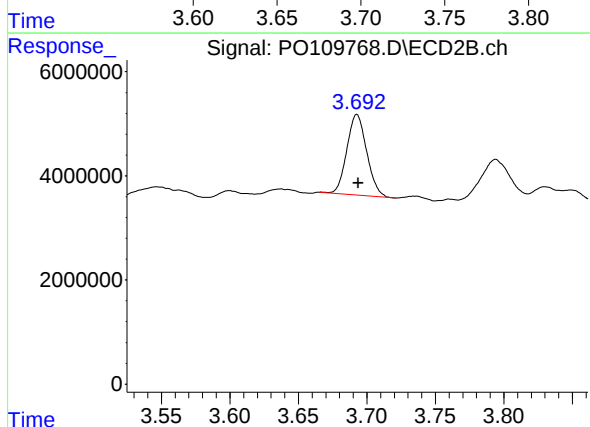


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: -0.001 min
Response: 15643315
Conc: 2.99 ng/ml

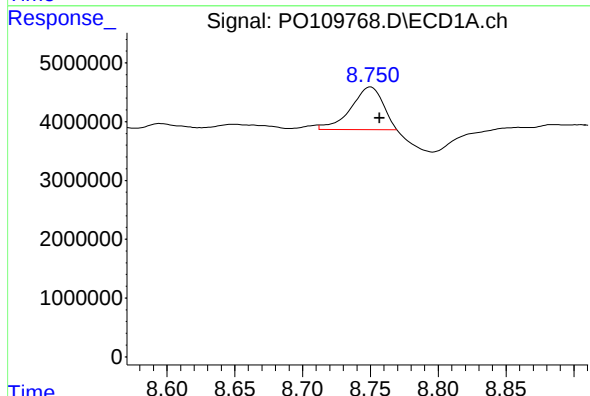

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: -0.007 min
Response: 11924428
Conc: 1.39 ng/ml m

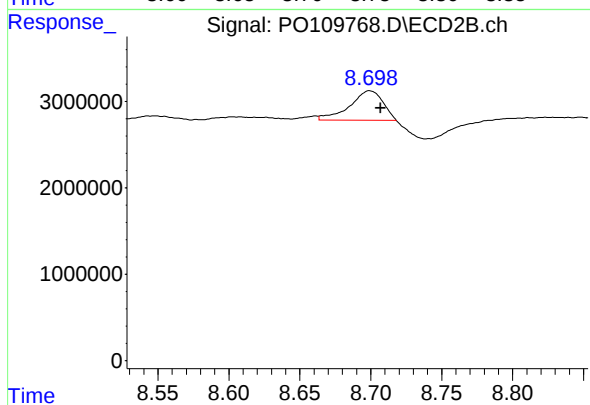

#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.008 min
Response: 5564950
Conc: 1.75 ng/ml m