

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031121\
 Data File : P0076060.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2021 15:18
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1268 LOD 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 16:25:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.939	1002780	795331	16.823	17.829
2) SA Decachlor...	10.931	9.210	725856	782737	22.095	21.527
Target Compounds						
41) L9 AR-1268-1	9.435	8.136	97510	126171	18.551	19.607
42) L9 AR-1268-2	9.532	8.200	85152	116168	18.222	19.615
43) L9 AR-1268-3	9.755	8.408	82276	97297	19.746	19.019
44) L9 AR-1268-4	10.190	8.696	30103	34509	19.203	17.508
45) L9 AR-1268-5	10.599	8.972	247709	285877	19.604	20.094



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031121\
Data File : P0076060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2021 15:18
Operator : DD\AJ
Sample : M1458-07
Misc : AR1268 LOD 25 PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 16:25:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

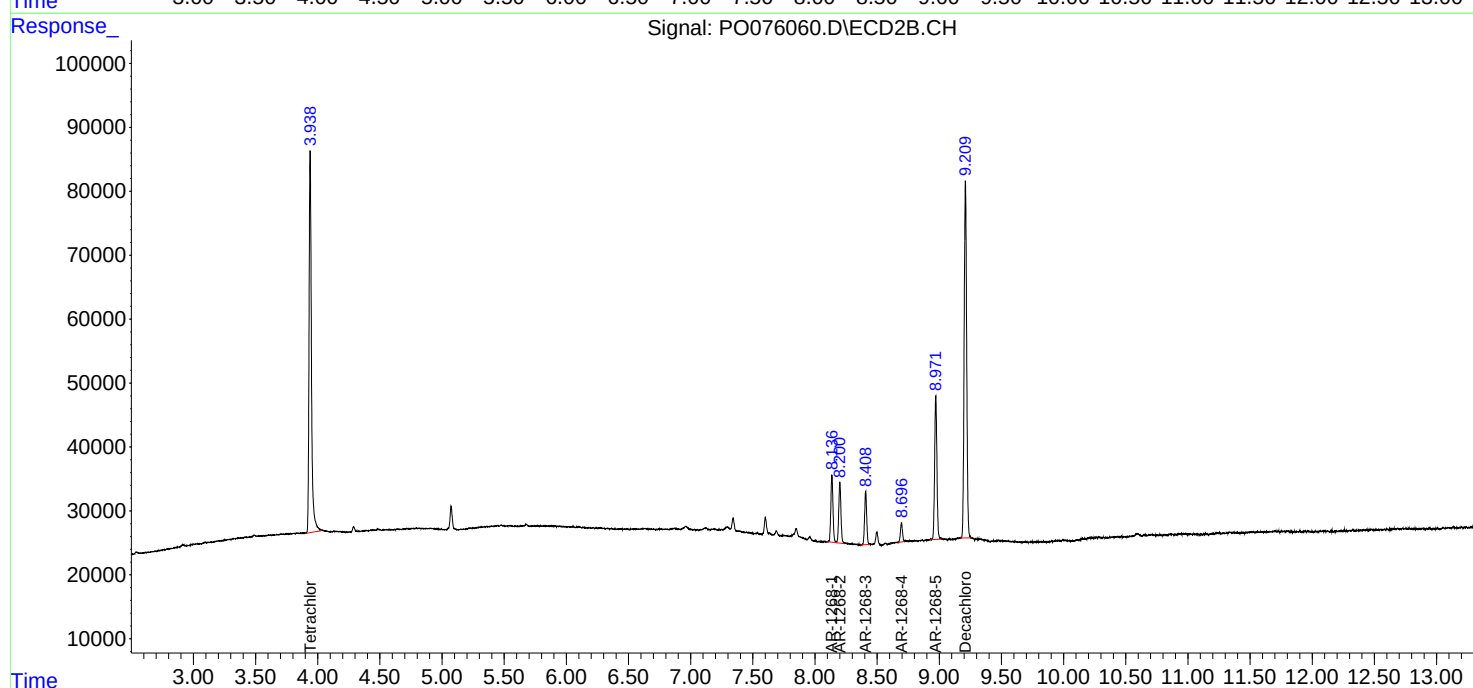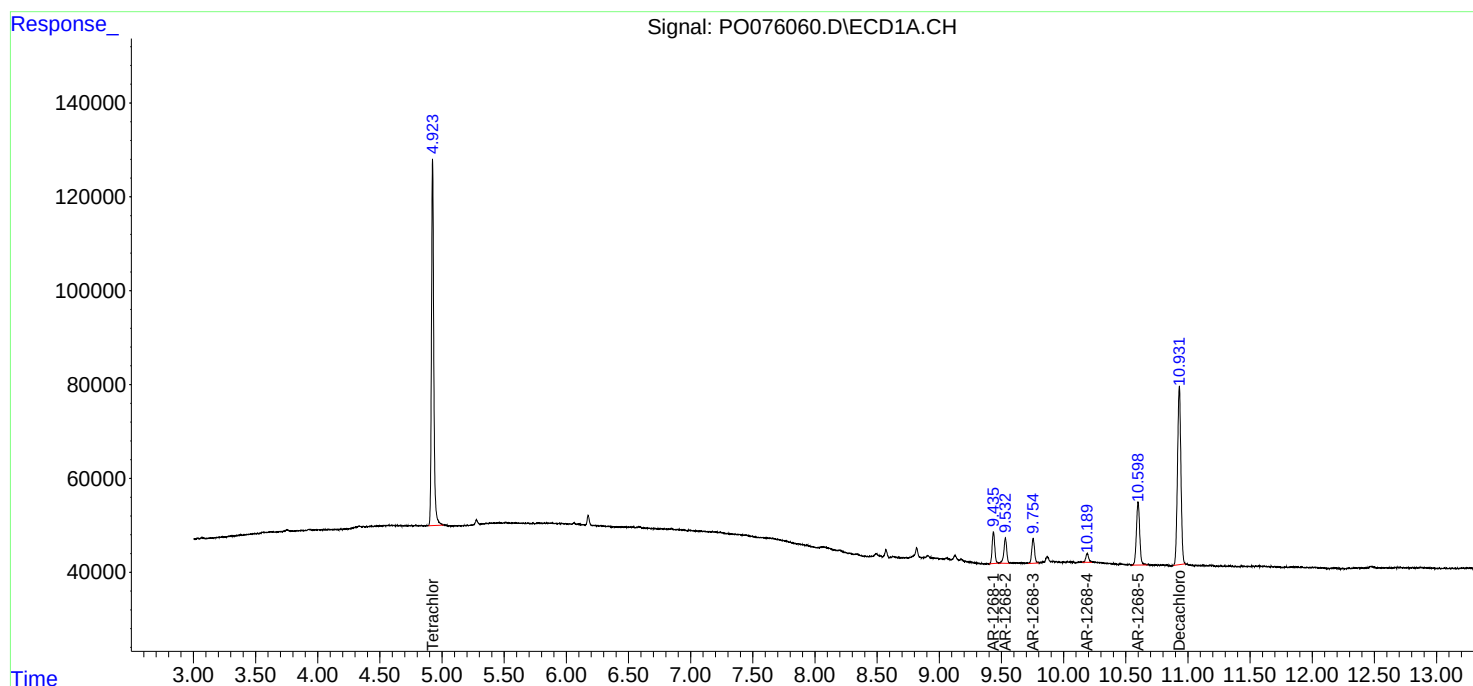


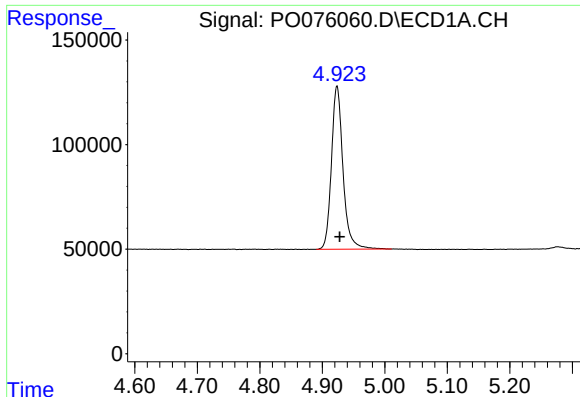

#1 Tetrachloro-m-xylene


R.T.: 4.924 min
Delta R.T.: -0.004 min
Response: 1002780
Conc: 16.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

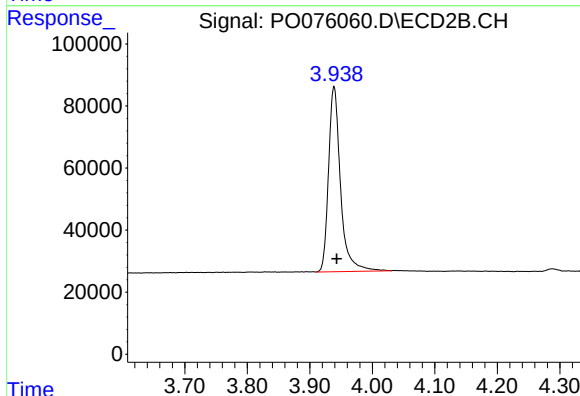


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: -0.004 min
Response: 795331
Conc: 17.83 ng/ml

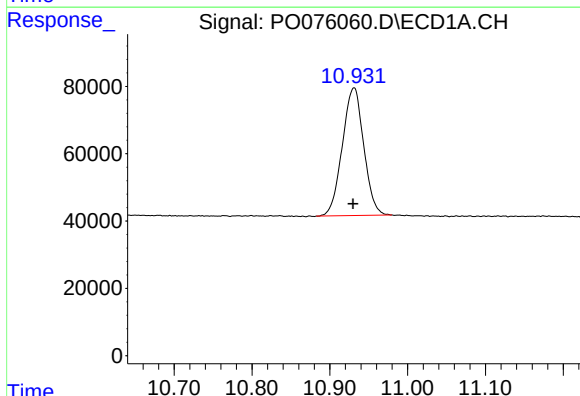


#2 Decachlorobiphenyl

R.T.: 10.931 min
Delta R.T.: 0.001 min
Response: 725856
Conc: 22.10 ng/ml

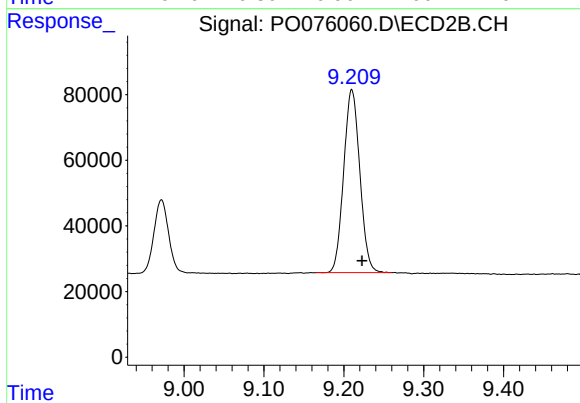

#2 Decachlorobiphenyl


R.T.: 9.210 min
Delta R.T.: -0.013 min
Response: 782737
Conc: 21.53 ng/ml

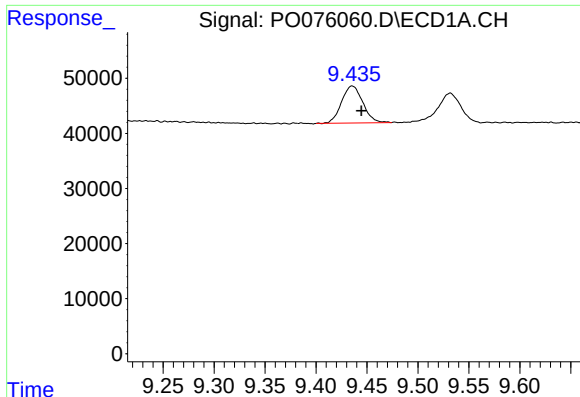

#41 AR-1268-1


R.T.: 9.435 min
Delta R.T.: -0.009 min
Response: 97510
Conc: 18.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

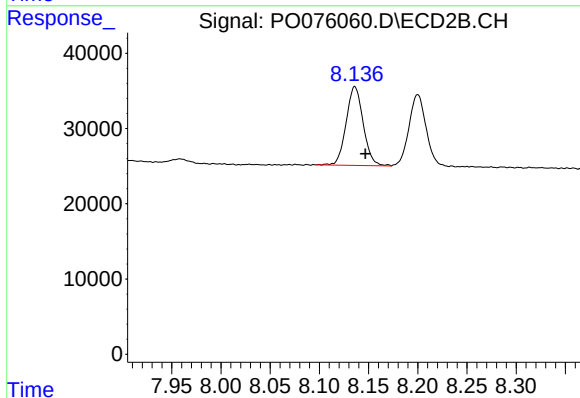


#41 AR-1268-1

R.T.: 8.136 min
Delta R.T.: -0.011 min
Response: 126171
Conc: 19.61 ng/ml

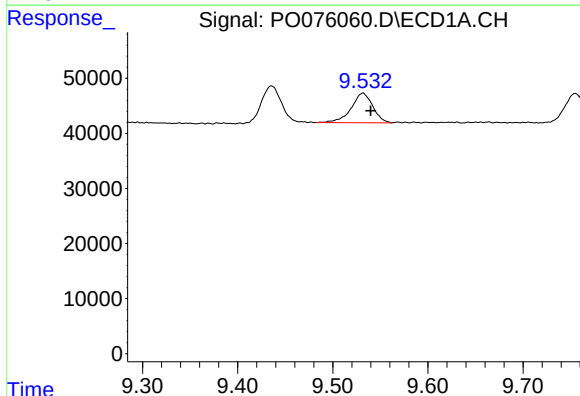


#42 AR-1268-2

R.T.: 9.532 min
Delta R.T.: -0.008 min
Response: 85152
Conc: 18.22 ng/ml

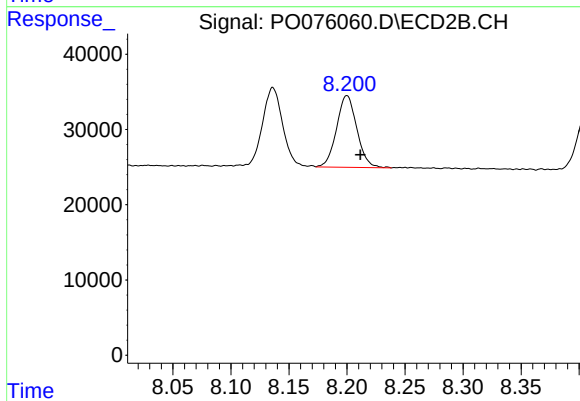

#42 AR-1268-2


R.T.: 8.200 min
Delta R.T.: -0.011 min
Response: 116168
Conc: 19.61 ng/ml

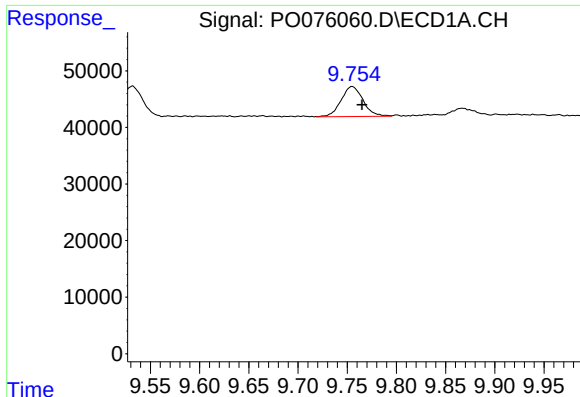

#43 AR-1268-3


R.T.: 9.755 min
Delta R.T.: -0.010 min
Response: 82276
Conc: 19.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

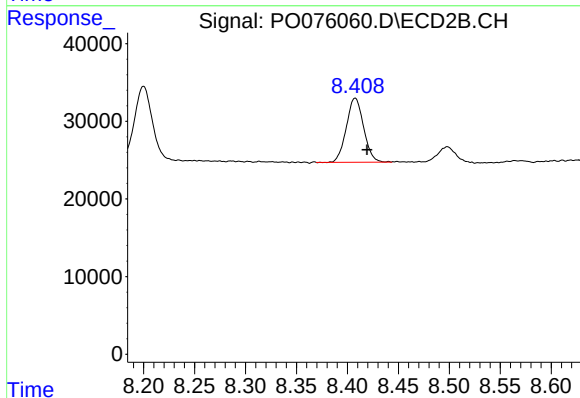


#43 AR-1268-3

R.T.: 8.408 min
Delta R.T.: -0.012 min
Response: 97297
Conc: 19.02 ng/ml

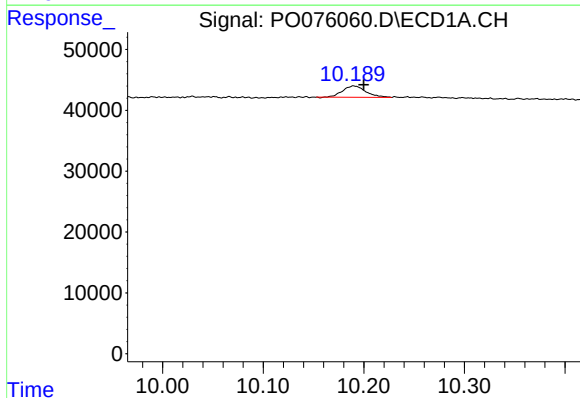


#44 AR-1268-4

R.T.: 10.190 min
Delta R.T.: -0.010 min
Response: 30103
Conc: 19.20 ng/ml

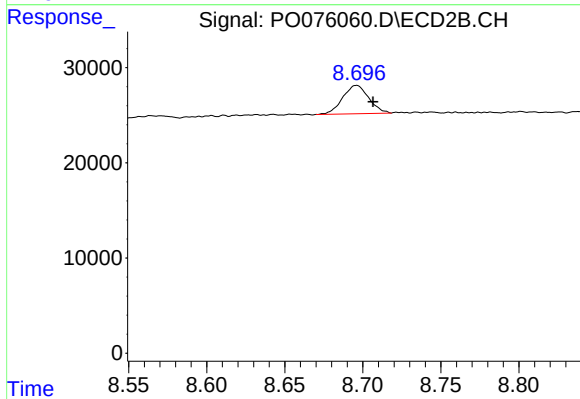

#44 AR-1268-4


R.T.: 8.696 min
Delta R.T.: -0.011 min
Response: 34509
Conc: 17.51 ng/ml

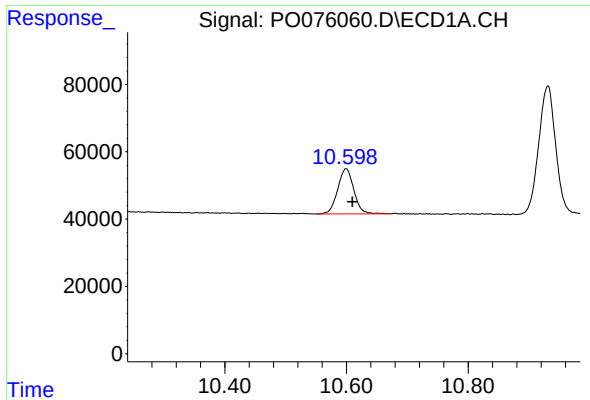

#45 AR-1268-5

R.T.: 10.599 min
Delta R.T.: -0.011 min
Response: 247709
Conc: 19.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

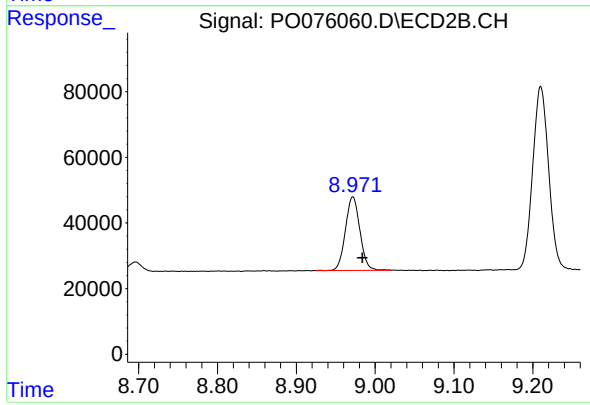

#45 AR-1268-5

R.T.: 8.972 min
Delta R.T.: -0.012 min
Response: 285877
Conc: 20.09 ng/ml