

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031125\
 Data File : P0109786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 15:22
 Operator : YP/AJ
 Sample : Q1534-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-363-COMP-18

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 15:32:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.693	178.1E6	100.7E6	18.815	19.245
2) SA Decachlor...	8.751	8.702	87398755	35566124	10.160	11.169m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031125\
Data File : PO109786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 15:22
Operator : YP/AJ
Sample : Q1534-13
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-363-COMP-18


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 15:32:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

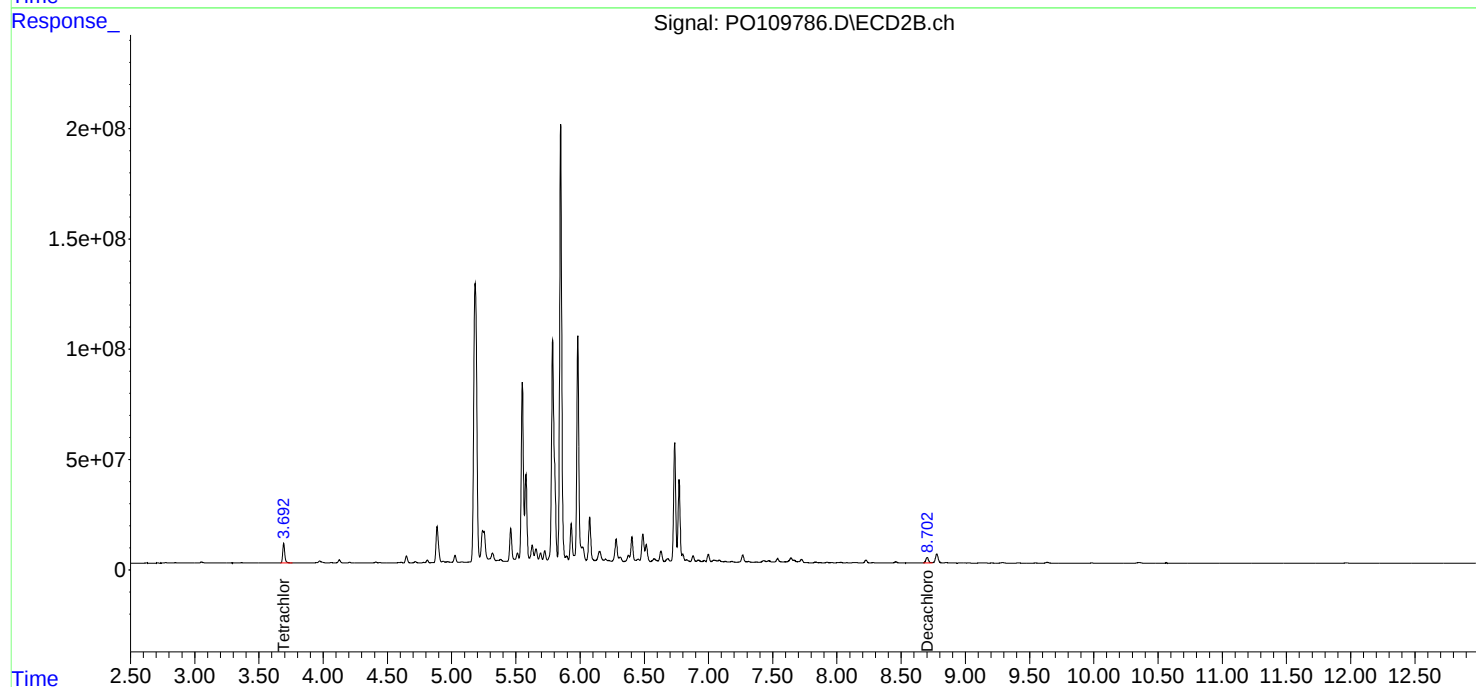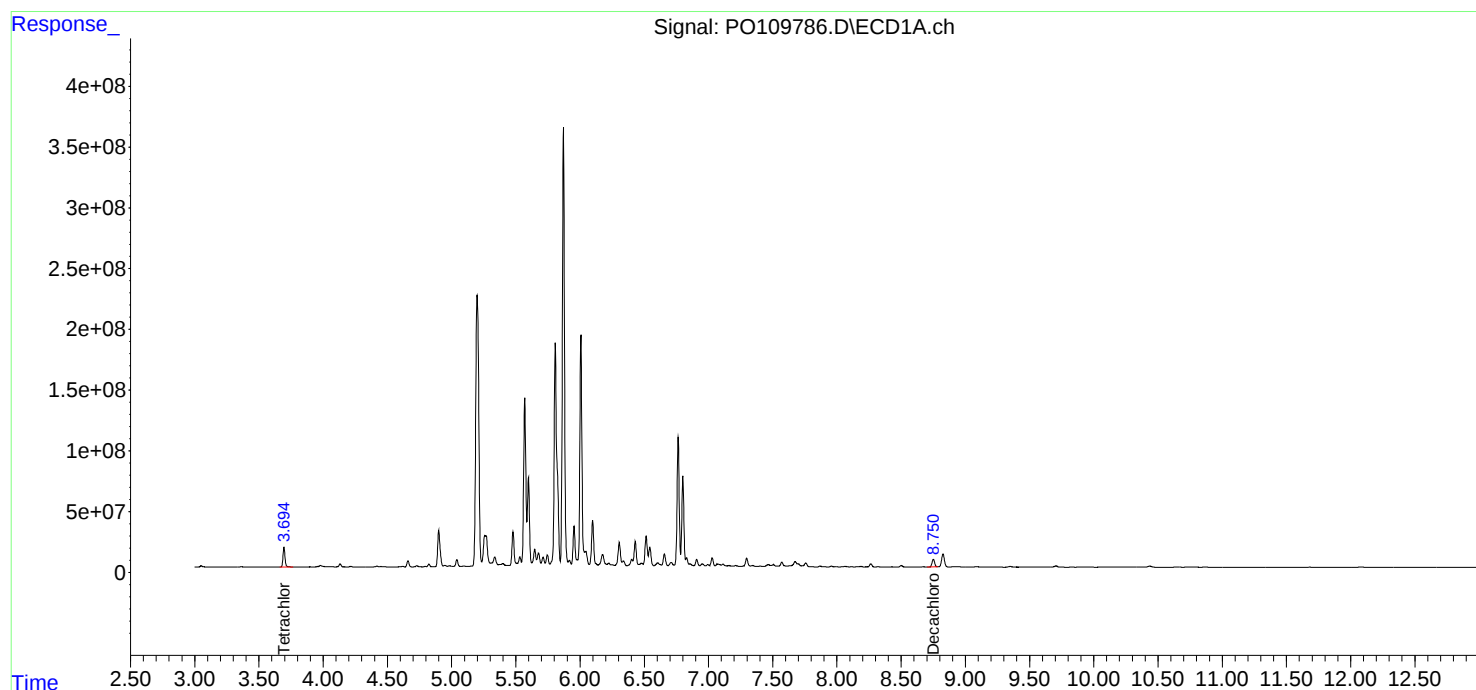

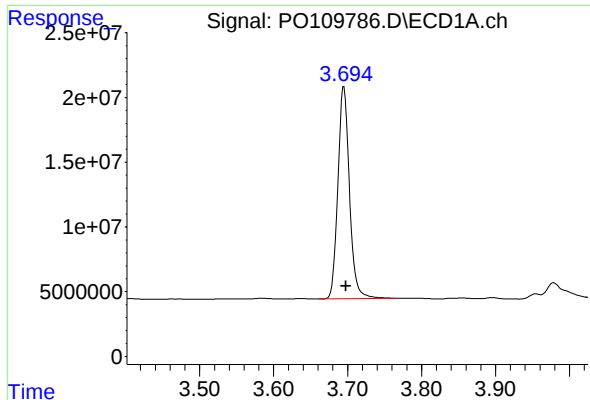


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: -0.003 min
Response: 178084695
Conc: 18.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-363-COMP-18


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

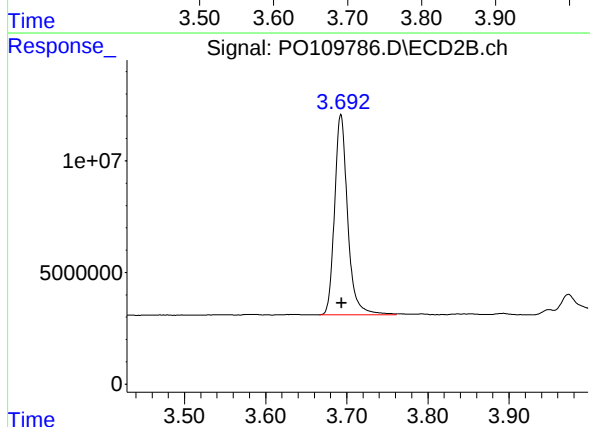


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: -0.001 min
Response: 100734785
Conc: 19.25 ng/ml

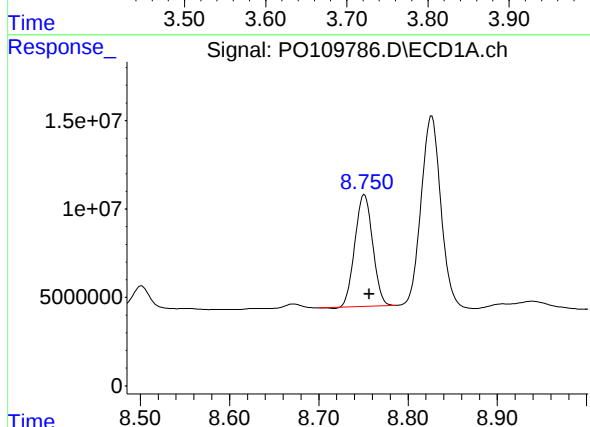

#2 Decachlorobiphenyl

R.T.: 8.751 min
Delta R.T.: -0.006 min
Response: 87398755
Conc: 10.16 ng/ml

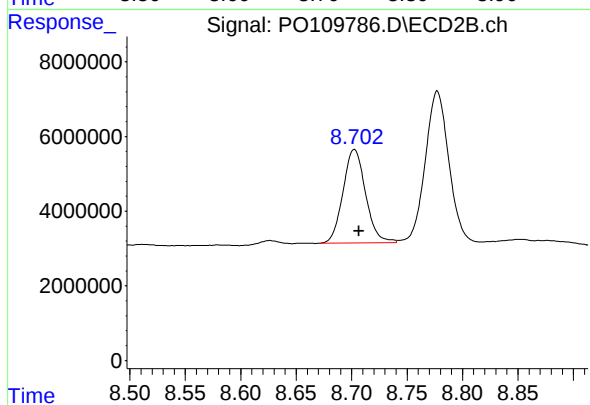

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.005 min
Response: 35566124
Conc: 11.17 ng/ml m