

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031125\
 Data File : P0109787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 15:40
 Operator : YP/AJ
 Sample : Q1534-19
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-363-COMP-19

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 15:51:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.693	194.4E6	109.6E6	20.536	20.944
2) SA Decachlor...	8.750	8.702	117.0E6	44771939	13.597m	14.060m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031125\
Data File : PO109787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 15:40
Operator : YP/AJ
Sample : Q1534-19
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-363-COMP-19


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 15:51:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

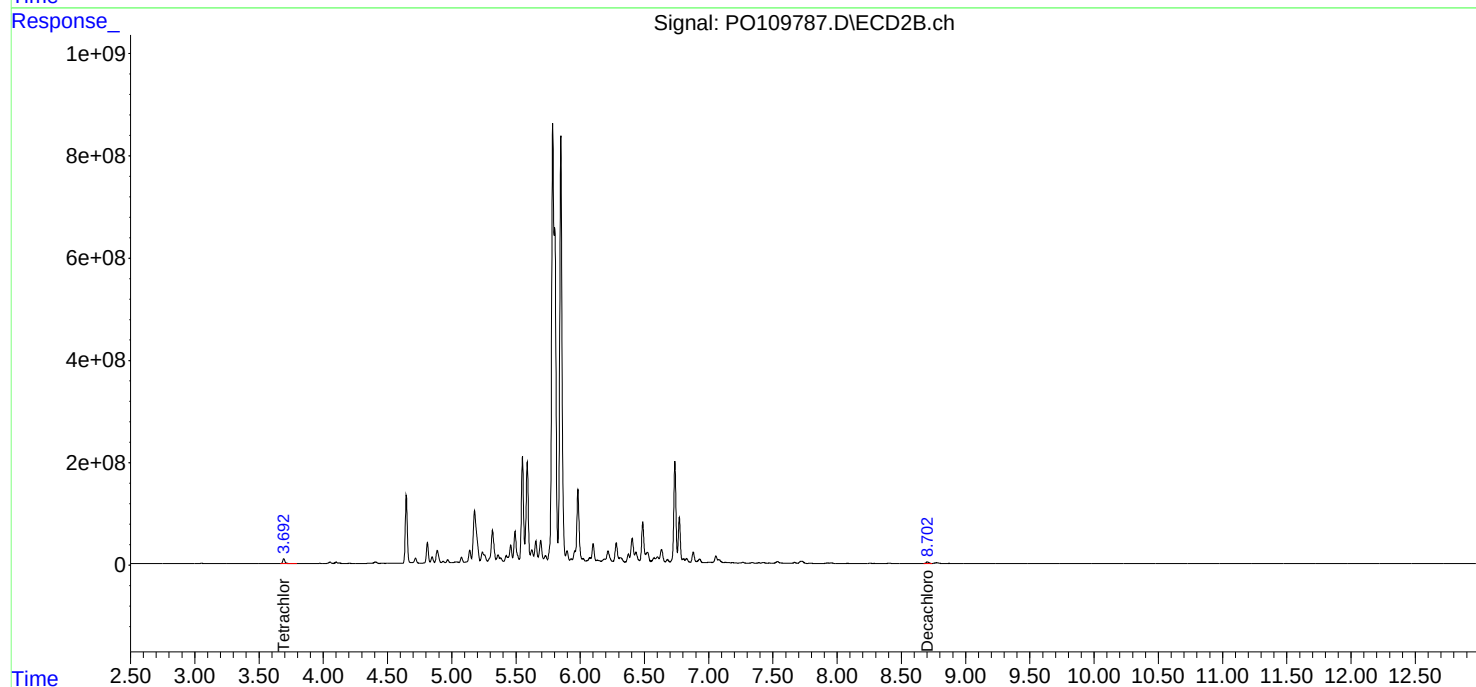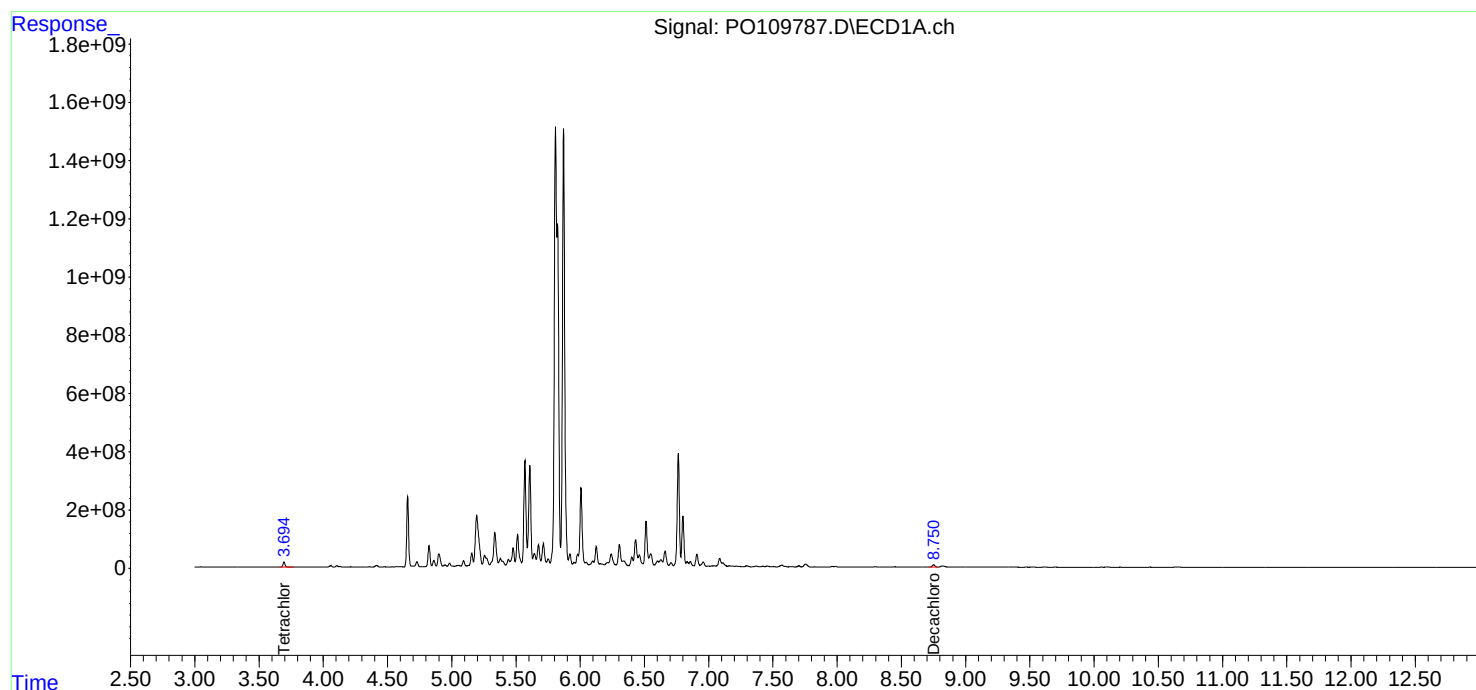

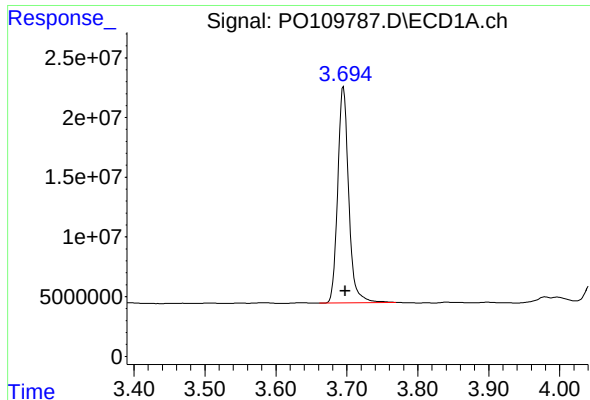


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: -0.003 min
Response: 194379836
Conc: 20.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-363-COMP-19


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

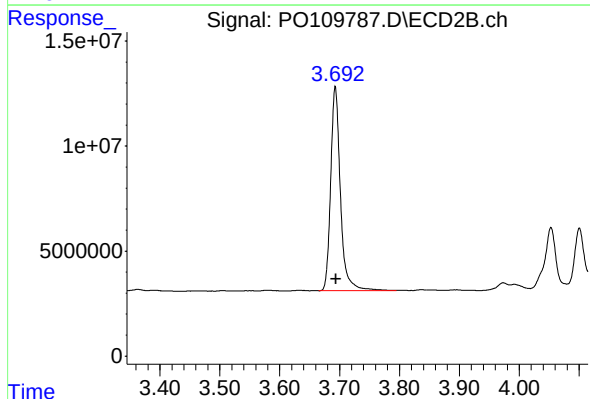


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: -0.001 min
Response: 109626142
Conc: 20.94 ng/ml

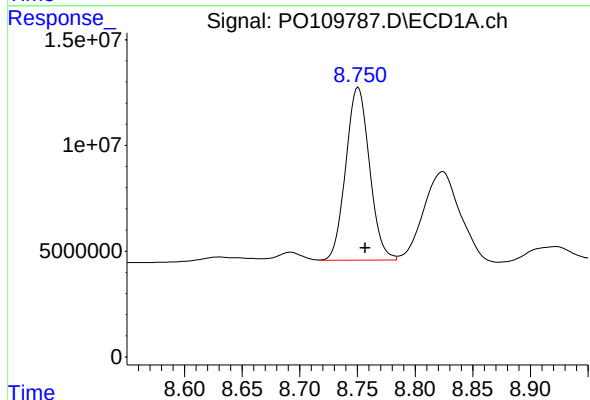

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: -0.007 min
Response: 116956569
Conc: 13.60 ng/ml m

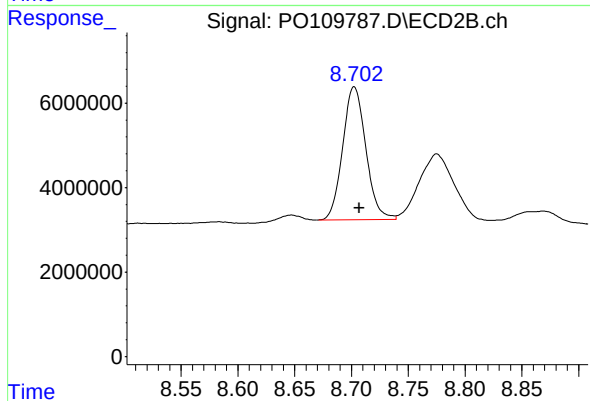

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.005 min
Response: 44771939
Conc: 14.06 ng/ml m