

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
 Data File : P0067169.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2020 9:48
 Operator : DD\AJ
 Sample : L1871-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-17-SA

Manual Integrations
 APPROVED

Sohil
 3/13/2020 8:31:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 11:25:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.111	3.397	664708	800888	21.265m	20.467
2) SA Decachlor...	9.570	8.271	501759	726728	13.813m	14.925m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
Data File : P0067169.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2020 9:48
Operator : DD\AJ
Sample : L1871-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-17-SA


Manual Integrations
APPROVED

Sohil
3/13/2020 8:31:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 11:25:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

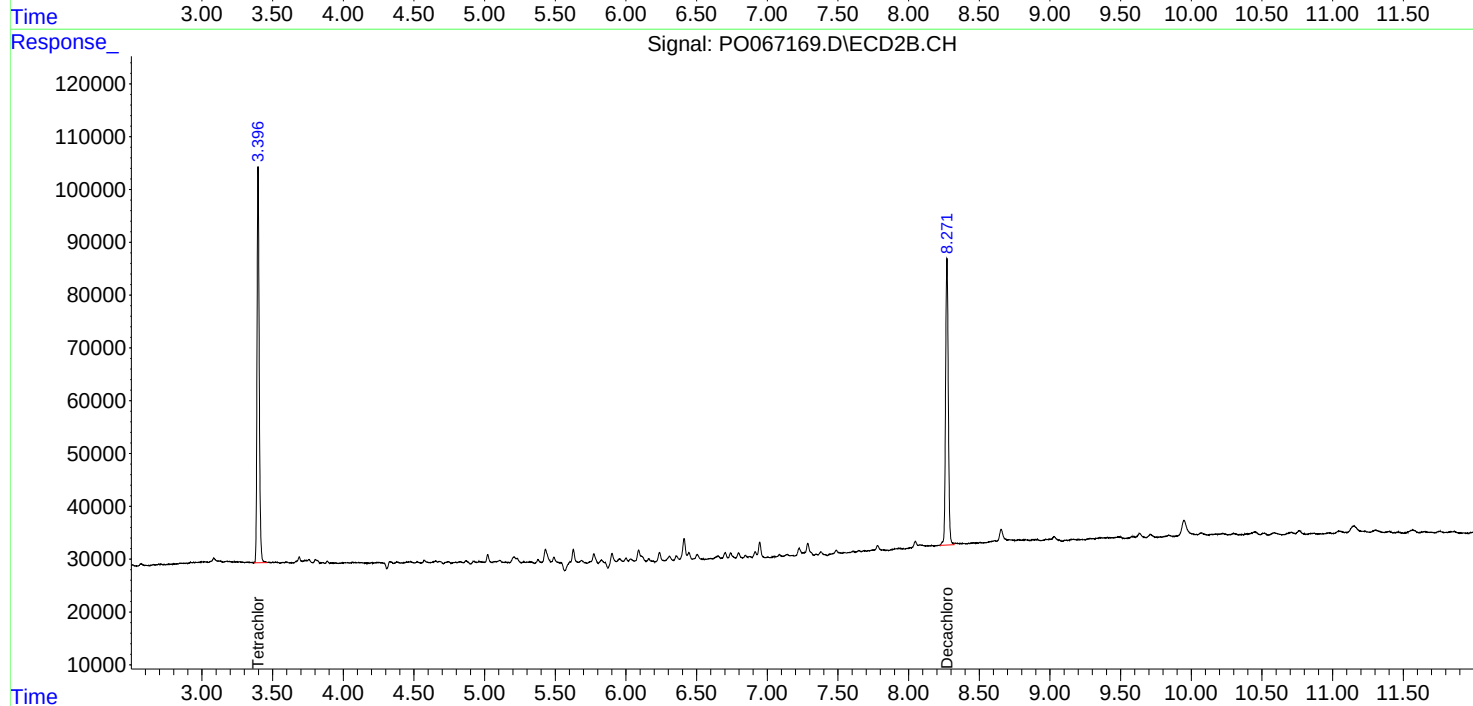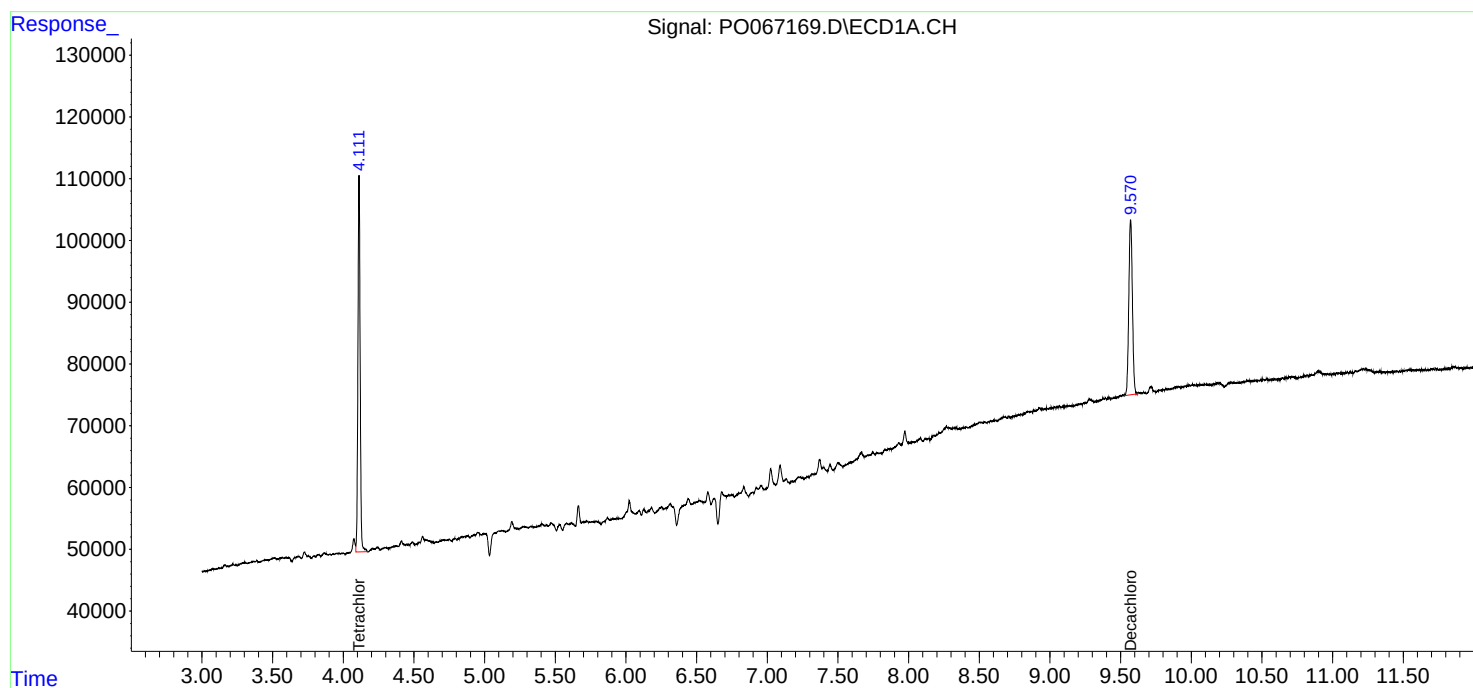

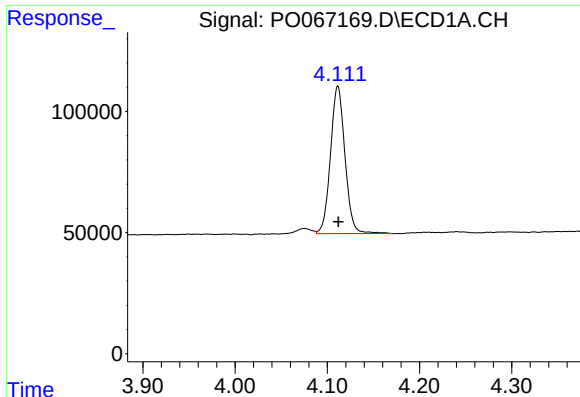


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: 0.000 min
Response: 664708
Conc: 21.26 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-17-SA


Manual Integrations
APPROVED

Sohil
3/13/2020 8:31:55 AM

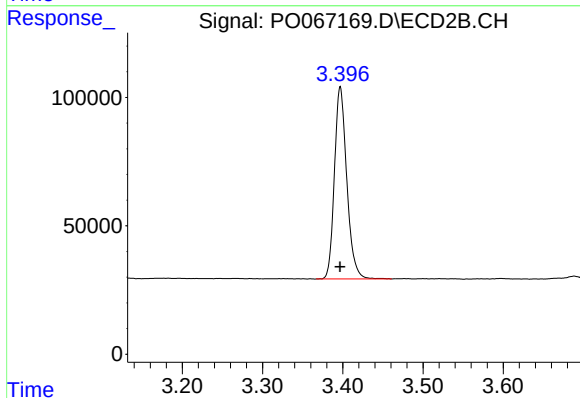


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 800888
Conc: 20.47 ng/ml

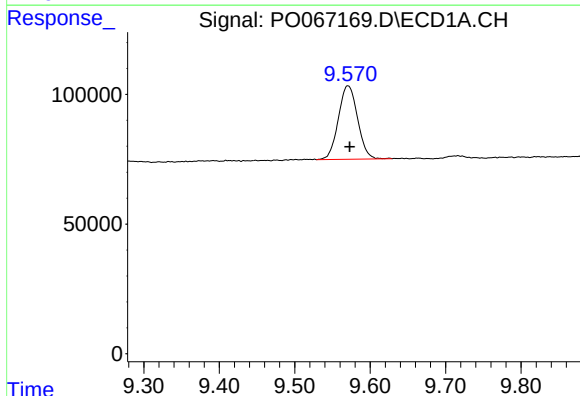

#2 Decachlorobiphenyl

R.T.: 9.570 min
Delta R.T.: -0.003 min
Response: 501759
Conc: 13.81 ng/ml m

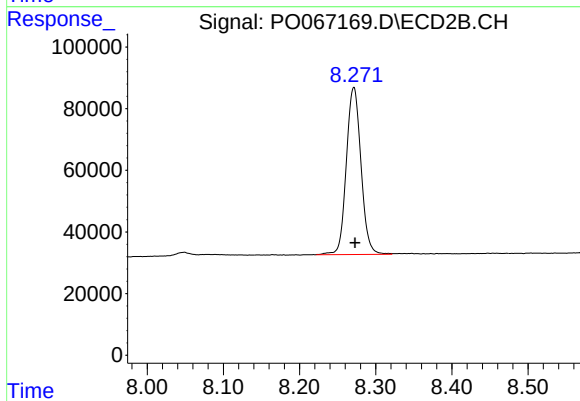

#2 Decachlorobiphenyl

R.T.: 8.271 min
Delta R.T.: -0.002 min
Response: 726728
Conc: 14.93 ng/ml m