

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
 Data File : P0067173.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2020 10:56
 Operator : DD\AJ
 Sample : L1868-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S4-01-A

Manual Integrations
 APPROVED

Sohil
 3/13/2020 8:31:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 11:27:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.111	3.396	1024892	1153067	32.787m	29.467m
2) SA Decachlor...	9.569	8.271	905834	1235980	24.938	25.384m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
Data File : P0067173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2020 10:56
Operator : DD\AJ
Sample : L1868-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S4-01-A


Manual Integrations
APPROVED

Sohil
3/13/2020 8:31:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 11:27:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

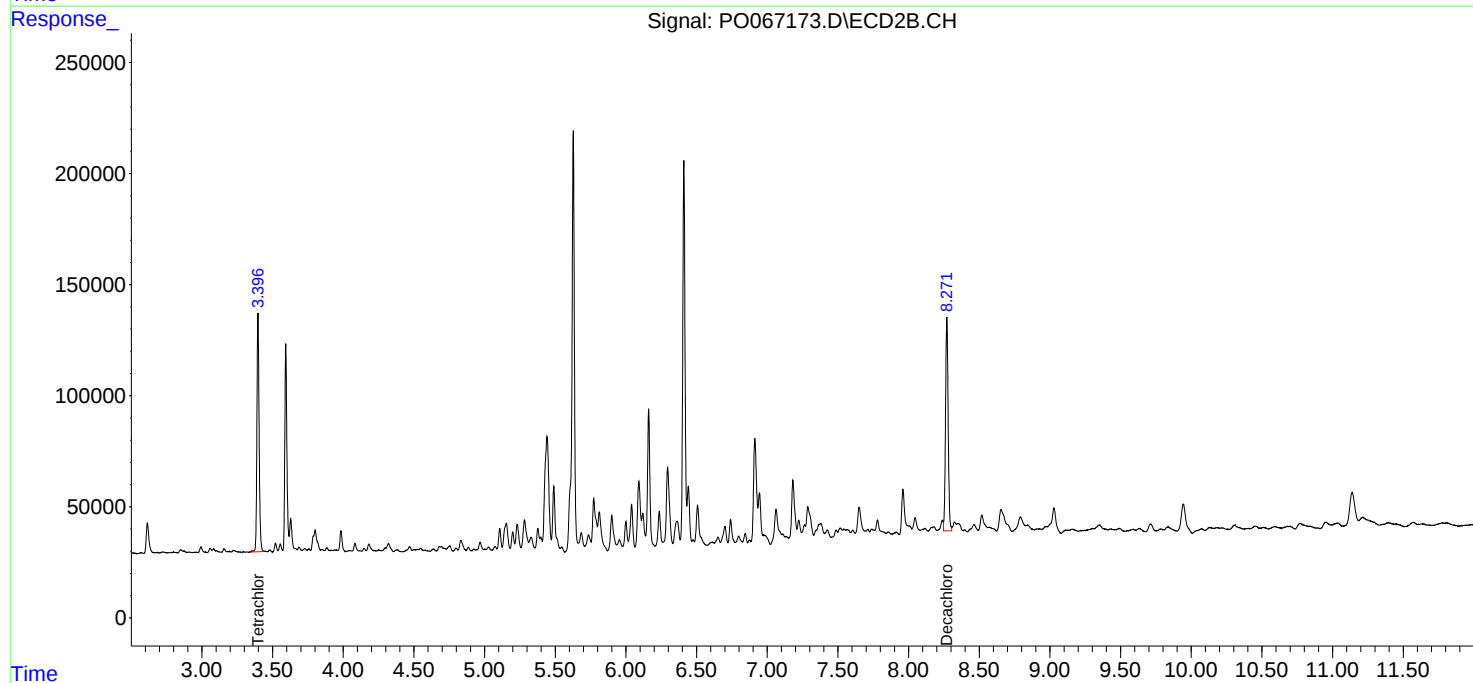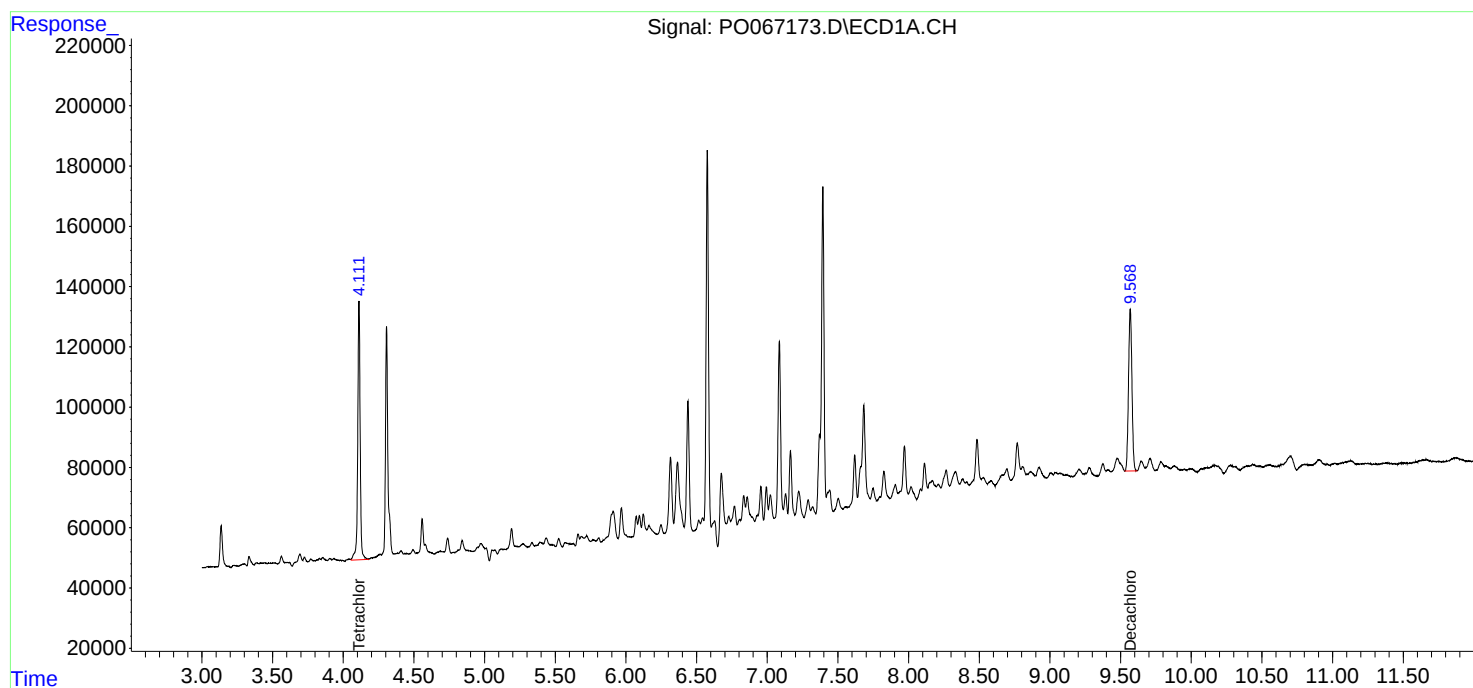

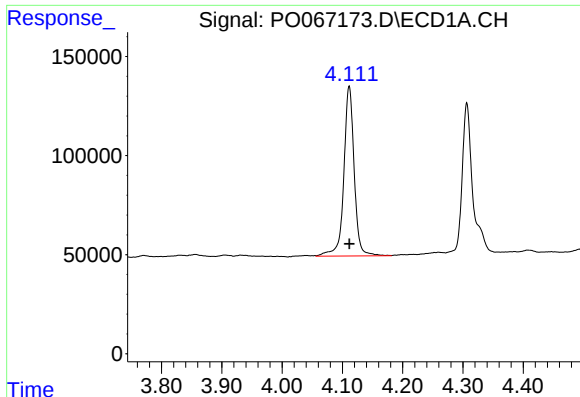


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.001 min
Response: 1024892
Conc: 32.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S4-01-A


Manual Integrations
APPROVED

Sohil
3/13/2020 8:31:59 AM

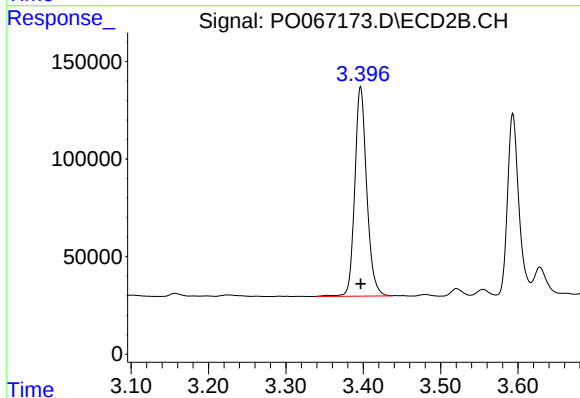


#1 Tetrachloro-m-xylene

R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 1153067
Conc: 29.47 ng/ml m

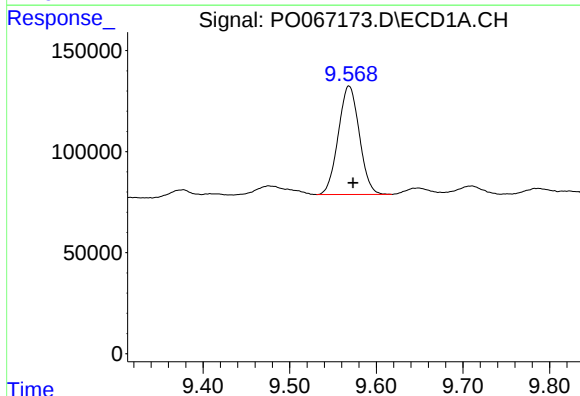

#2 Decachlorobiphenyl

R.T.: 9.569 min
Delta R.T.: -0.005 min
Response: 905834
Conc: 24.94 ng/ml

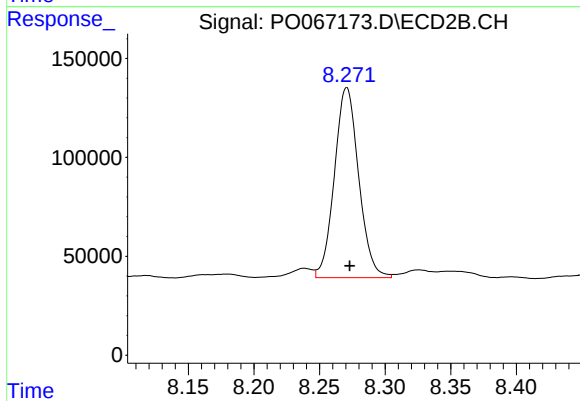

#2 Decachlorobiphenyl

R.T.: 8.271 min
Delta R.T.: -0.003 min
Response: 1235980
Conc: 25.38 ng/ml m