

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
 Data File : P0067184.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2020 14:37
 Operator : DD\AJ
 Sample : L1752-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-01-031120

Manual Integrations
 APPROVED

Sohil
 3/13/2020 8:32:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 18:14:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.110	3.397	626629	762116	20.047m	19.476
2) SA Decachlor...	9.569	8.271	698474	891346	19.229	18.306

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
Data File : P0067184.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2020 14:37
Operator : DD\AJ
Sample : L1752-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-01-031120


Manual Integrations
APPROVED

Sohil
3/13/2020 8:32:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 18:14:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

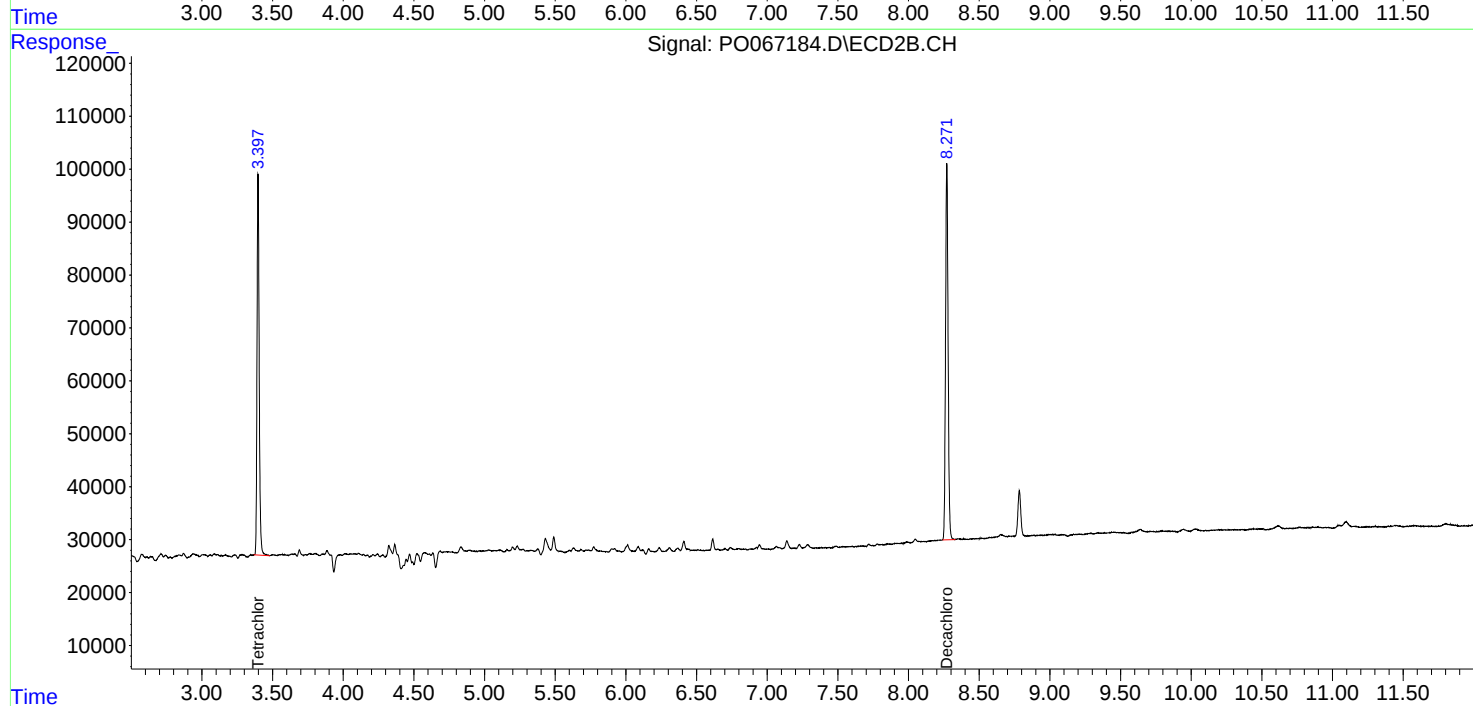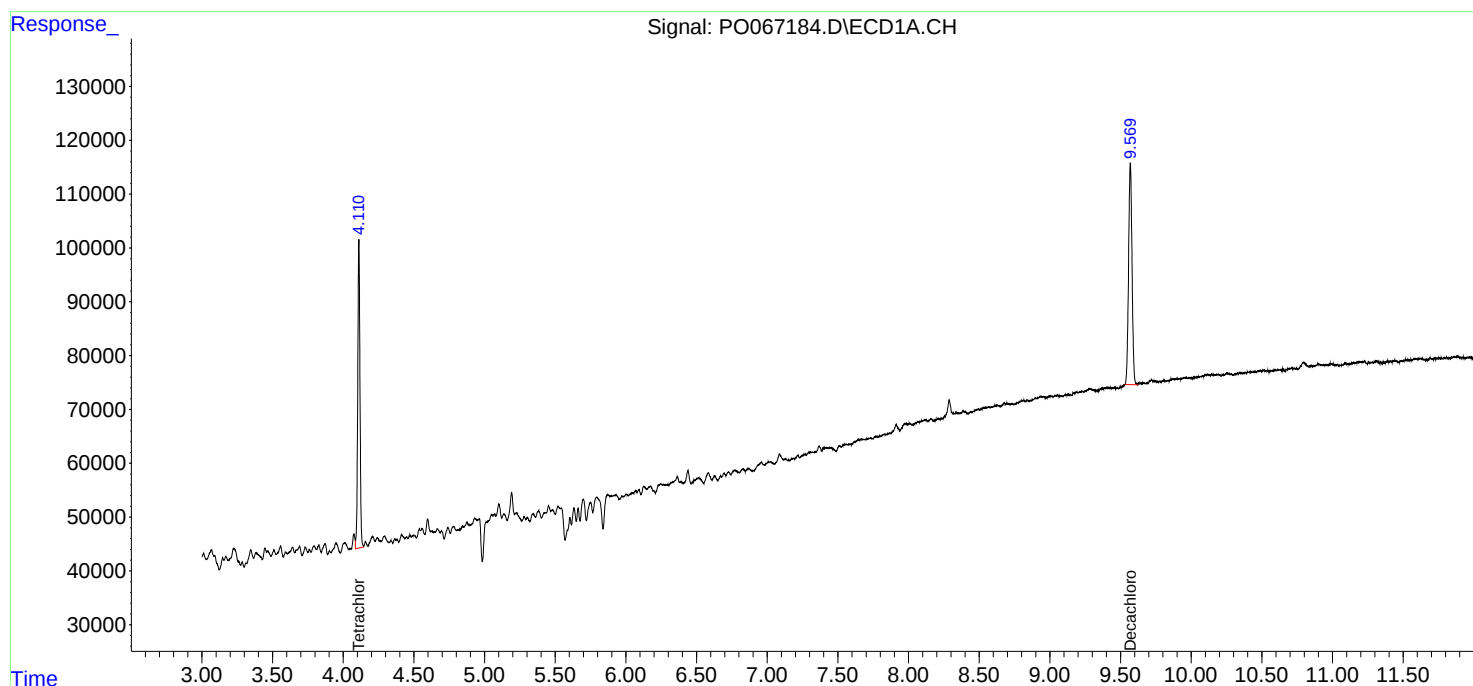

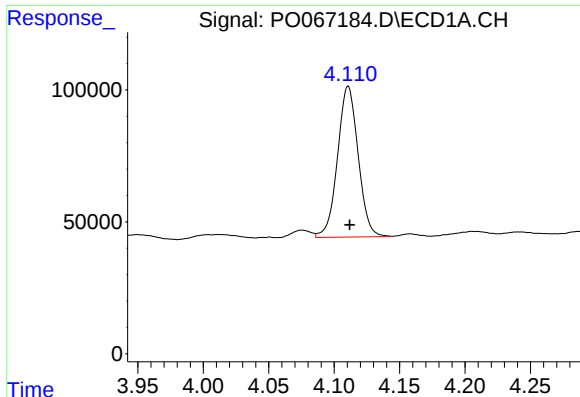


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 626629
Conc: 20.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HD-01-031120


Manual Integrations
APPROVED

Sohil
3/13/2020 8:32:07 AM

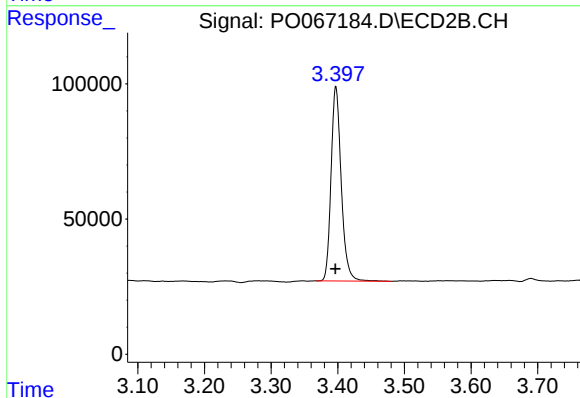


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 762116
Conc: 19.48 ng/ml

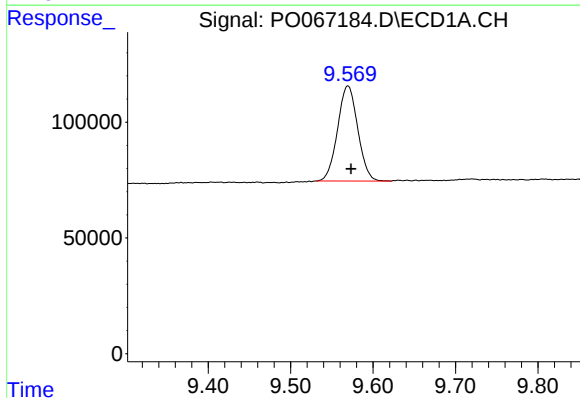

#2 Decachlorobiphenyl

R.T.: 9.569 min
Delta R.T.: -0.004 min
Response: 698474
Conc: 19.23 ng/ml

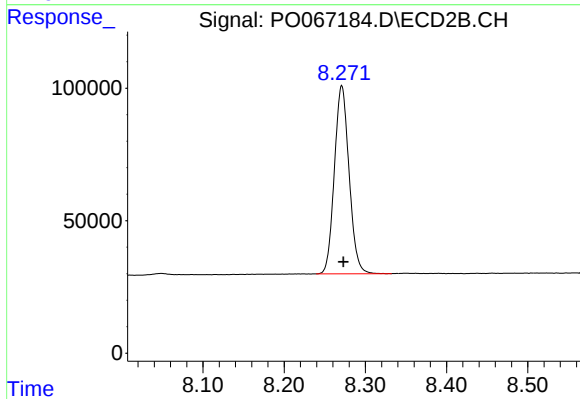

#2 Decachlorobiphenyl

R.T.: 8.271 min
Delta R.T.: -0.002 min
Response: 891346
Conc: 18.31 ng/ml