

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
Data File : P0067191.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2020 16:52
Operator : DD\AJ
Sample : L1889-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:55:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.112	3.397	744835	873479	23.828	22.322
2) SA Decachlor...	9.573	8.271	709581	937048	19.535	19.245

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
Data File : P0067191.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2020 16:52
Operator : DD\AJ
Sample : L1889-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:55:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

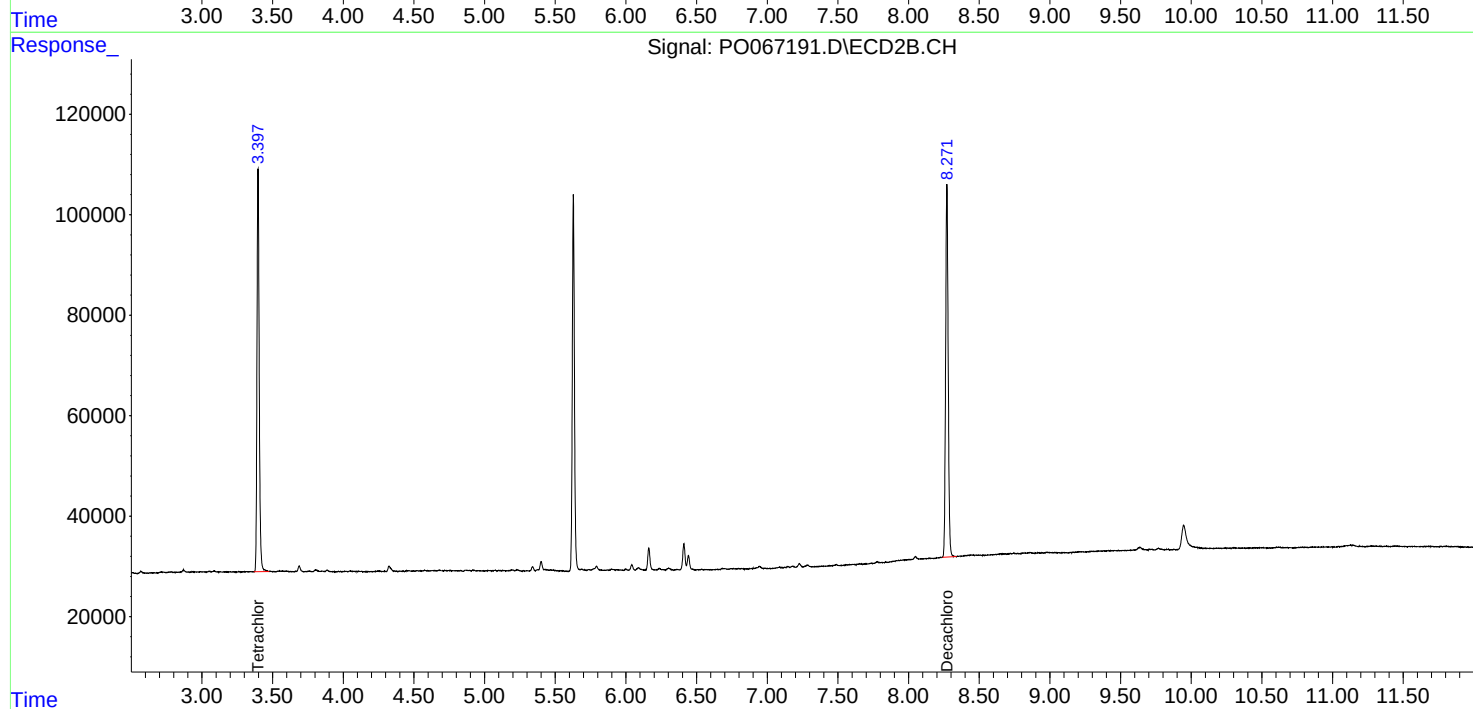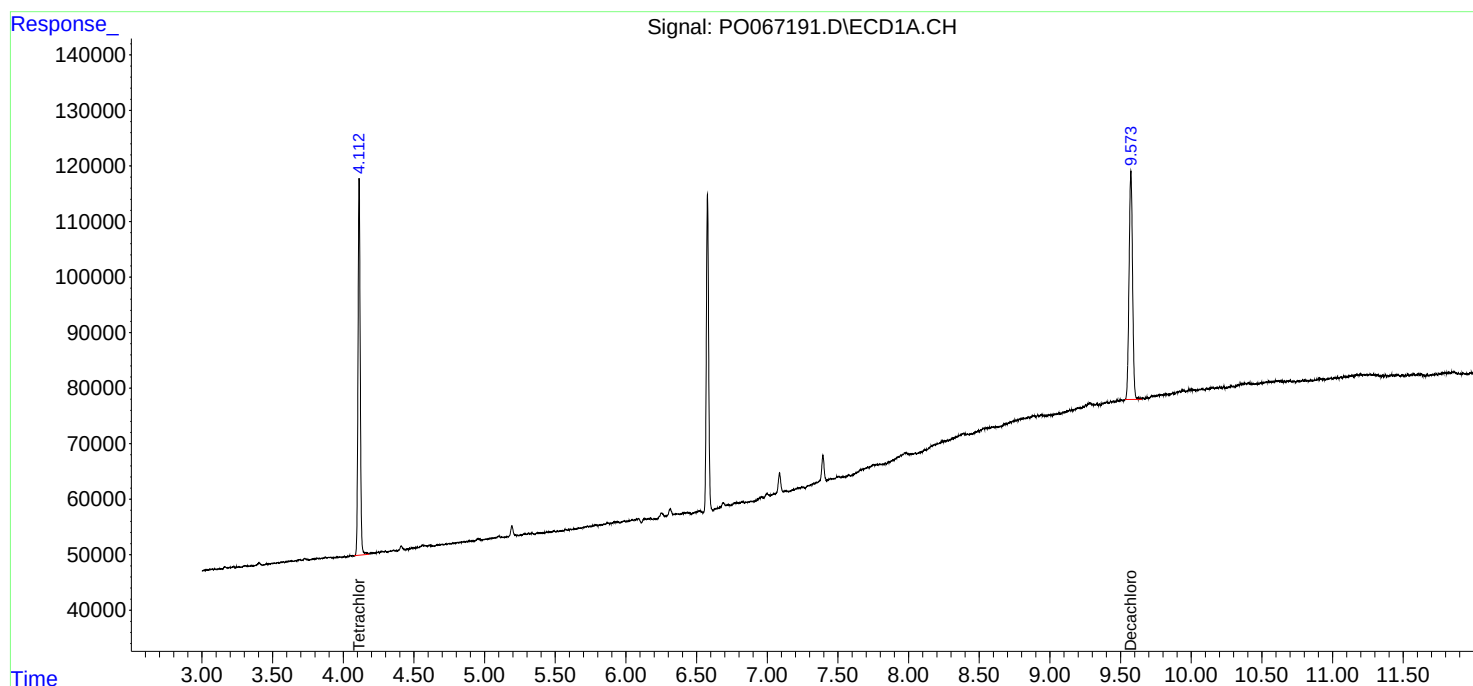


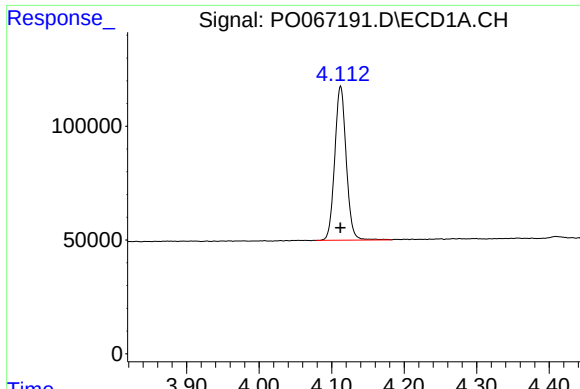

#1 Tetrachloro-m-xylene


R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 744835
Conc: 23.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
CP-2

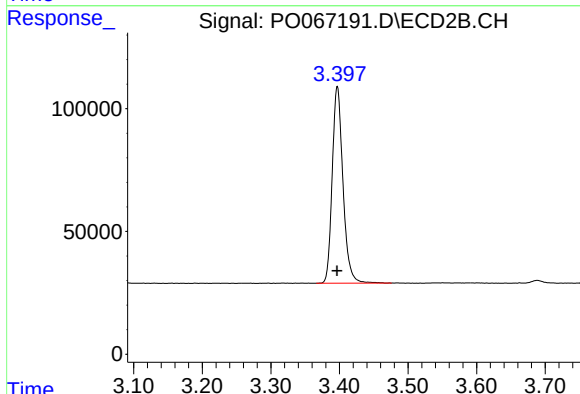


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 873479
Conc: 22.32 ng/ml

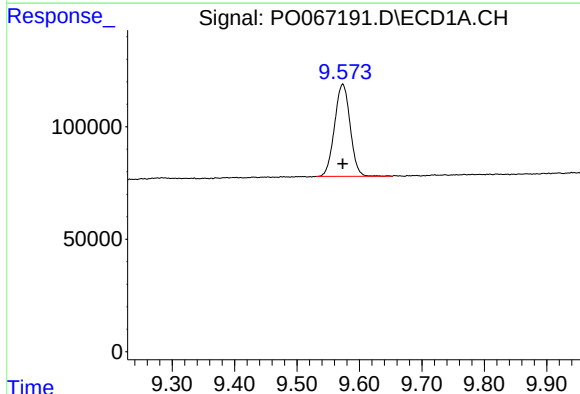

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: 0.000 min
Response: 709581
Conc: 19.53 ng/ml

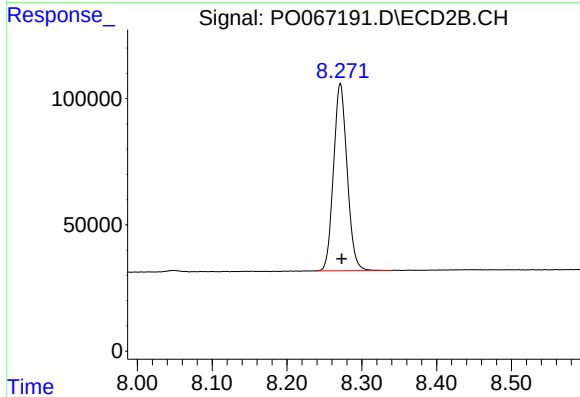

#2 Decachlorobiphenyl

R.T.: 8.271 min
Delta R.T.: -0.002 min
Response: 937048
Conc: 19.24 ng/ml