

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
 Data File : P0067197.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2020 18:32
 Operator : DD\AJ
 Sample : L1893-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2-SA

Manual Integrations
 APPROVED

Sohil
 3/13/2020 8:32:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 04:59:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 11 15:01:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.110	3.397	739597	861429	23.660	22.014
2) SA Decachlor...	9.568	8.270	717657	953060	19.757	19.574m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031220\
Data File : P0067197.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2020 18:32
Operator : DD\AJ
Sample : L1893-06
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-2-SA


Manual Integrations
APPROVED

Sohil
3/13/2020 8:32:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 04:59:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031120.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 11 15:01:31 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

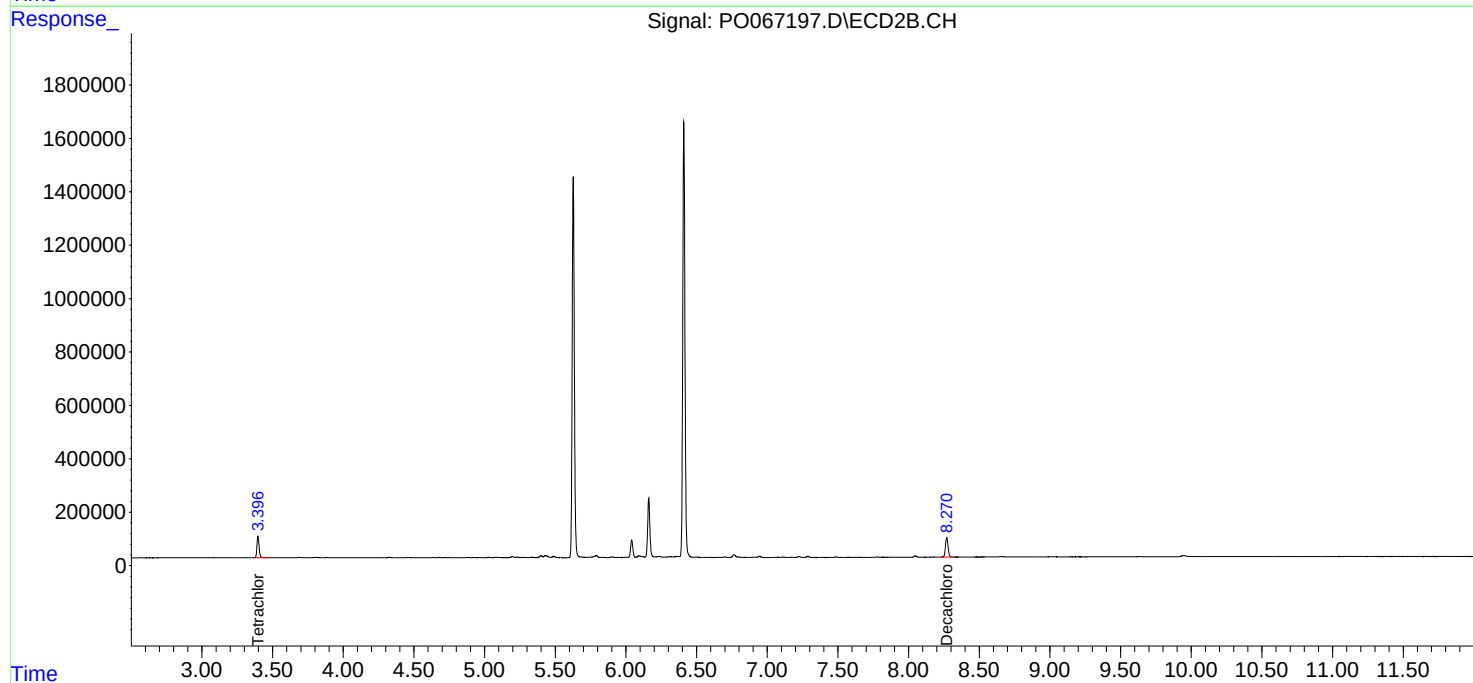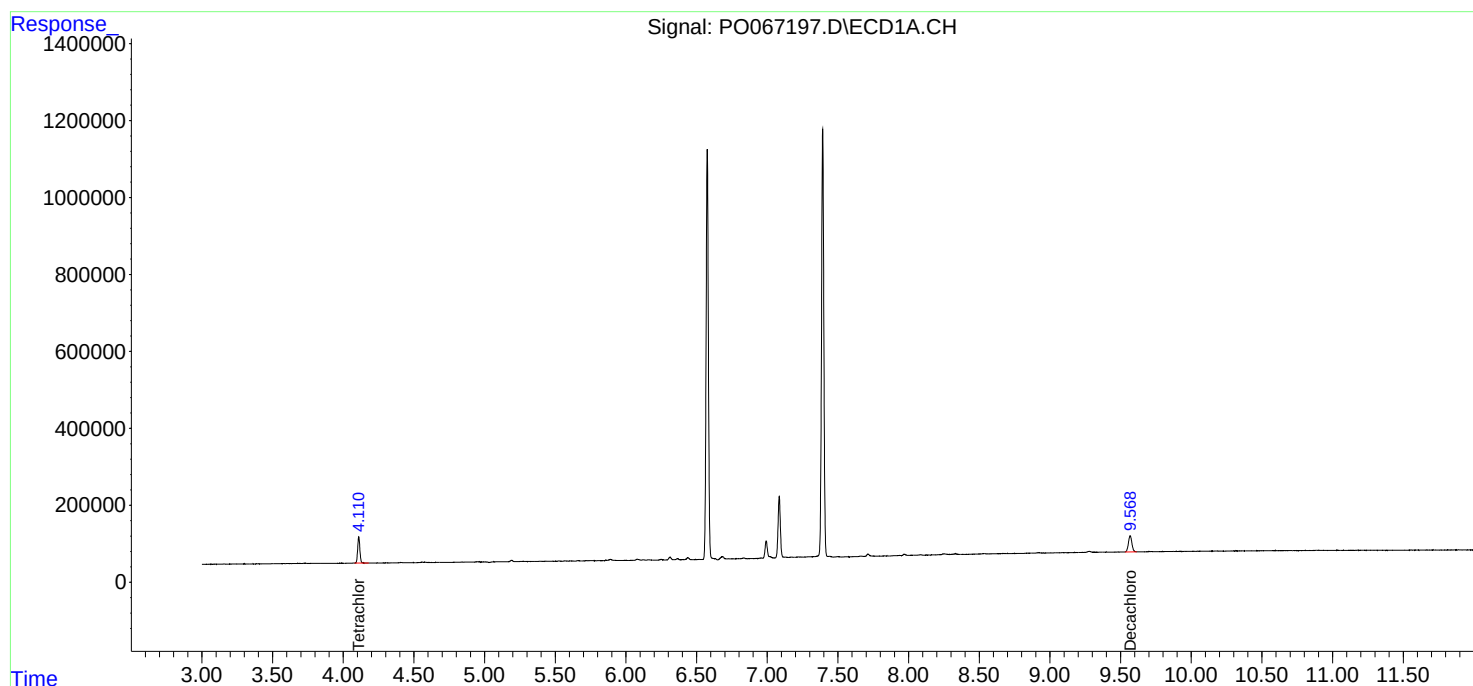

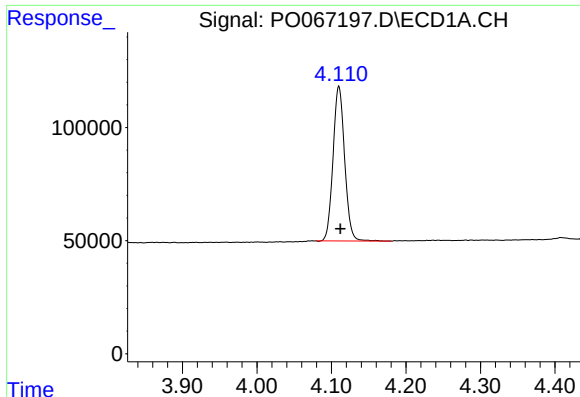


#1 Tetrachloro-m-xylene

R.T.: 4.110 min
Delta R.T.: -0.002 min
Response: 739597
Conc: 23.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2-SA


Manual Integrations
APPROVED

Sohil
3/13/2020 8:32:11 AM

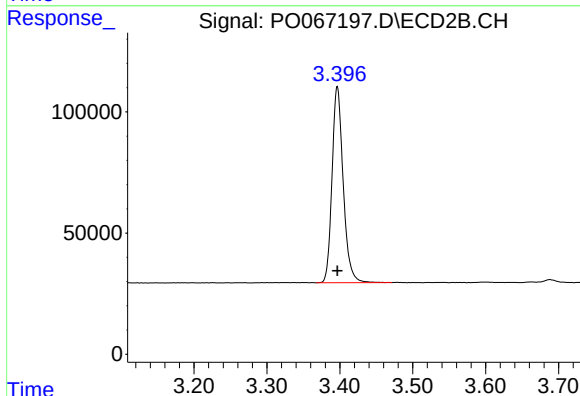


#1 Tetrachloro-m-xylene

R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 861429
Conc: 22.01 ng/ml

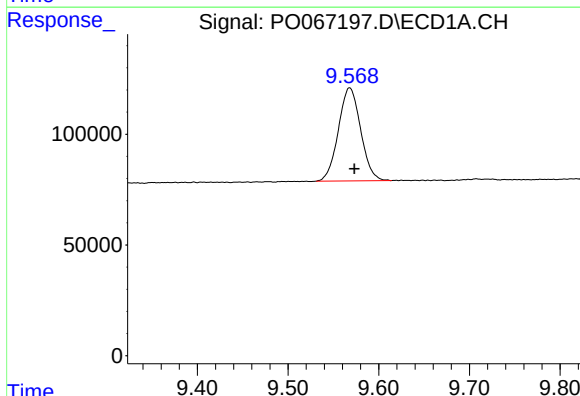

#2 Decachlorobiphenyl

R.T.: 9.568 min
Delta R.T.: -0.005 min
Response: 717657
Conc: 19.76 ng/ml

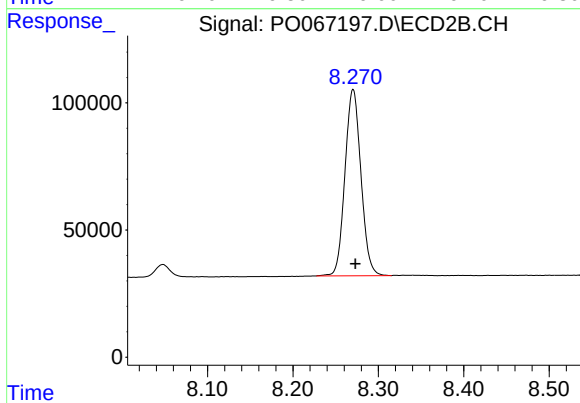

#2 Decachlorobiphenyl

R.T.: 8.270 min
Delta R.T.: -0.003 min
Response: 953060
Conc: 19.57 ng/ml m