

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031225\
 Data File : P0109825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 15:12
 Operator : YP/AJ
 Sample : Q1544-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 5A-5B-5C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/13/2025
 Supervised By :Ankita Jodhani 03/13/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 18:51:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.694	3.691	210.6E6	120.9E6	22.250	23.095
2) SA Decachlor...	8.747	8.699	179.5E6	65317108	20.870m	20.512m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031225\
Data File : PO109825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 15:12
Operator : YP/AJ
Sample : Q1544-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
5A-5B-5C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/13/2025
Supervised By :Ankita Jodhani 03/13/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 18:51:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

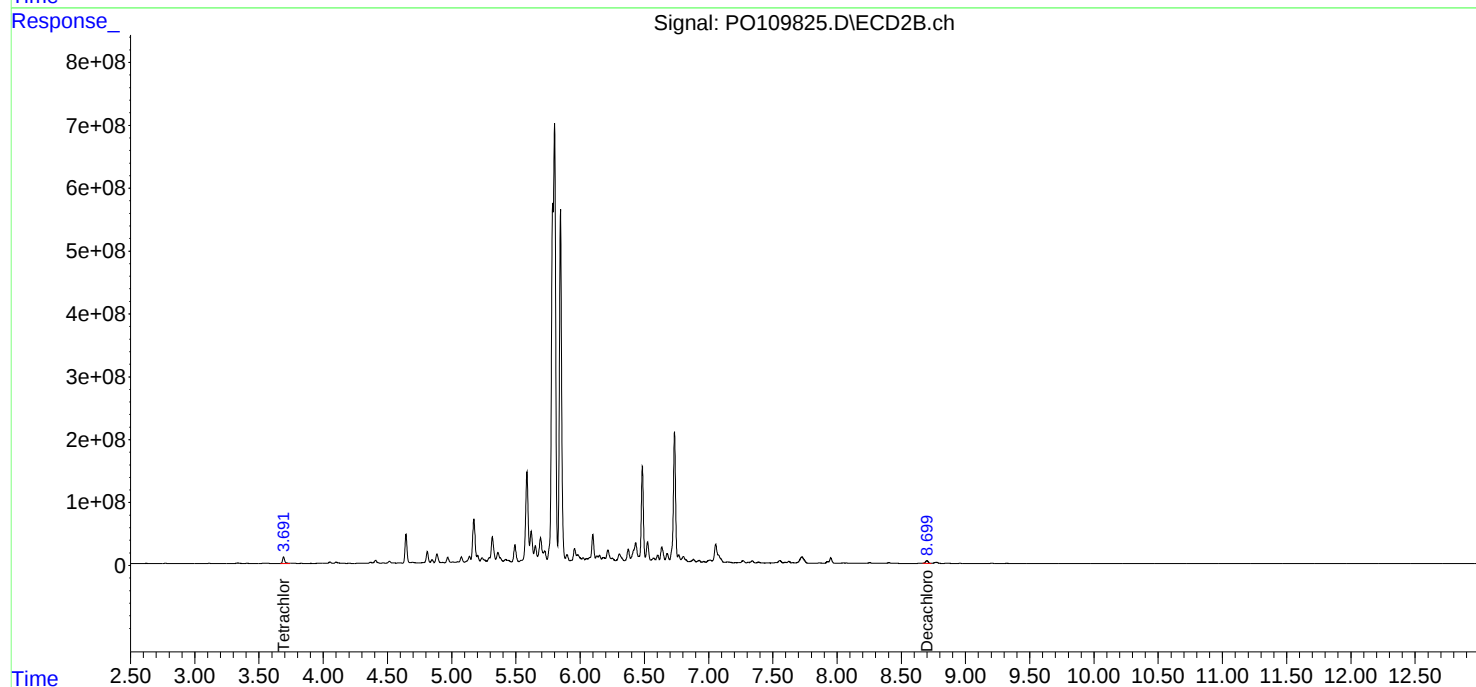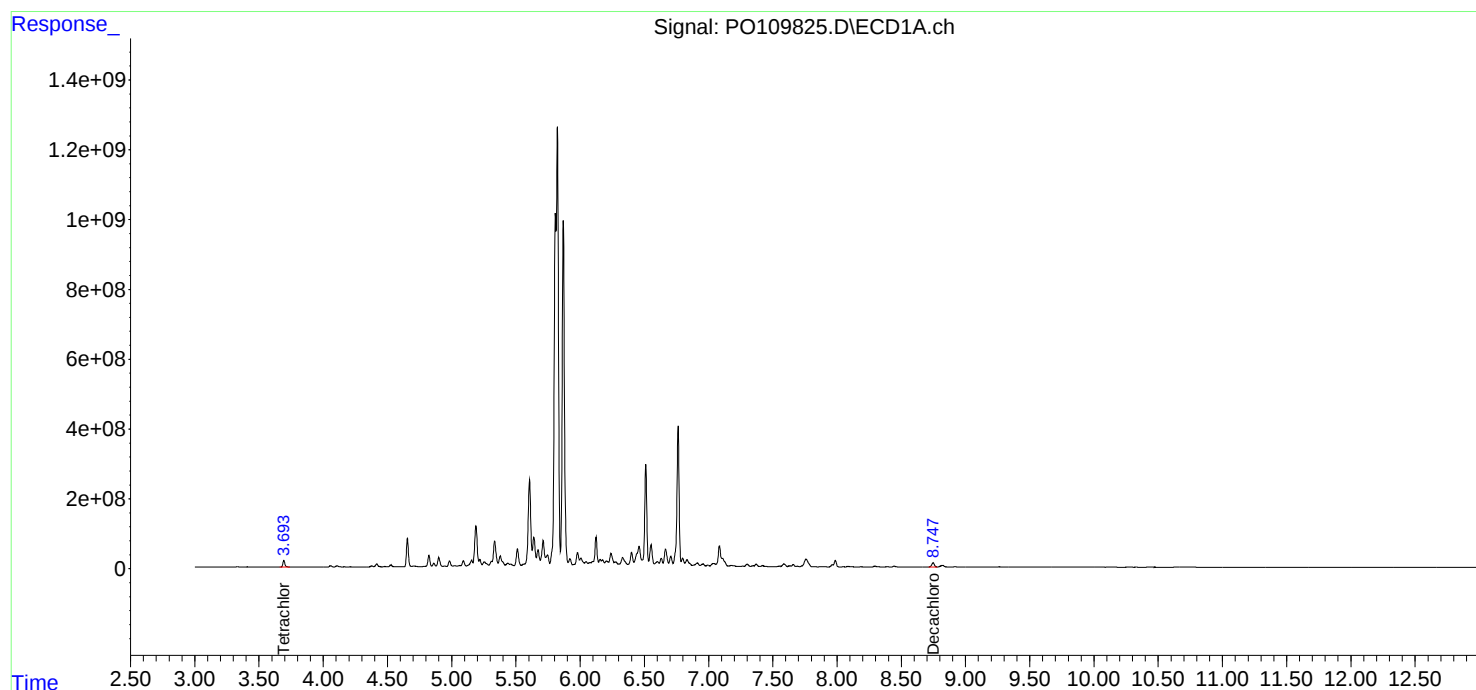

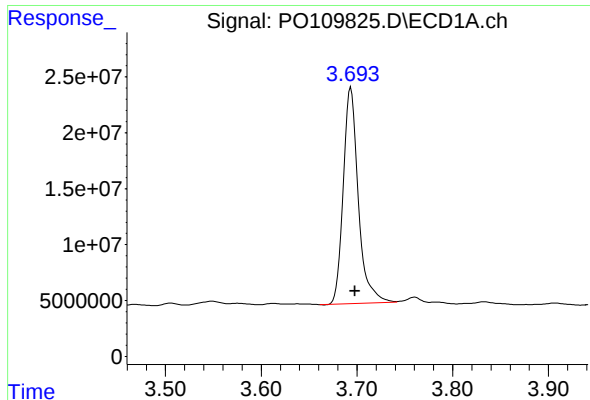


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: -0.004 min
Response: 210601709
Conc: 22.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
5A-5B-5C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/13/2025
Supervised By :Ankita Jodhani 03/13/2025

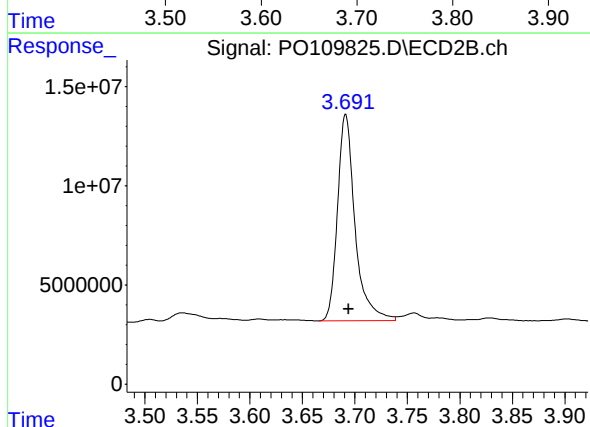


#1 Tetrachloro-m-xylene

R.T.: 3.691 min
Delta R.T.: -0.003 min
Response: 120886427
Conc: 23.10 ng/ml

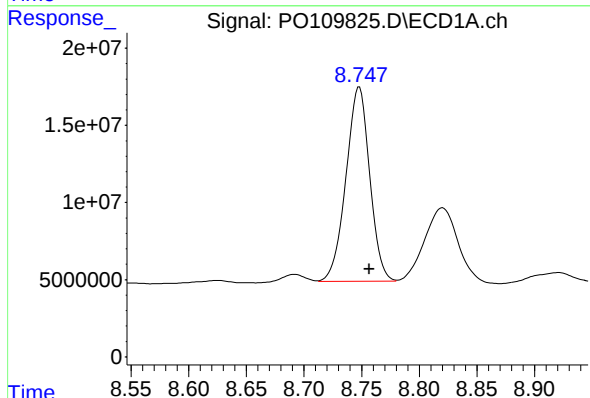

#2 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: -0.009 min
Response: 179524719
Conc: 20.87 ng/ml m

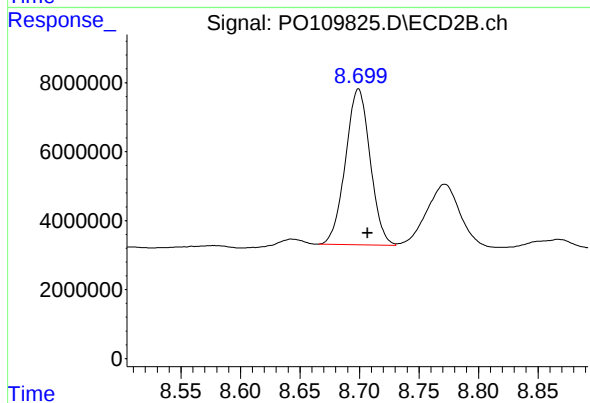

#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: -0.008 min
Response: 65317108
Conc: 20.51 ng/ml m