

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
 Data File : P0076137.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 6:45
 Operator : DD\AJ
 Sample : M1649-07 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONCRETE-PILE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 03:09:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.922	3.940	120868	89119	2.028	1.998
2)	SA Decachlor...	10.925	9.206f	92795	99024	2.825	2.723

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
Data File : P0076137.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 6:45
Operator : DD\AJ
Sample : M1649-07 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 03:09:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

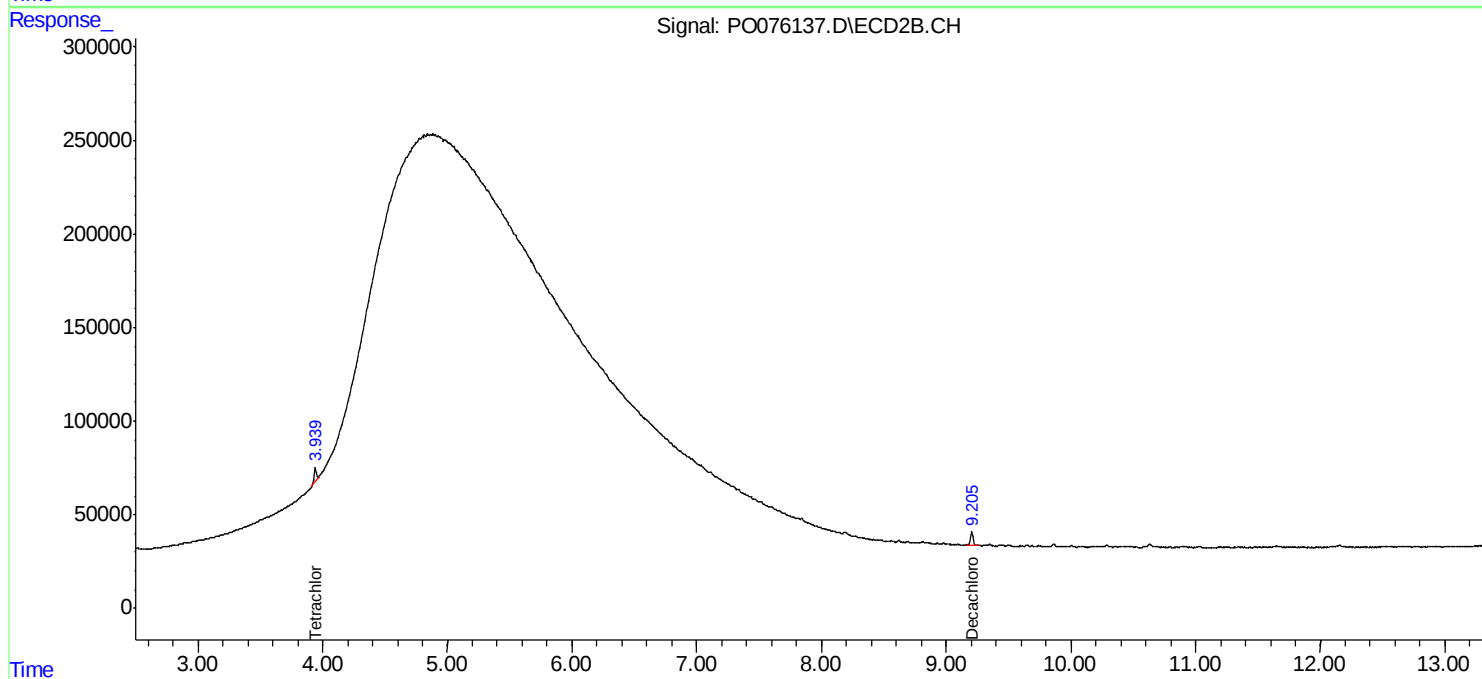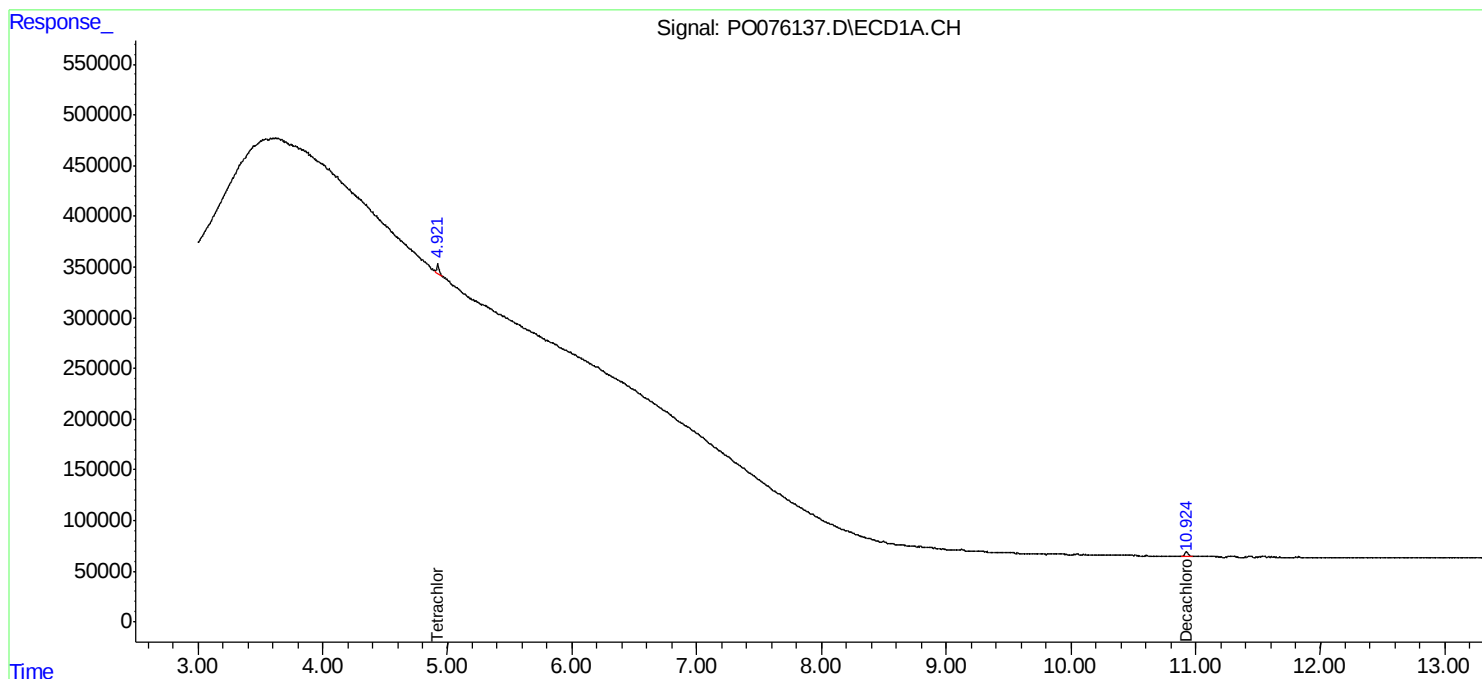


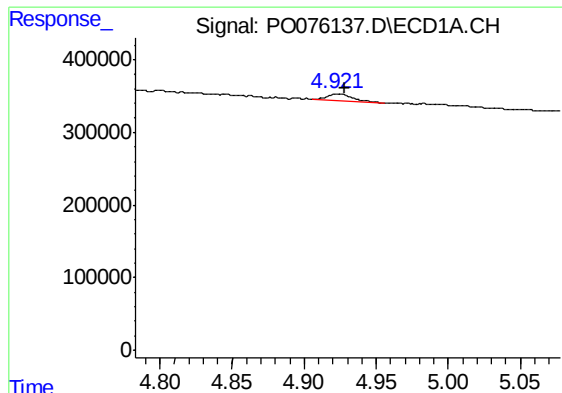

#1 Tetrachloro-m-xylene


R.T.: 4.922 min
Delta R.T.: -0.006 min
Response: 120868
Conc: 2.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONCRETE-PILE-1

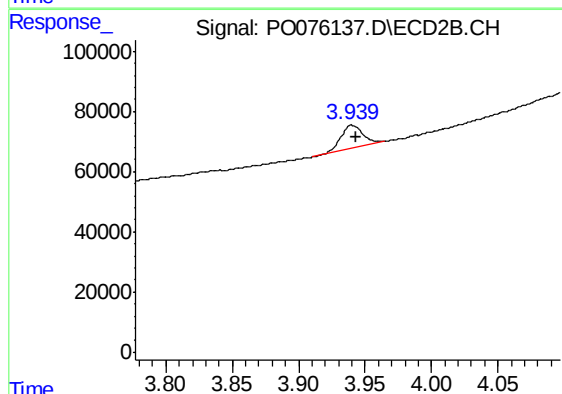


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: -0.003 min
Response: 89119
Conc: 2.00 ng/ml

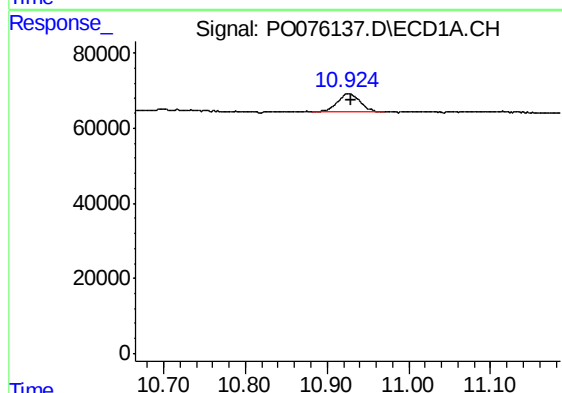

#2 Decachlorobiphenyl

R.T.: 10.925 min
Delta R.T.: -0.005 min
Response: 92795
Conc: 2.82 ng/ml

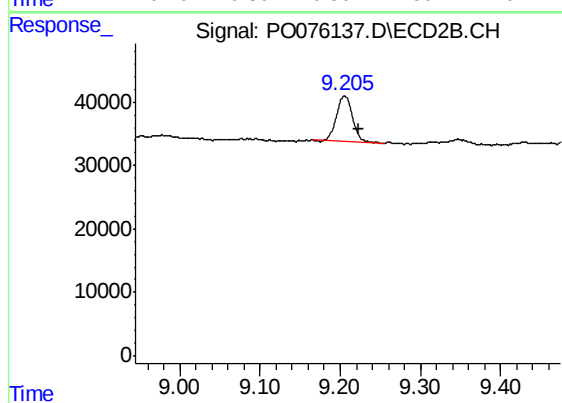

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.017 min
Response: 99024
Conc: 2.72 ng/ml