

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
 Data File : P0076110.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2021 16:27
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:07:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 02:56:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	3.941	2770160	2054551	46.474	46.058
2) SA Decachlor...	10.933	9.211	1747508	1727075	53.194	47.498
Target Compounds						
21) L5 AR-1248-1	6.250	5.189	453845	424213	416.368	459.691m
22) L5 AR-1248-2	6.545	5.450	663336	640582	423.050	447.719
23) L5 AR-1248-3	6.762	5.494	799115	647119	444.885	439.463
24) L5 AR-1248-4	7.192	5.677	855869	736689	447.954	436.069
25) L5 AR-1248-5	7.232	6.100	849693	726422	448.803	435.826

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031321\
Data File : PO076110.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2021 16:27
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:07:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 02:56:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

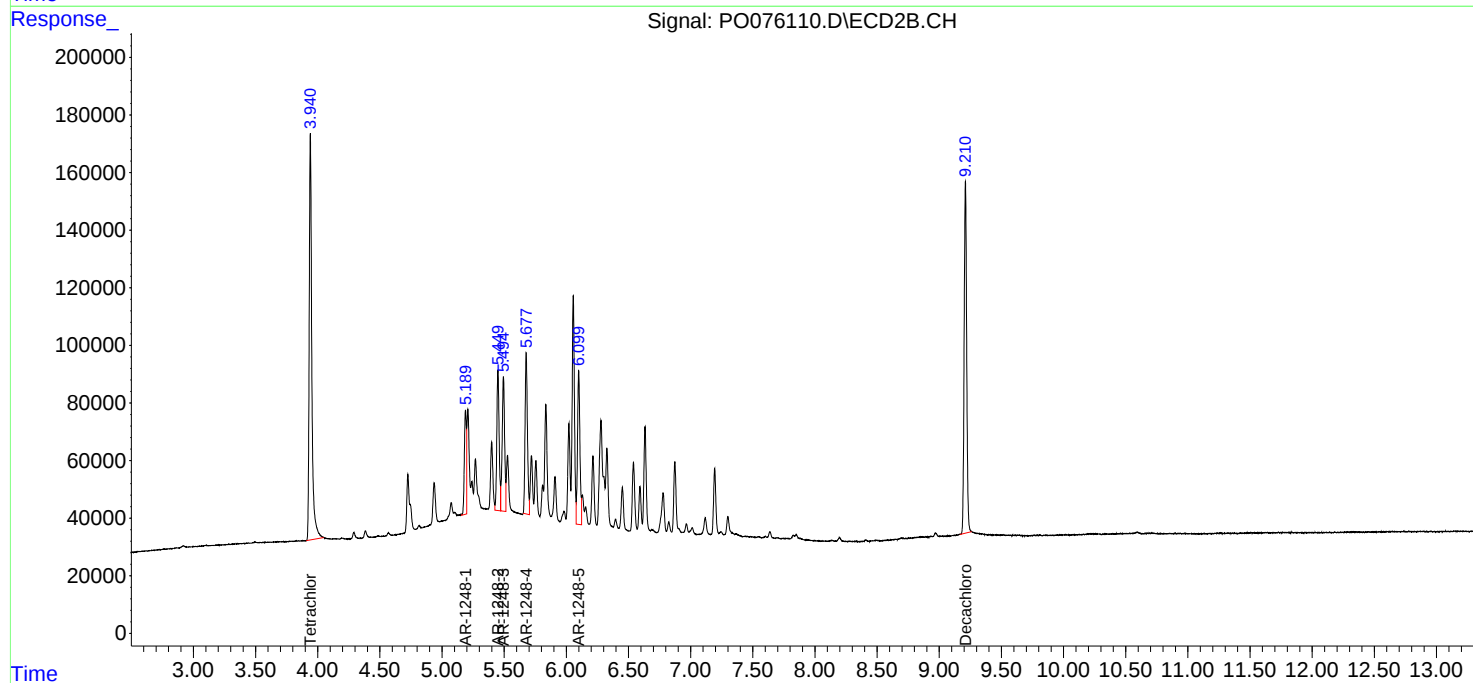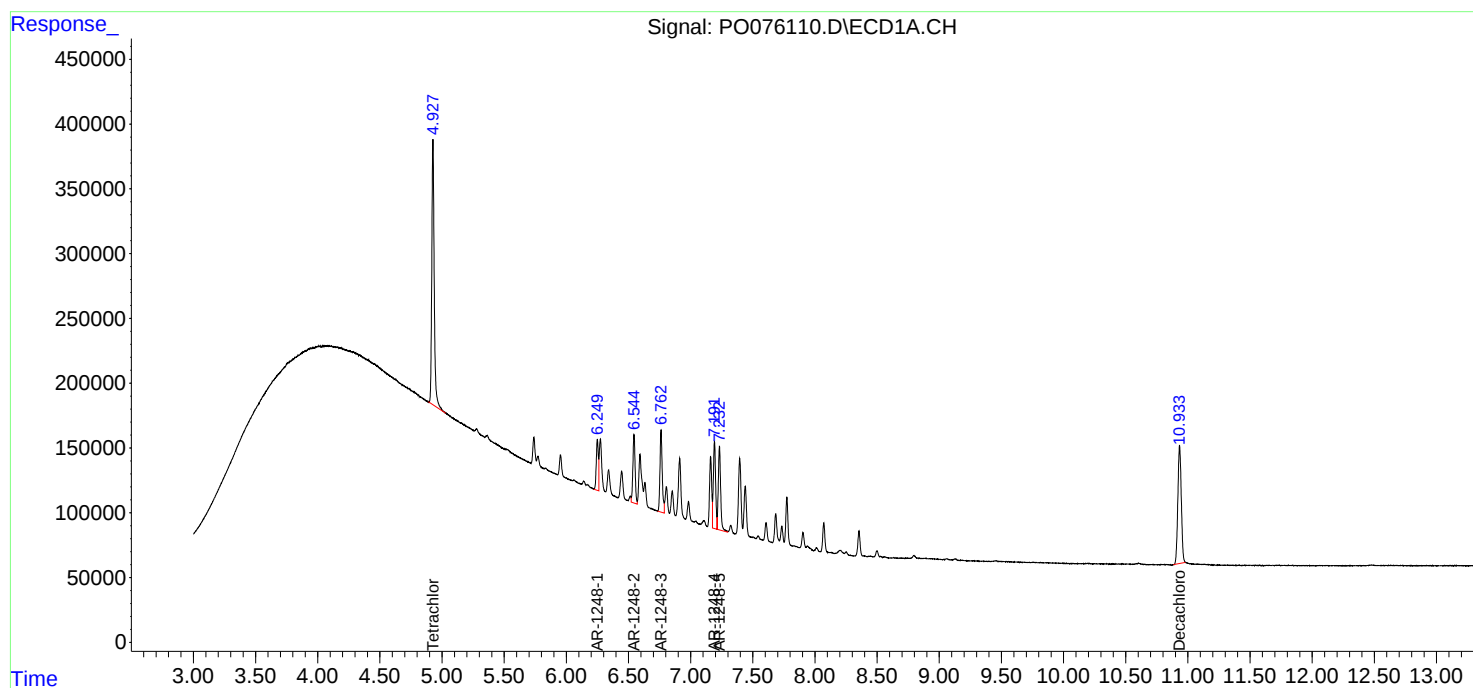

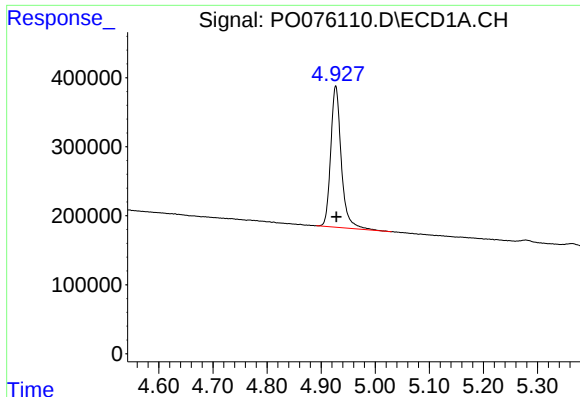


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 2770160
Conc: 46.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:07:31 PM

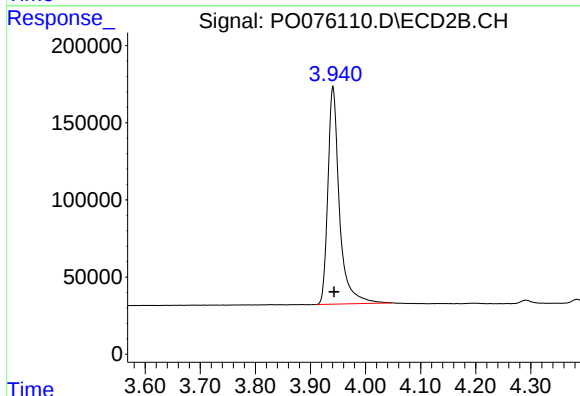


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 2054551
Conc: 46.06 ng/ml

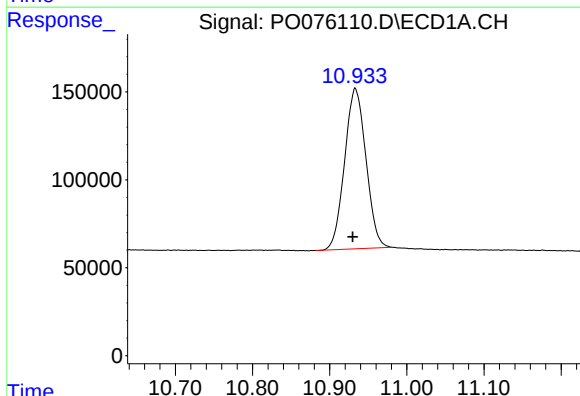


#2 Decachlorobiphenyl

R.T.: 10.933 min
Delta R.T.: 0.003 min
Response: 1747508
Conc: 53.19 ng/ml

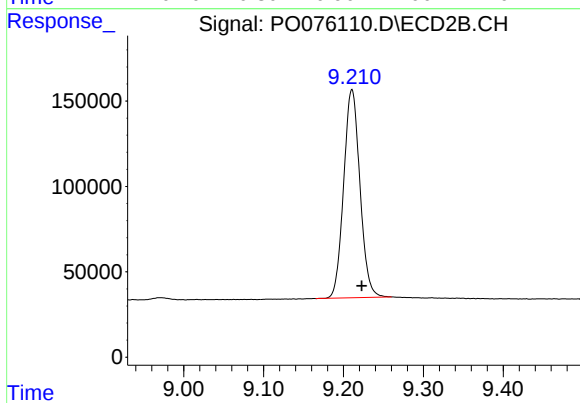

#2 Decachlorobiphenyl

R.T.: 9.211 min
Delta R.T.: -0.012 min
Response: 1727075
Conc: 47.50 ng/ml

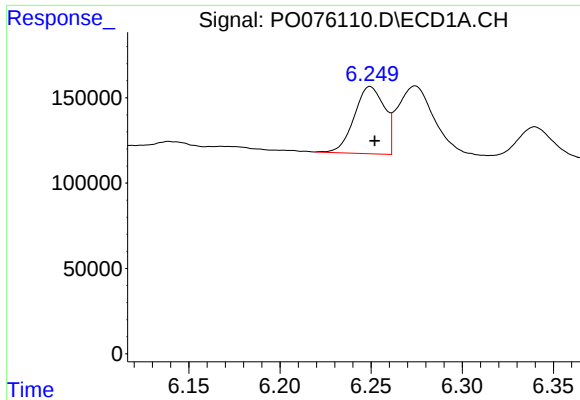


#21 AR-1248-1

R.T.: 6.250 min
Delta R.T.: -0.002 min
Response: 453845
Conc: 416.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:07:31 PM

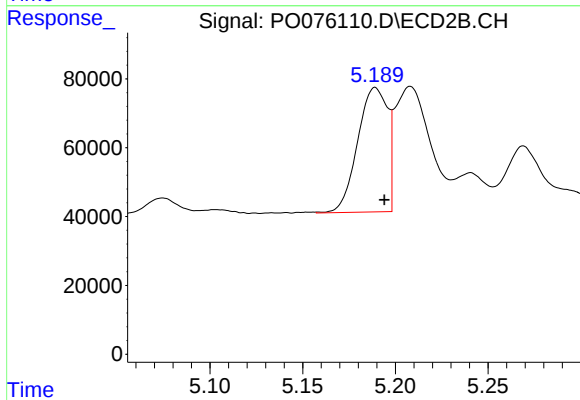


#21 AR-1248-1

R.T.: 5.189 min
Delta R.T.: -0.005 min
Response: 424213
Conc: 459.69 ng/ml m

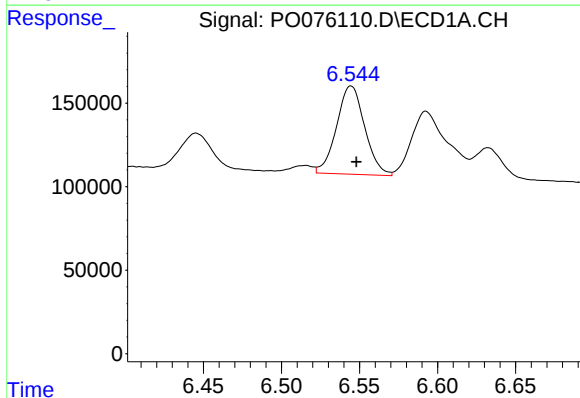


#22 AR-1248-2

R.T.: 6.545 min
Delta R.T.: -0.003 min
Response: 663336
Conc: 423.05 ng/ml

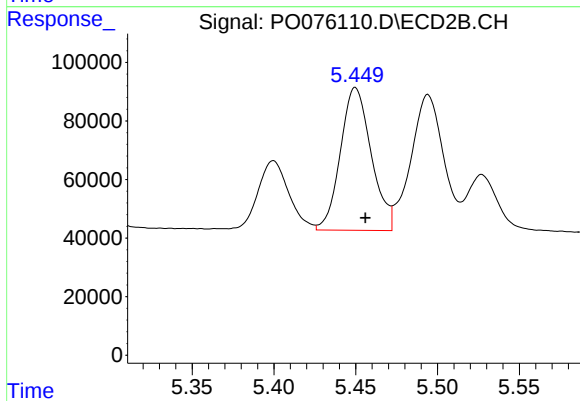

#22 AR-1248-2

R.T.: 5.450 min
Delta R.T.: -0.006 min
Response: 640582
Conc: 447.72 ng/ml

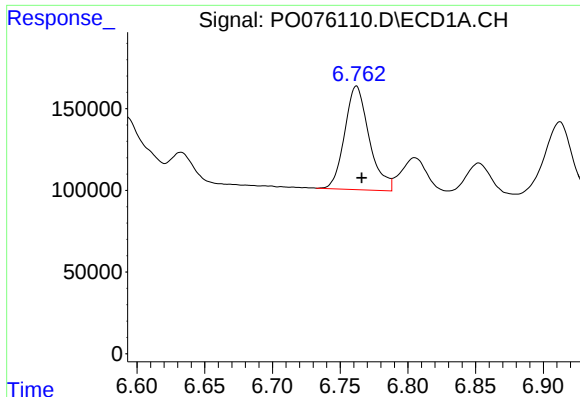


#23 AR-1248-3

R.T.: 6.762 min
Delta R.T.: -0.004 min
Response: 799115
Conc: 444.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/15/2021 1:07:31 PM

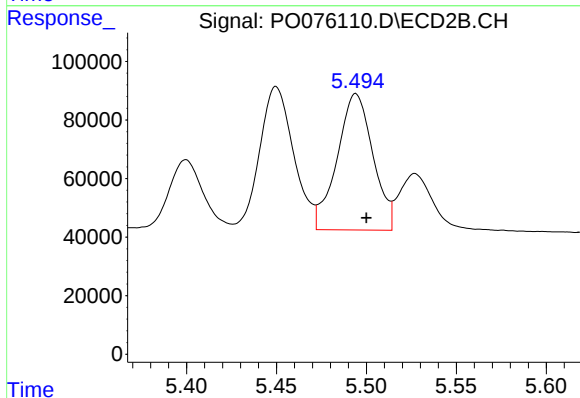


#23 AR-1248-3

R.T.: 5.494 min
Delta R.T.: -0.006 min
Response: 647119
Conc: 439.46 ng/ml

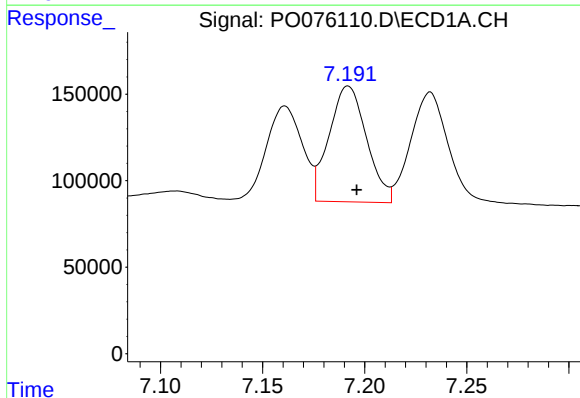


#24 AR-1248-4

R.T.: 7.192 min
Delta R.T.: -0.004 min
Response: 855869
Conc: 447.95 ng/ml

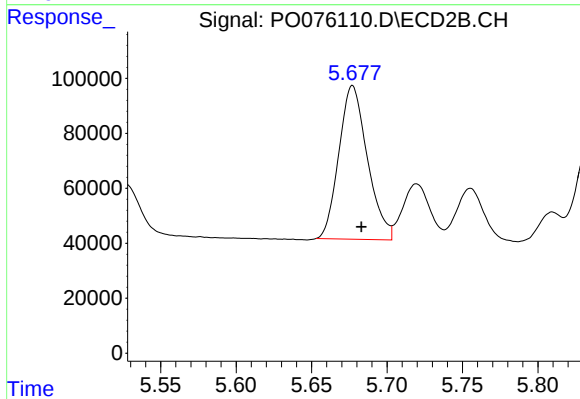

#24 AR-1248-4

R.T.: 5.677 min
Delta R.T.: -0.006 min
Response: 736689
Conc: 436.07 ng/ml

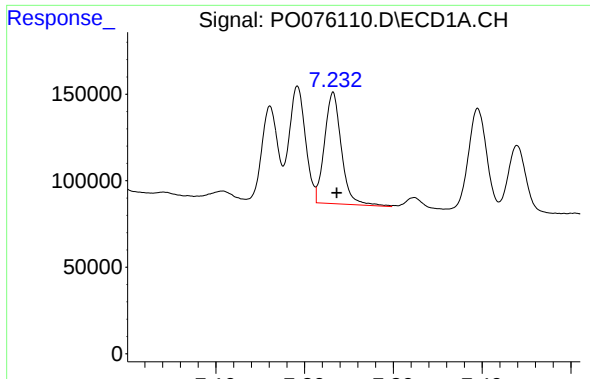


#25 AR-1248-5

R.T.: 7.232 min
Delta R.T.: -0.004 min
Response: 849693
Conc: 448.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/15/2021 1:07:31 PM

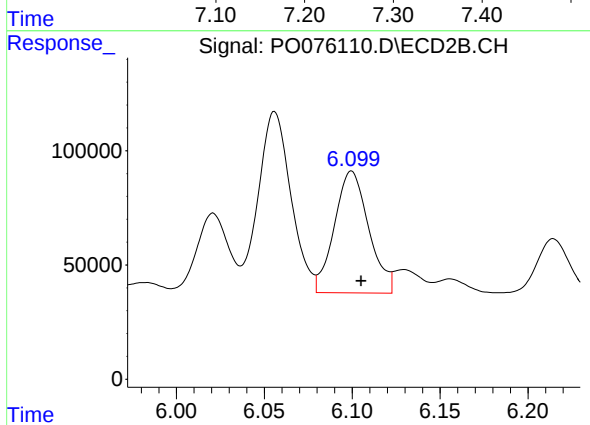

#25 AR-1248-5

R.T.: 6.100 min
Delta R.T.: -0.005 min
Response: 726422
Conc: 435.83 ng/ml