

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
 Data File : P0076116.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2021 19:18
 Operator : DD\AJ
 Sample : M1619-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30624

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:08:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 02:59:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.941	75477	138933	1.266	3.115 #
2) SA Decachlor...	10.935	9.213	80094	112641	2.438m	3.098m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
Data File : P0076116.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2021 19:18
Operator : DD\AJ
Sample : M1619-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30624


Manual Integrations
APPROVED

Ankita
3/15/2021 1:08:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 02:59:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

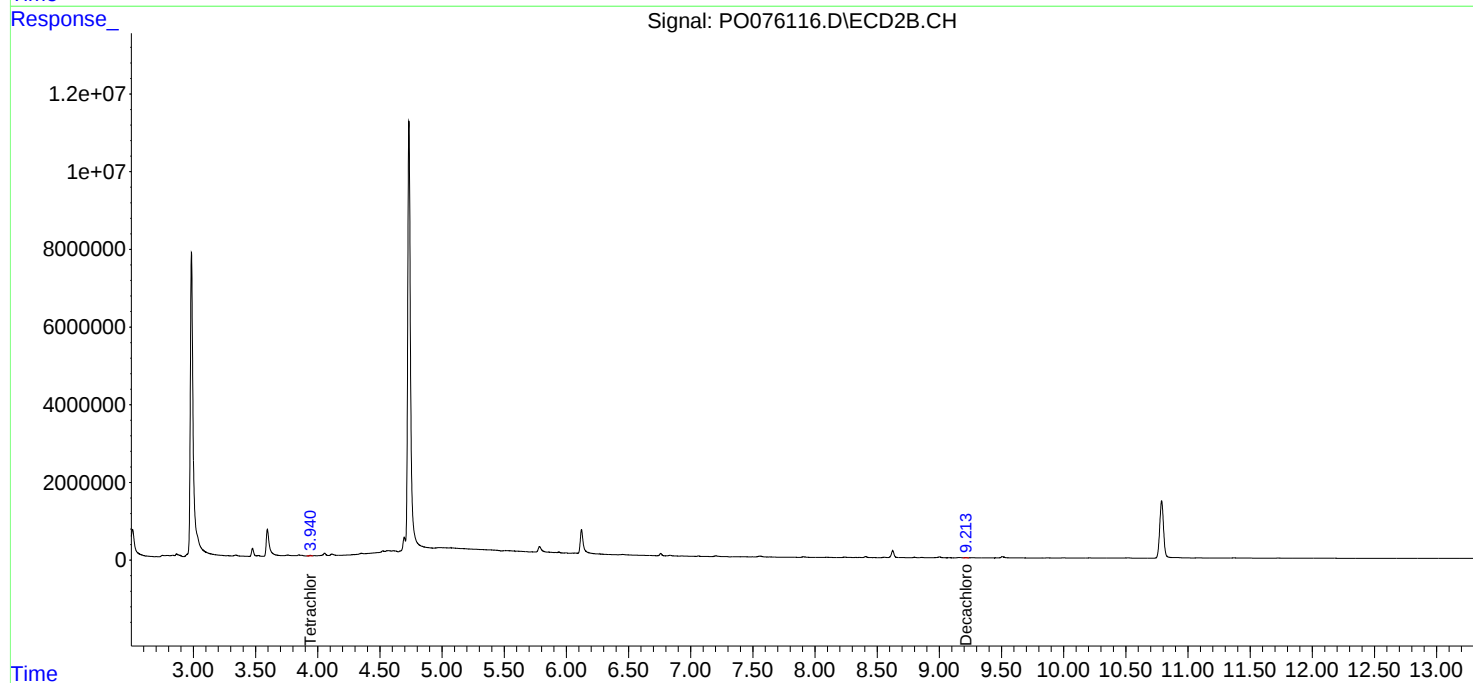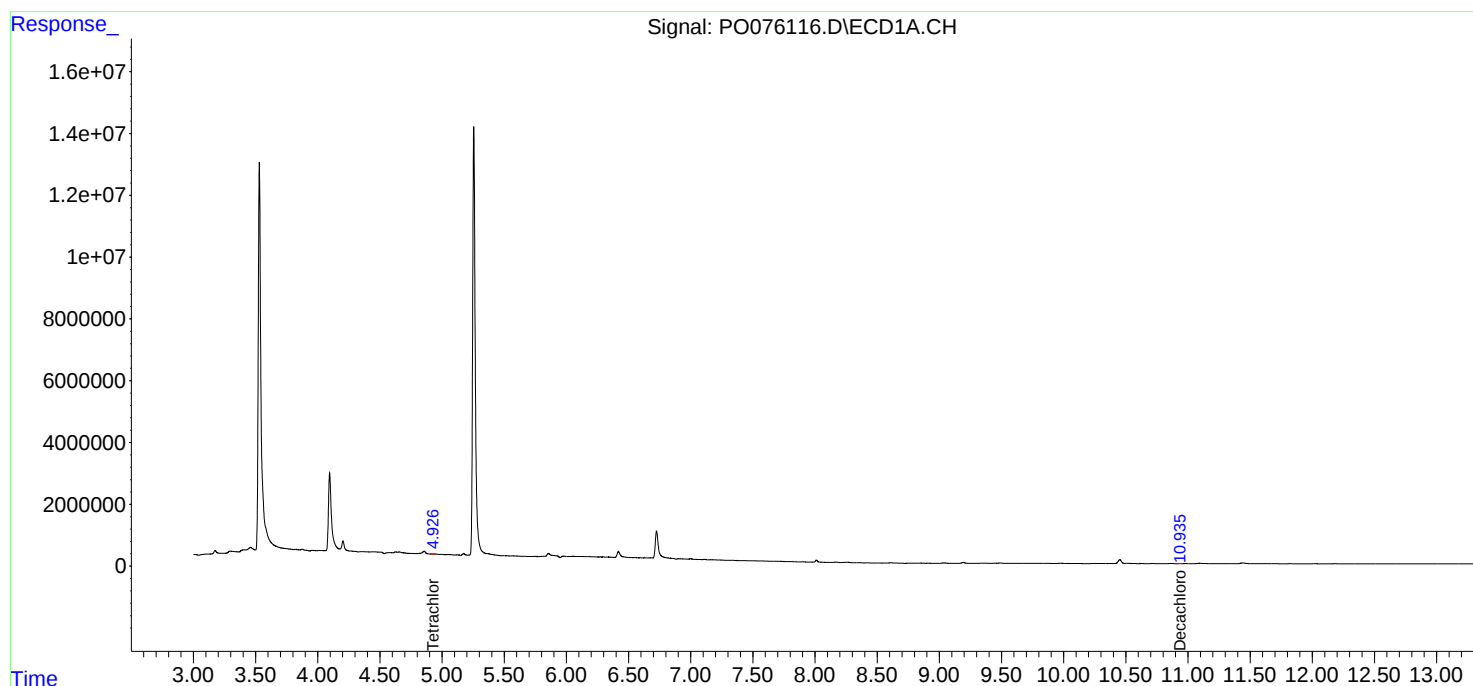

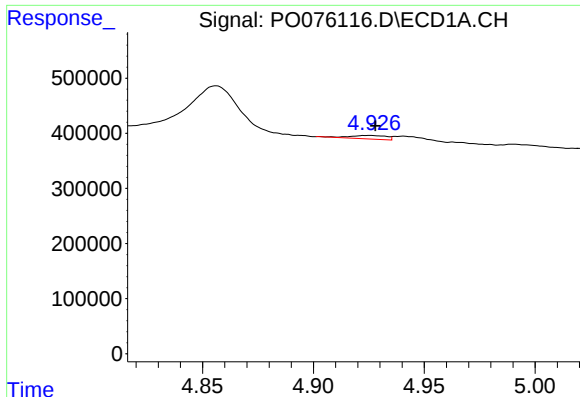


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: -0.003 min
Response: 75477
Conc: 1.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
30624


Manual Integrations
APPROVED

Ankita
3/15/2021 1:08:03 PM

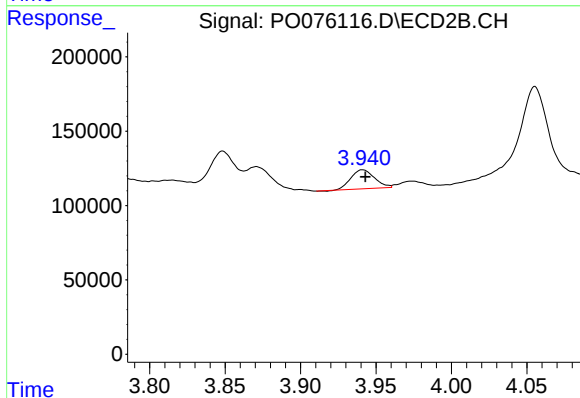


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 138933
Conc: 3.11 ng/ml

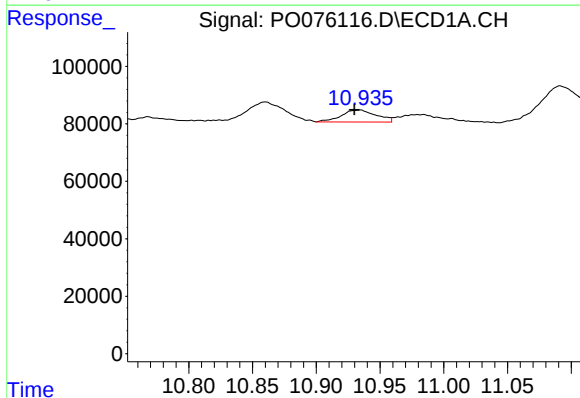

#2 Decachlorobiphenyl

R.T.: 10.935 min
Delta R.T.: 0.005 min
Response: 80094
Conc: 2.44 ng/ml m

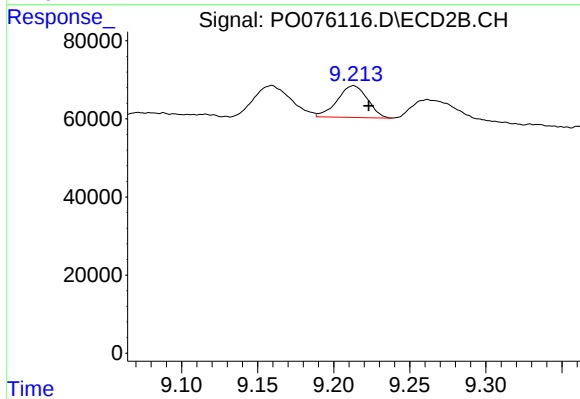

#2 Decachlorobiphenyl

R.T.: 9.213 min
Delta R.T.: -0.010 min
Response: 112641
Conc: 3.10 ng/ml m