

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
 Data File : P0076120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Mar 2021 21:36
 Operator : DD\AJ
 Sample : M1627-02 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEH585T-END-2

Manual Integrations
 APPROVED

Ankita
 3/15/2021 1:08:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 03:01:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.941	99967	80421	1.677	1.803
2) SA Decachlor...	10.933	9.213	70243	77317	2.138	2.126m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
Data File : P0076120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Mar 2021 21:36
Operator : DD\AJ
Sample : M1627-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEH585T-END-2


Manual Integrations
APPROVED

Ankita
3/15/2021 1:08:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 03:01:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

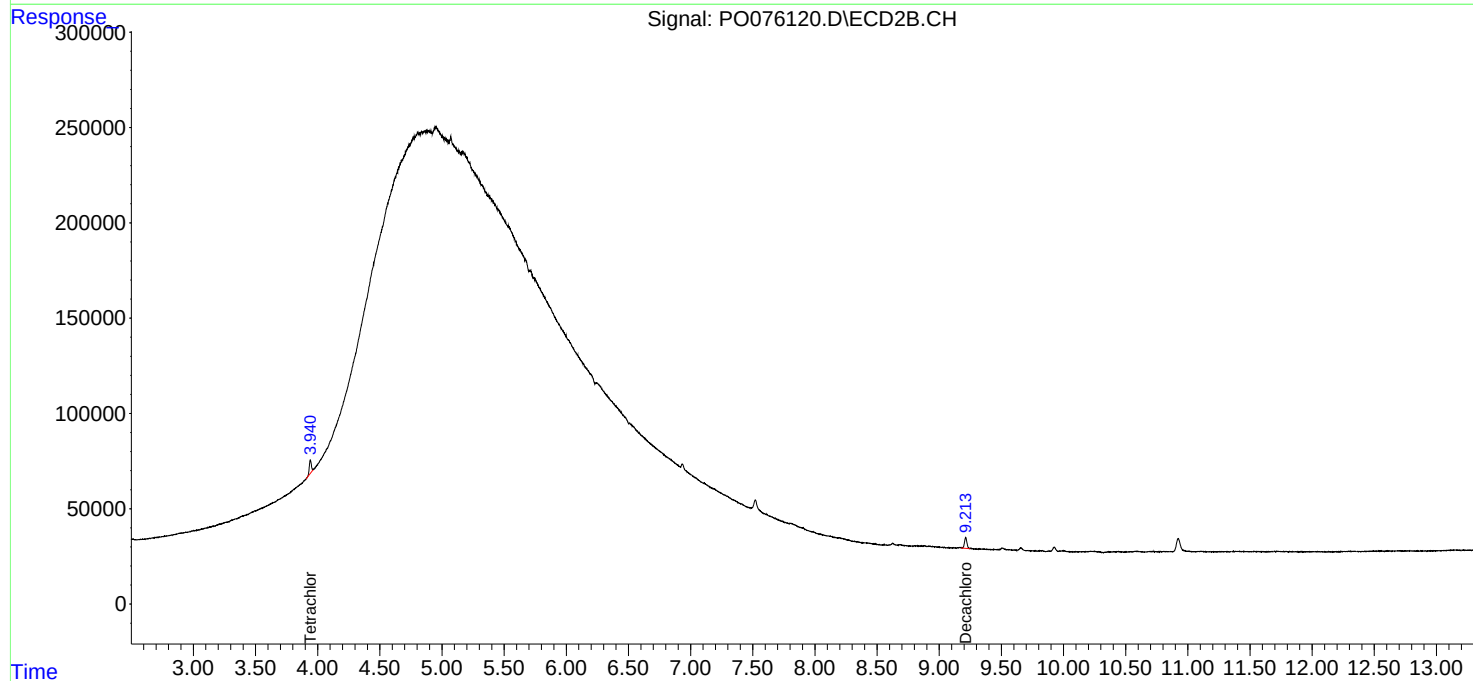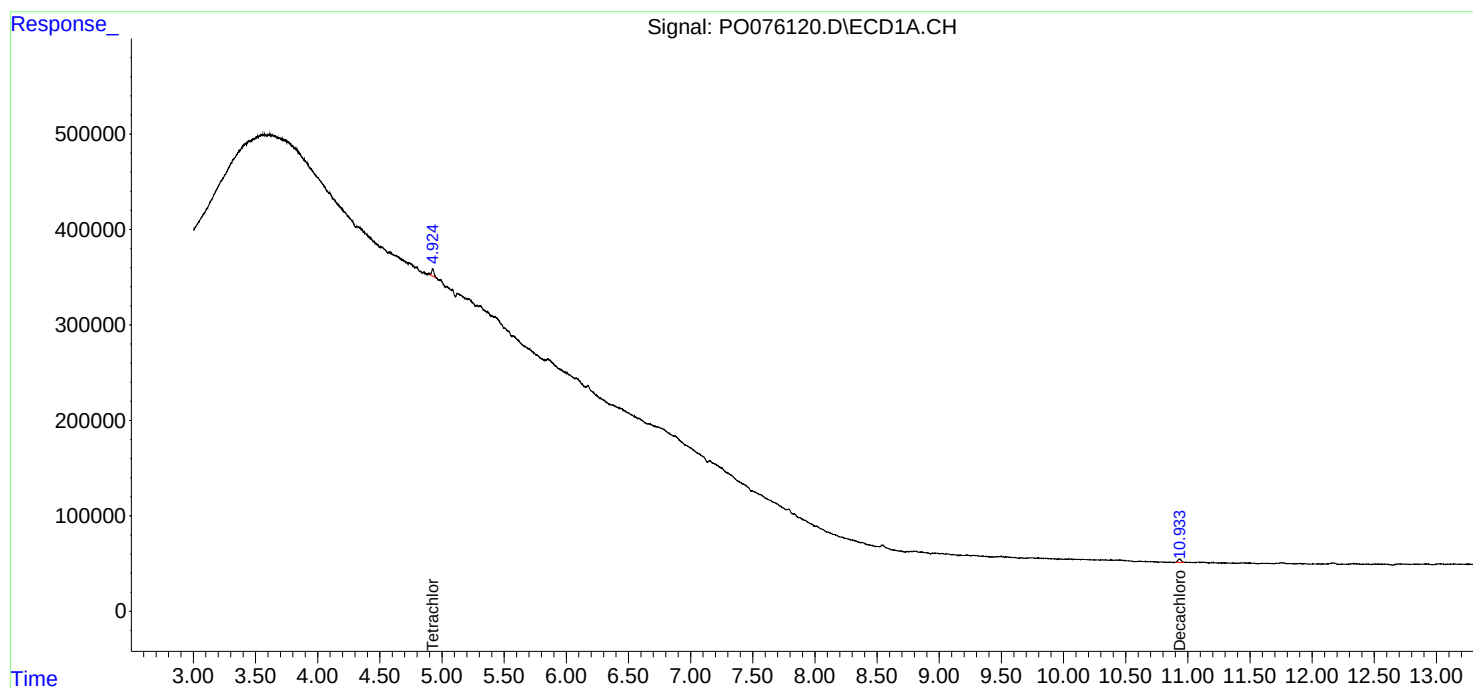

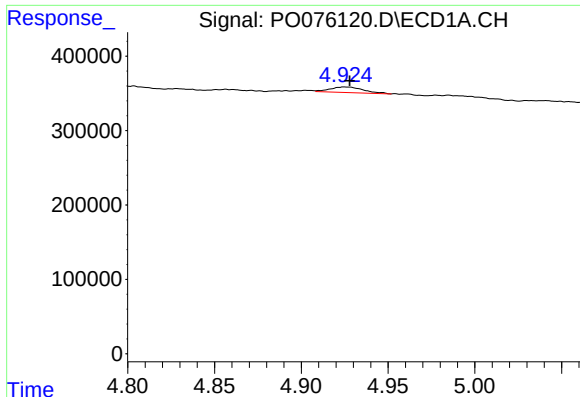


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: -0.003 min
Response: 99967
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
JEH585T-END-2


Manual Integrations
APPROVED

Ankita
3/15/2021 1:08:07 PM

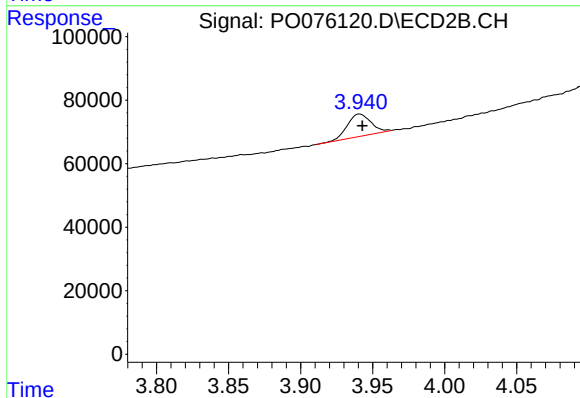


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 80421
Conc: 1.80 ng/ml

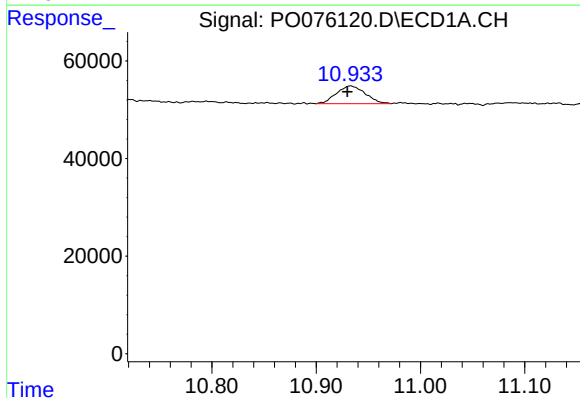

#2 Decachlorobiphenyl

R.T.: 10.933 min
Delta R.T.: 0.003 min
Response: 70243
Conc: 2.14 ng/ml

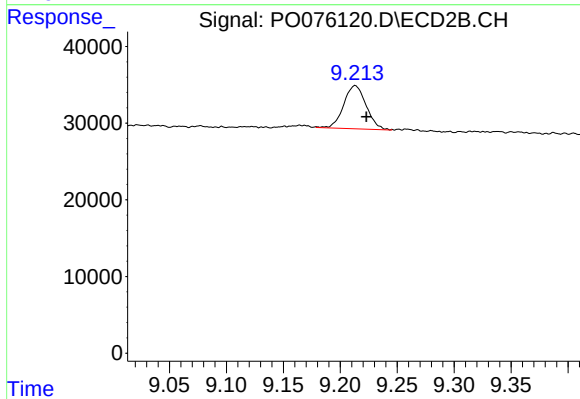

#2 Decachlorobiphenyl

R.T.: 9.213 min
Delta R.T.: -0.010 min
Response: 77317
Conc: 2.13 ng/ml m