

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
 Data File : P0076140.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Mar 2021 8:10
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:28:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 09:12:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 08:07:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.941	2772497	2011702	46.513	45.097
2) SA Decachlor...	10.926	9.206	1846558	1695221	56.209	46.622
Target Compounds						
21) L5 AR-1248-1	6.246	5.187	499745	380698	458.478	412.537m
22) L5 AR-1248-2	6.541	5.447	678829	771448	432.931	539.185
23) L5 AR-1248-3	6.759	5.491	755980	726523	420.871	493.387
24) L5 AR-1248-4	7.188	5.674	817552	688666	427.899	407.642
25) L5 AR-1248-5	7.228	6.097	854356	788320	451.266	472.962

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031321\
Data File : P0076140.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Mar 2021 8:10
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/16/2021 11:28:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 09:12:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 08:07:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

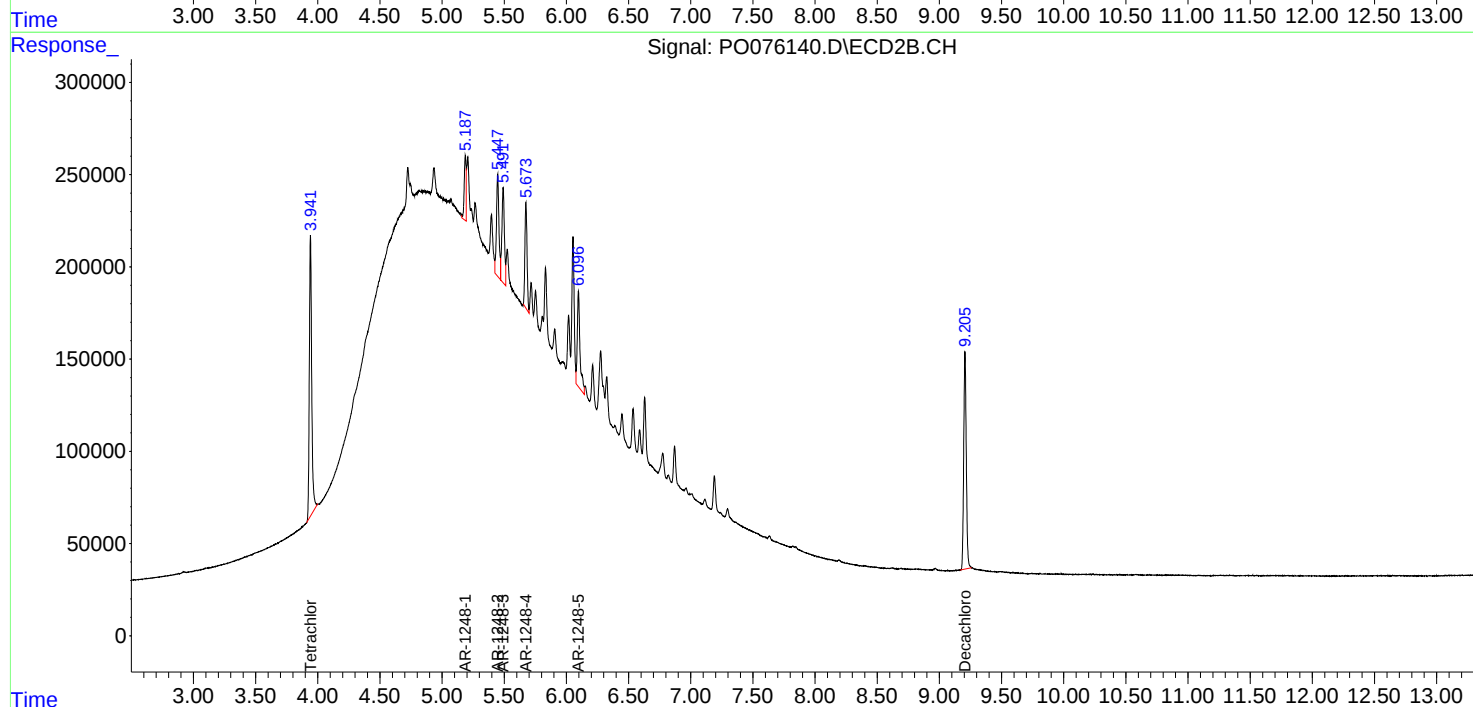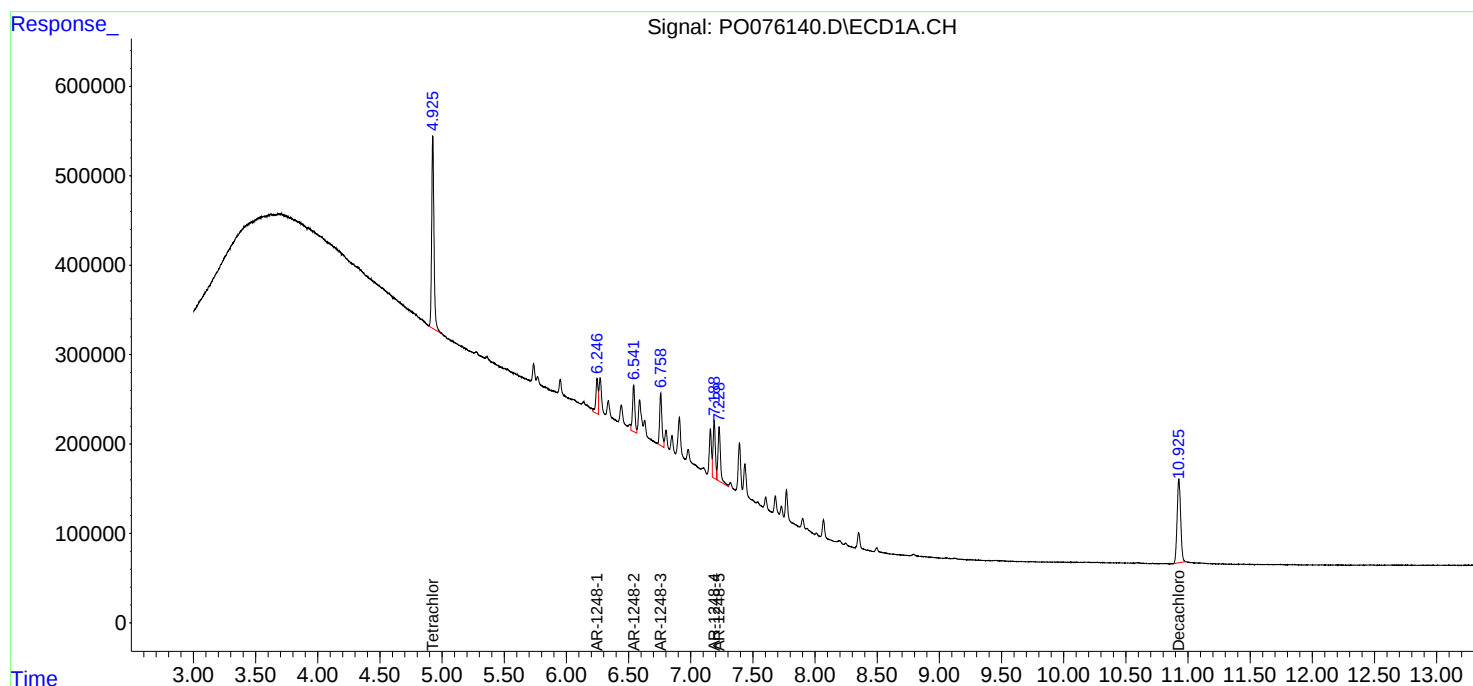

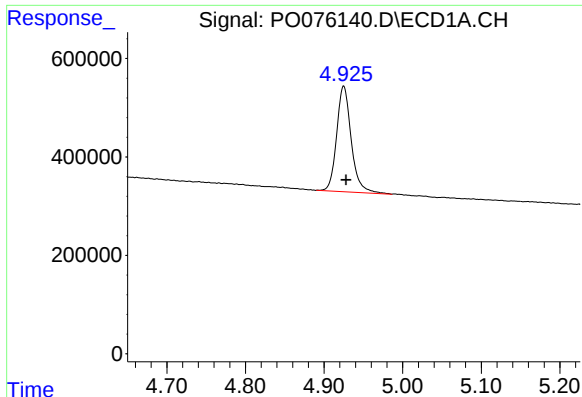


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: -0.003 min
Response: 2772497
Conc: 46.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/16/2021 11:28:38 AM

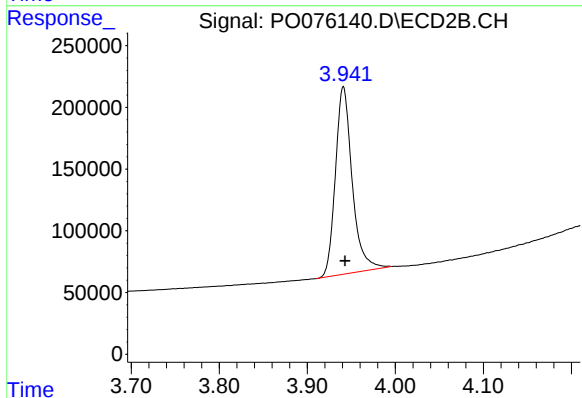


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 2011702
Conc: 45.10 ng/ml

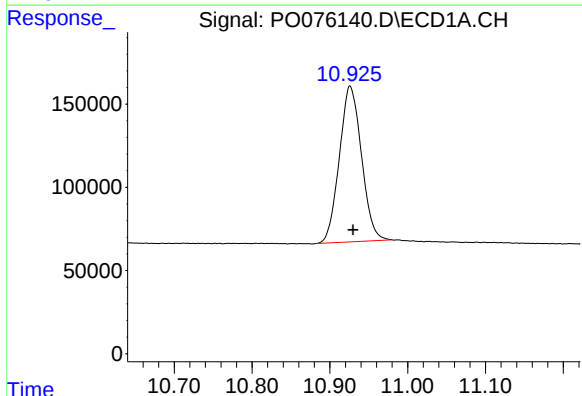


#2 Decachlorobiphenyl

R.T.: 10.926 min
Delta R.T.: -0.004 min
Response: 1846558
Conc: 56.21 ng/ml

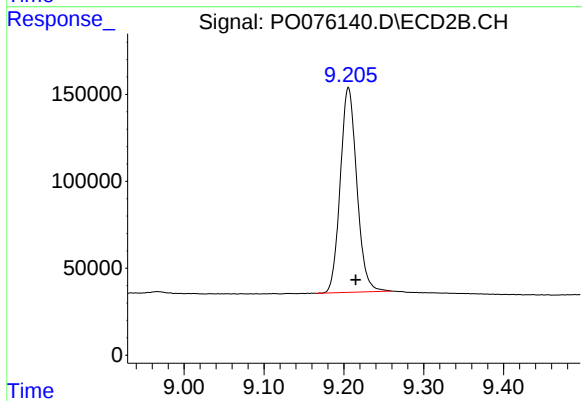

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.009 min
Response: 1695221
Conc: 46.62 ng/ml

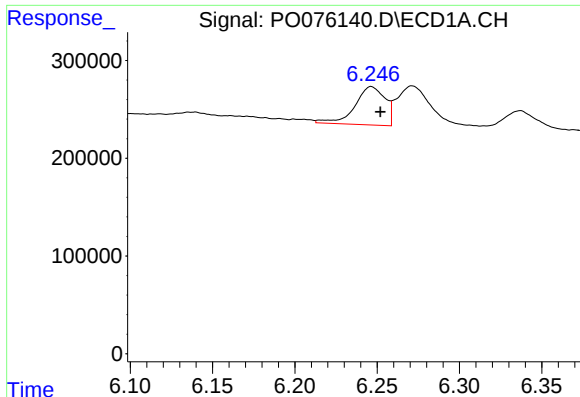


#21 AR-1248-1

R.T.: 6.246 min
Delta R.T.: -0.006 min
Response: 499745
Conc: 458.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/16/2021 11:28:38 AM

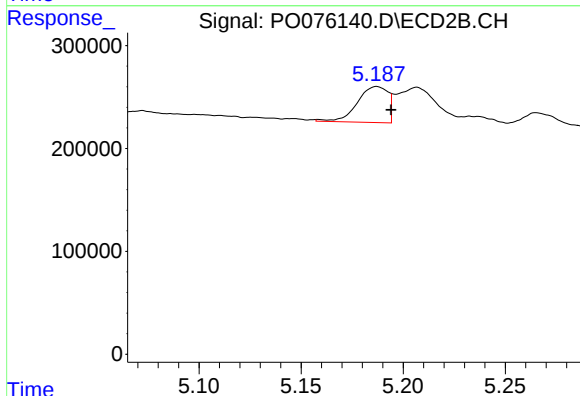


#21 AR-1248-1

R.T.: 5.187 min
Delta R.T.: -0.007 min
Response: 380698
Conc: 412.54 ng/ml m

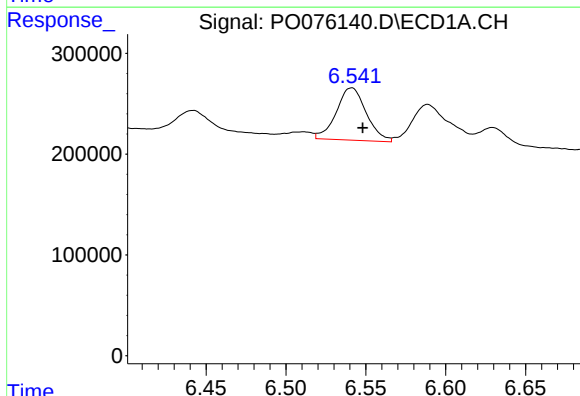


#22 AR-1248-2

R.T.: 6.541 min
Delta R.T.: -0.007 min
Response: 678829
Conc: 432.93 ng/ml

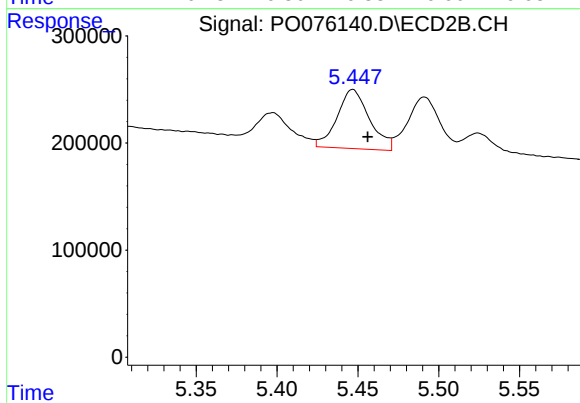

#22 AR-1248-2

R.T.: 5.447 min
Delta R.T.: -0.009 min
Response: 771448
Conc: 539.19 ng/ml

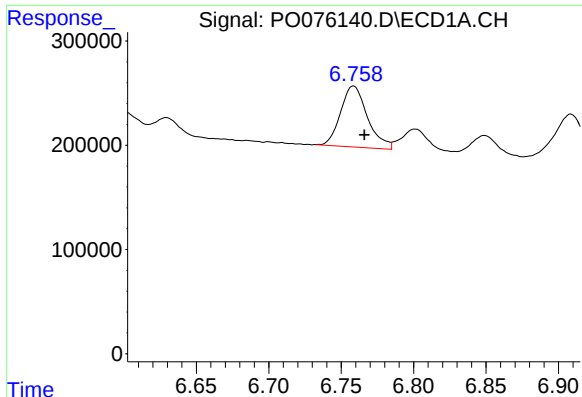


#23 AR-1248-3

R.T.: 6.759 min
Delta R.T.: -0.007 min
Response: 755980
Conc: 420.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/16/2021 11:28:38 AM

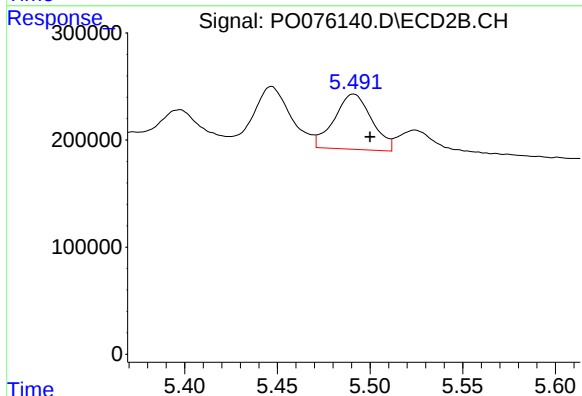


#23 AR-1248-3

R.T.: 5.491 min
Delta R.T.: -0.009 min
Response: 726523
Conc: 493.39 ng/ml

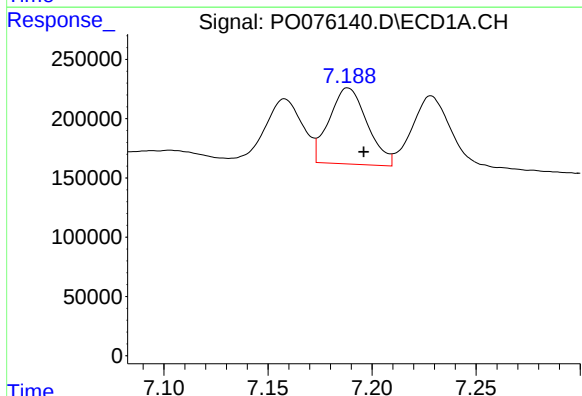


#24 AR-1248-4

R.T.: 7.188 min
Delta R.T.: -0.008 min
Response: 817552
Conc: 427.90 ng/ml

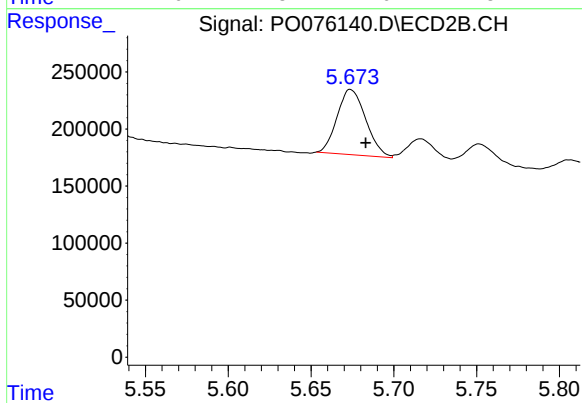

#24 AR-1248-4

R.T.: 5.674 min
Delta R.T.: -0.009 min
Response: 688666
Conc: 407.64 ng/ml

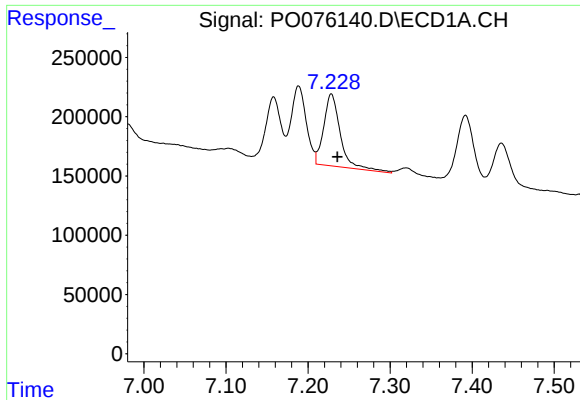


#25 AR-1248-5

R.T.: 7.228 min
Delta R.T.: -0.008 min
Response: 854356
Conc: 451.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/16/2021 11:28:38 AM

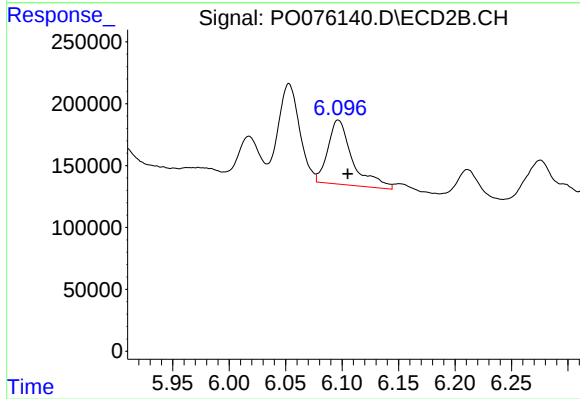

#25 AR-1248-5

R.T.: 6.097 min
Delta R.T.: -0.008 min
Response: 788320
Conc: 472.96 ng/ml