

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031324\
 Data File : P0102478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2024 20:04
 Operator : YP/AJ
 Sample : P1734-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/14/2024
 Supervised By :Ankita Jodhani 03/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 01:48:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 13 04:51:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.269	3.384	82003365	54638540	20.006m	19.500
2) SA Decachlor...	9.811	8.250	40818214	28498678	21.496	23.116

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031324\
Data File : PO102478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2024 20:04
Operator : YP/AJ
Sample : P1734-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2024
Supervised By :Ankita Jodhani 03/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 01:48:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031224.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 13 04:51:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

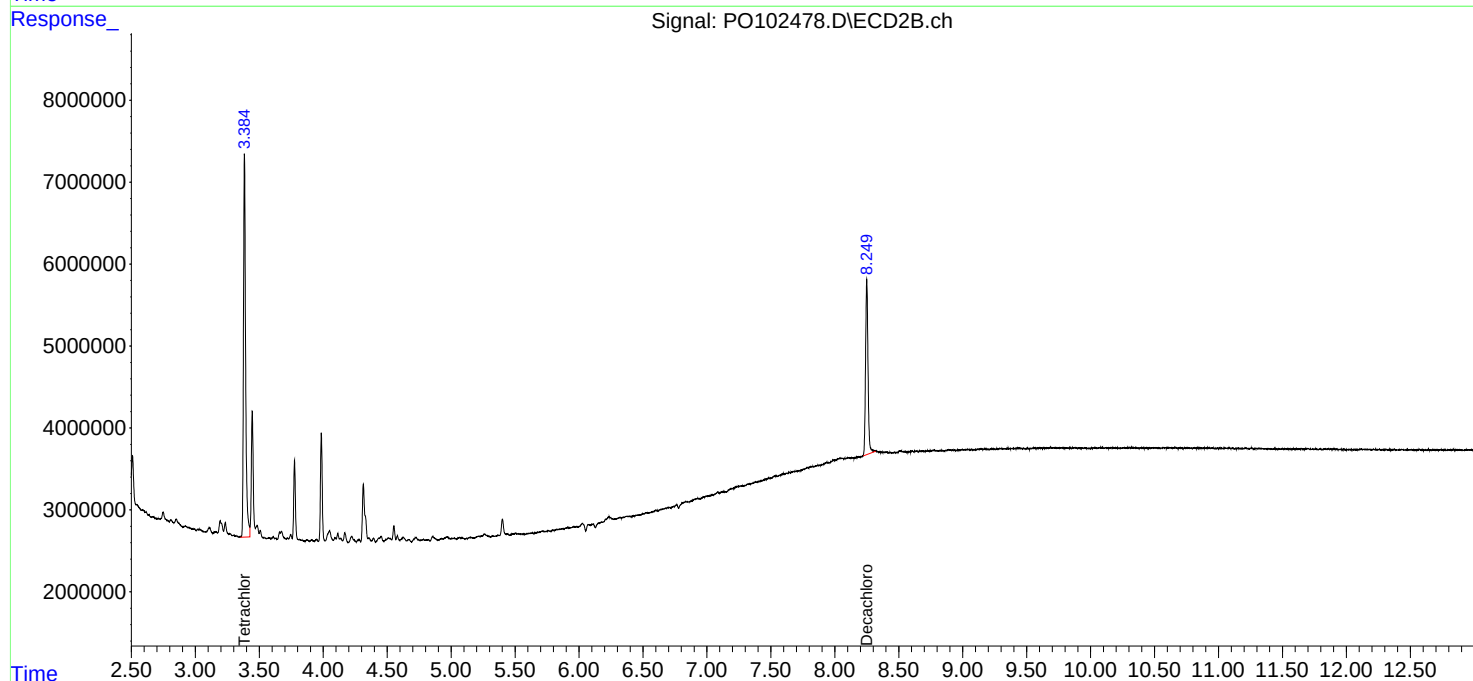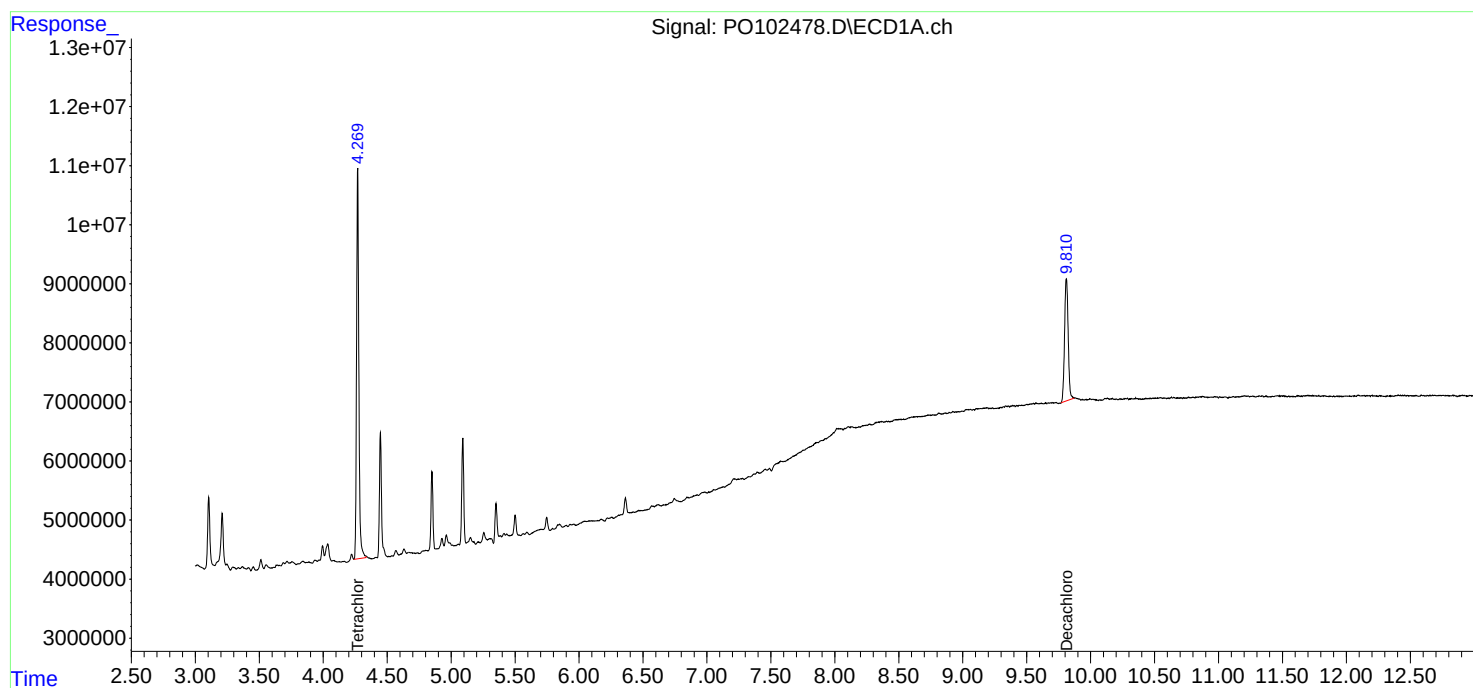

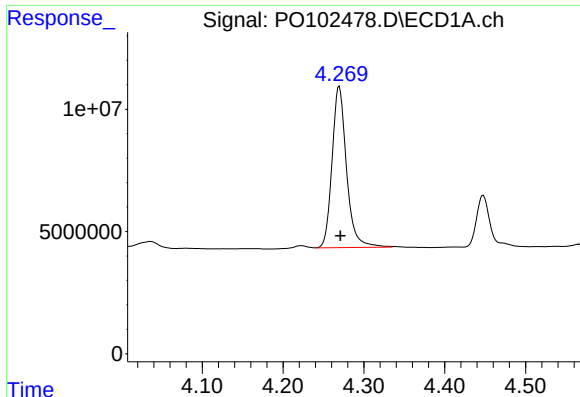


#1 Tetrachloro-m-xylene

R.T.: 4.269 min
Delta R.T.: -0.002 min
Response: 82003365
Conc: 20.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2024
Supervised By :Ankita Jodhani 03/14/2024

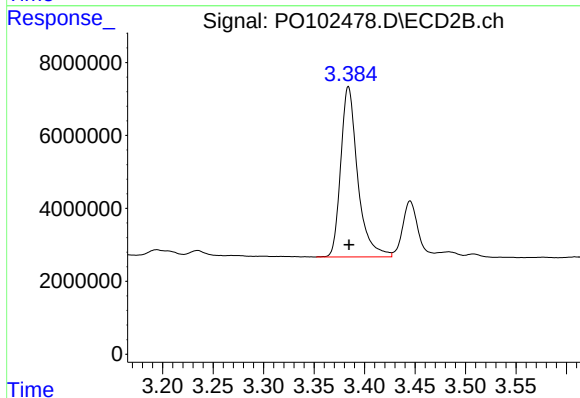


#1 Tetrachloro-m-xylene

R.T.: 3.384 min
Delta R.T.: 0.000 min
Response: 54638540
Conc: 19.50 ng/ml

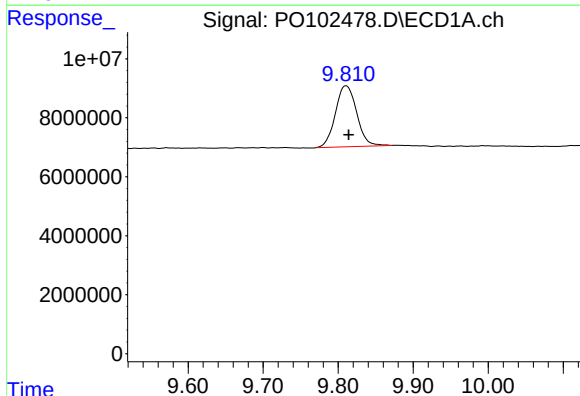

#2 Decachlorobiphenyl

R.T.: 9.811 min
Delta R.T.: -0.003 min
Response: 40818214
Conc: 21.50 ng/ml

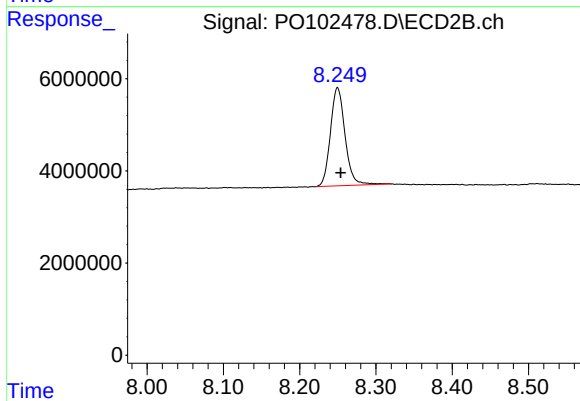

#2 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: -0.004 min
Response: 28498678
Conc: 23.12 ng/ml