

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031325\
 Data File : P0109834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2025 09:27
 Operator : YP/AJ
 Sample : Q1554-09 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC122669LOK-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/14/2025
 Supervised By :Ankita Jodhani 03/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 11:21:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.692	3.690	13069157	7568517	1.381m	1.446m
2) SA Decachlor...	8.746	8.698	15224056	5587586	1.770	1.755

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031325\
Data File : PO109834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2025 09:27
Operator : YP/AJ
Sample : Q1554-09 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC122669LOK-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2025
Supervised By :Ankita Jodhani 03/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 11:21:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

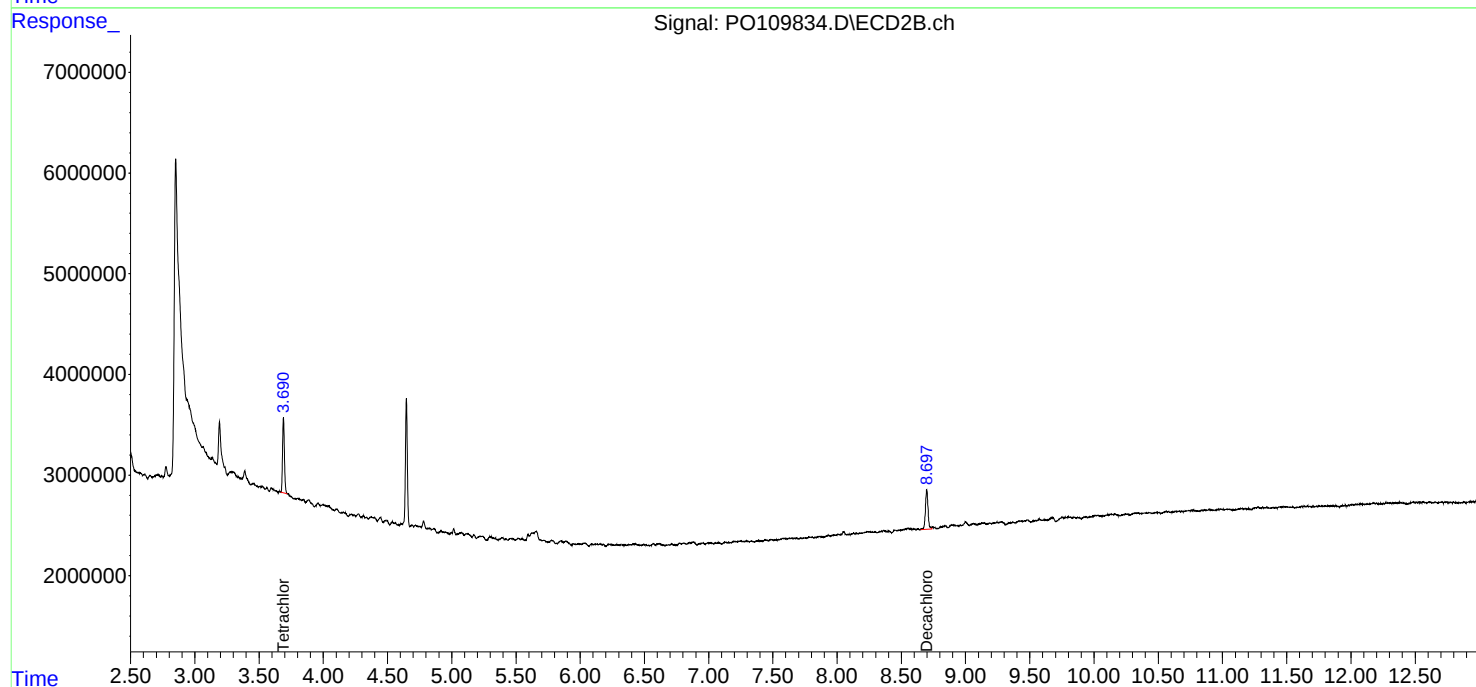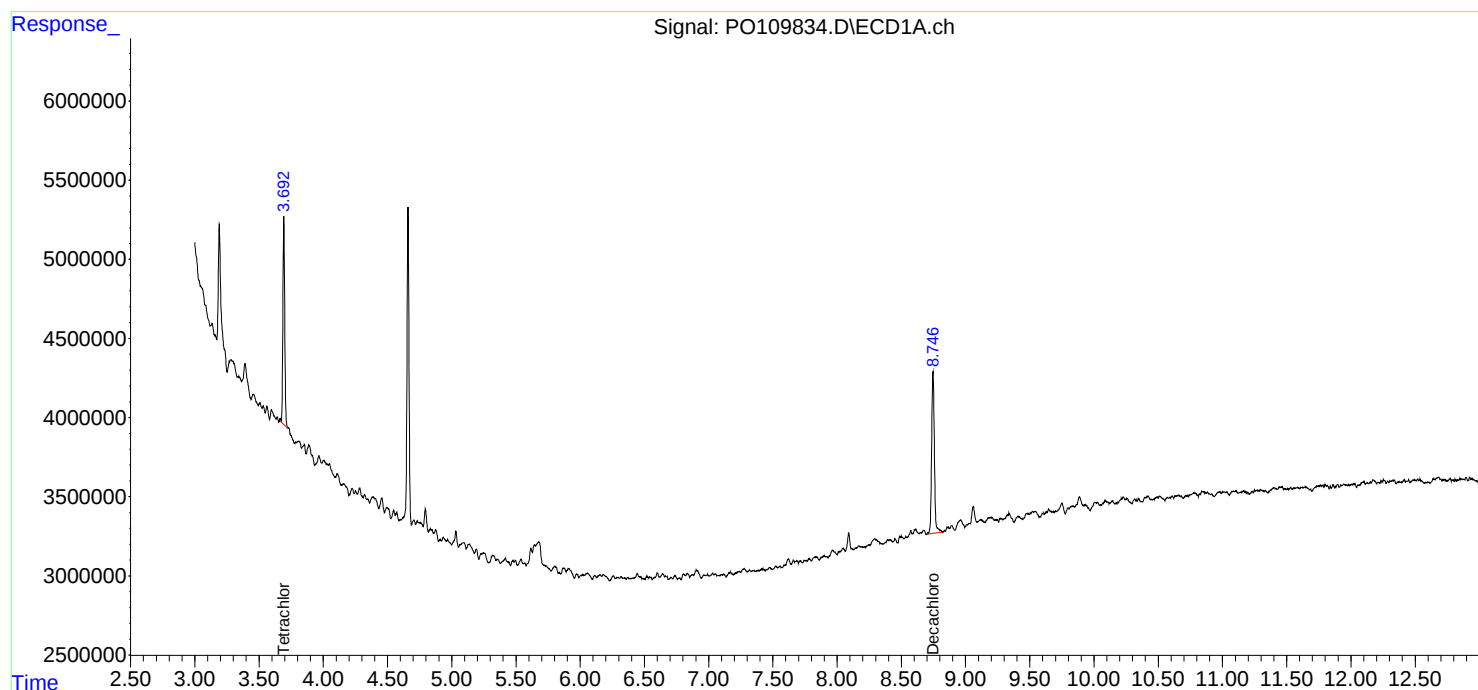

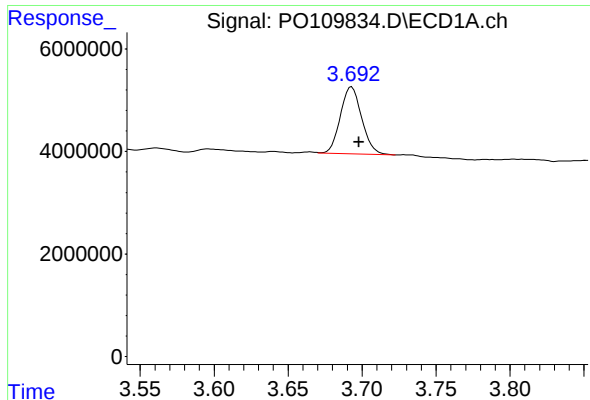


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: -0.006 min
Response: 13069157
Conc: 1.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC122669LOK-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/14/2025
Supervised By :Ankita Jodhani 03/14/2025

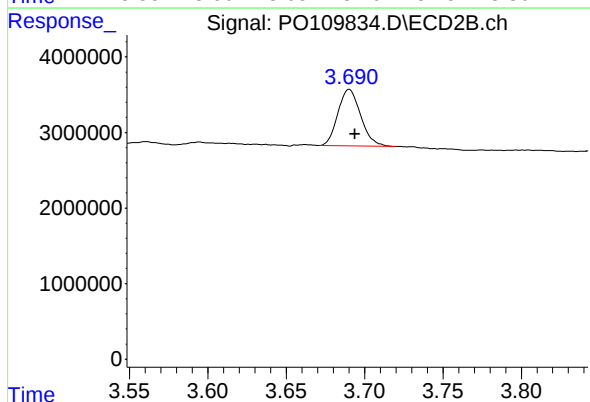


#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: -0.004 min
Response: 7568517
Conc: 1.45 ng/ml

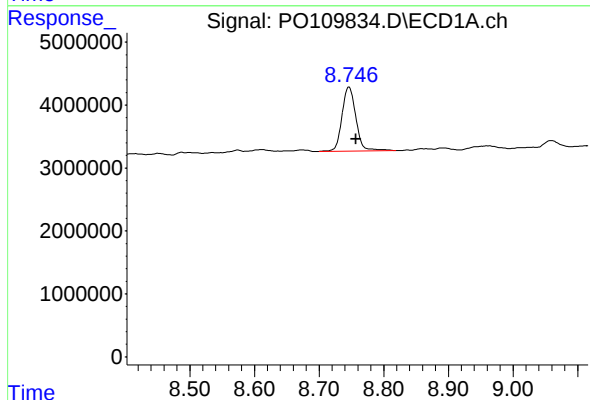

#2 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.010 min
Response: 15224056
Conc: 1.77 ng/ml

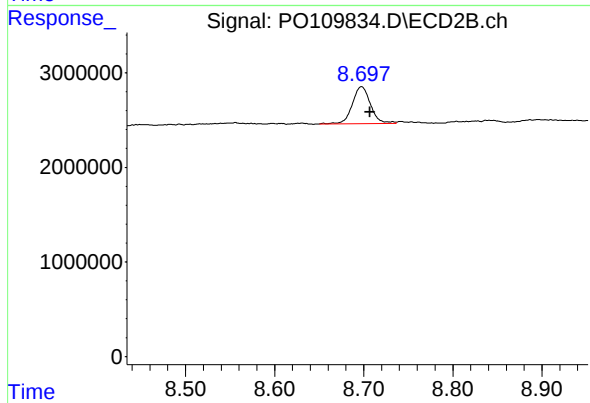

#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.009 min
Response: 5587586
Conc: 1.75 ng/ml