

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031419\
 Data File : P0054367.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Mar 2019 8:22
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 14:34:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 14 14:30:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.016	3.105	107.8E6	5405952	21.894	21.276
2) SA Decachlor...	9.324	7.667	29897825	6487748	21.703	21.937

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031419\
Data File : P0054367.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Mar 2019 8:22
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 14:34:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 14 14:30:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

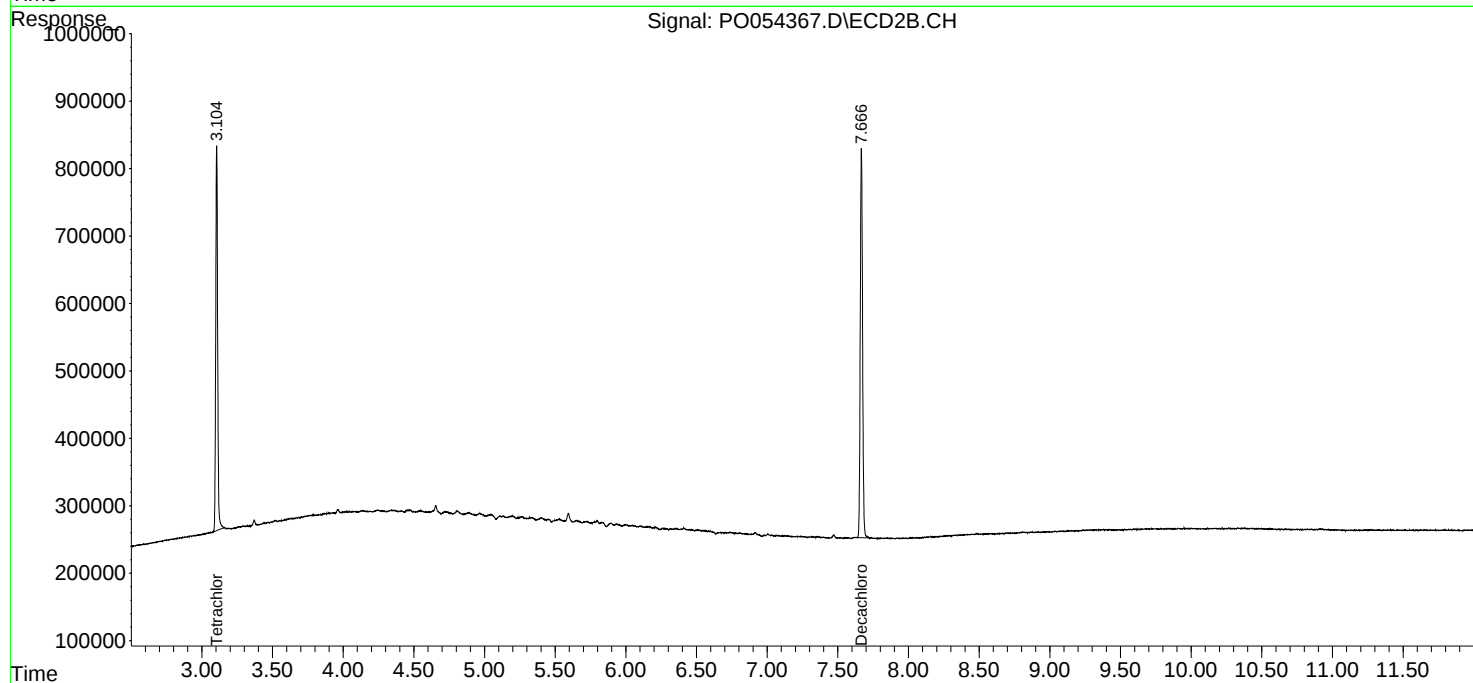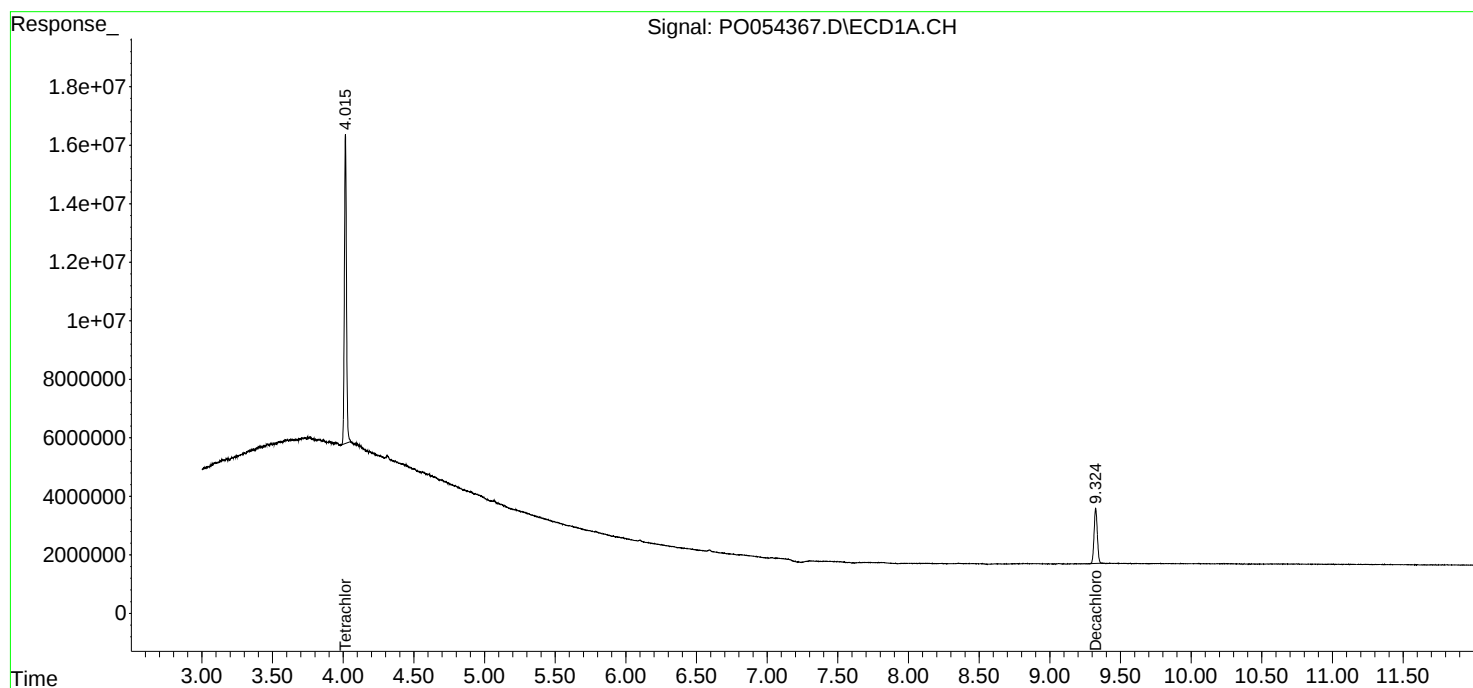


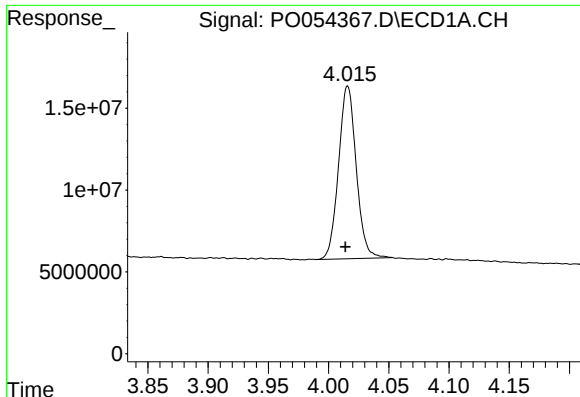

#1 Tetrachloro-m-xylene


R.T.: 4.016 min
Delta R.T.: 0.002 min
Response: 107824551
Conc: 21.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

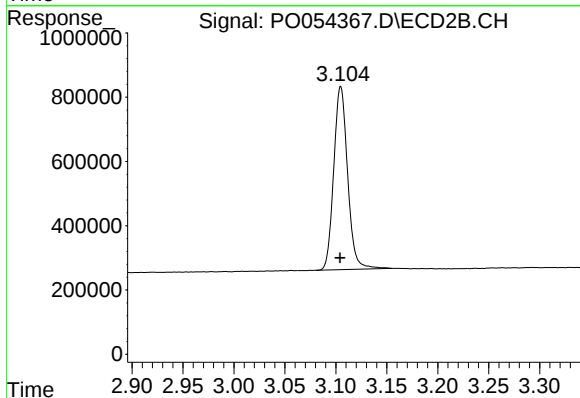


#1 Tetrachloro-m-xylene

R.T.: 3.105 min
Delta R.T.: 0.000 min
Response: 5405952
Conc: 21.28 ng/ml

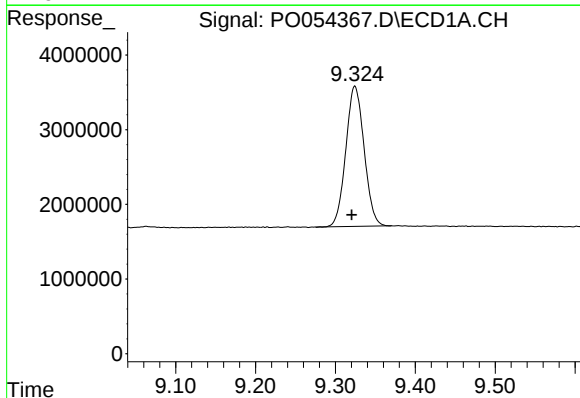

#2 Decachlorobiphenyl

R.T.: 9.324 min
Delta R.T.: 0.004 min
Response: 29897825
Conc: 21.70 ng/ml

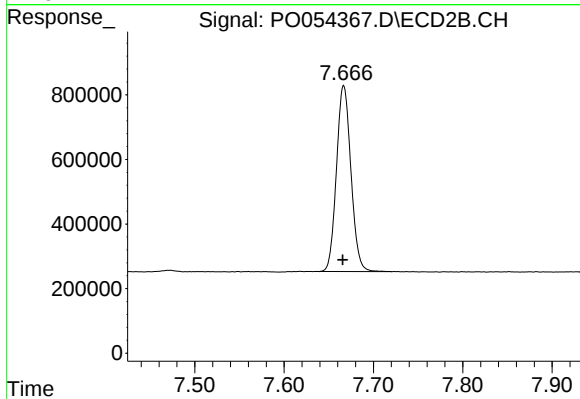

#2 Decachlorobiphenyl

R.T.: 7.667 min
Delta R.T.: 0.001 min
Response: 6487748
Conc: 21.94 ng/ml