

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031423\
 Data File : P0093102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 14:09
 Operator : YP/AJ
 Sample : 01895-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 103122

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/15/2023
 Supervised By :Ankita Jodhani 03/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 21:35:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.431	3.637	6255552	1973175	1.998	1.749m
2) SA Decachlor...	10.275	8.673	5837645	3523653	2.697	3.599 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031423\
Data File : PO093102.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 14:09
Operator : YP/AJ
Sample : 01895-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
103122


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2023
Supervised By :Ankita Jodhani 03/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 21:35:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

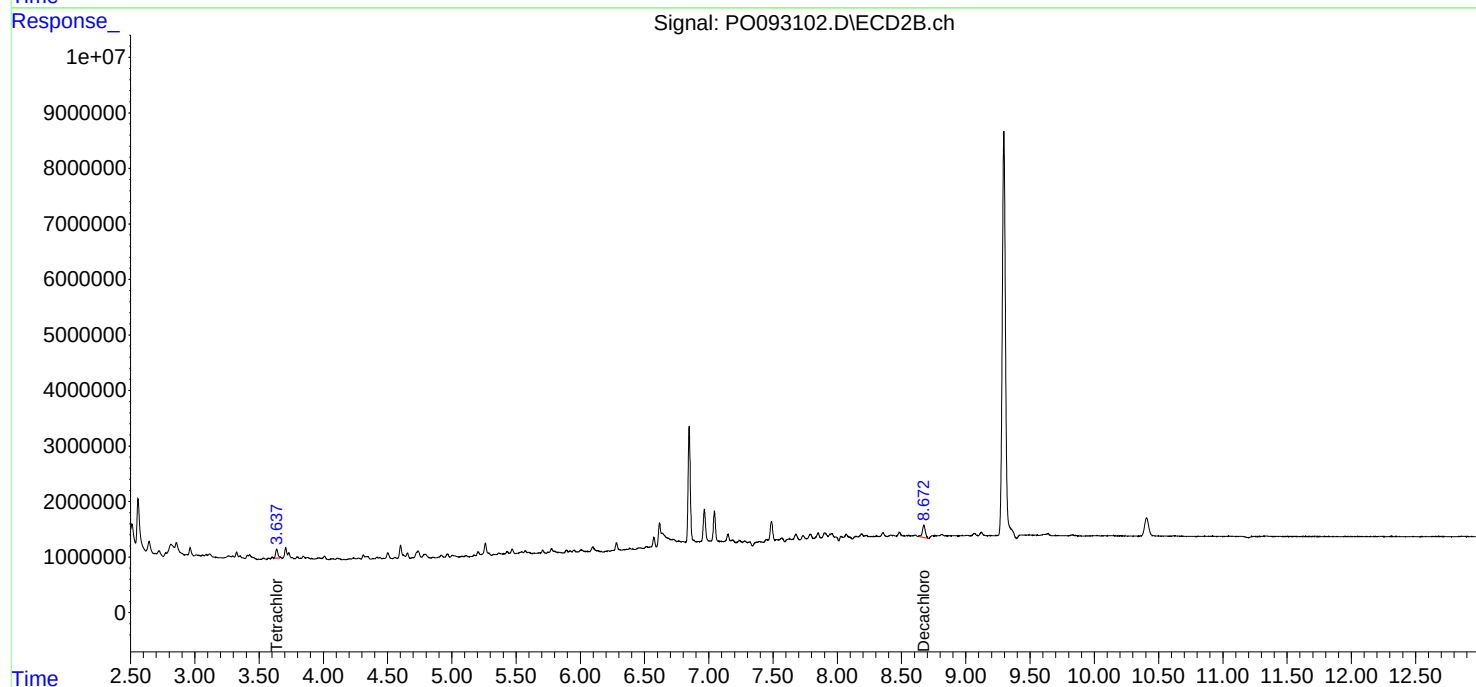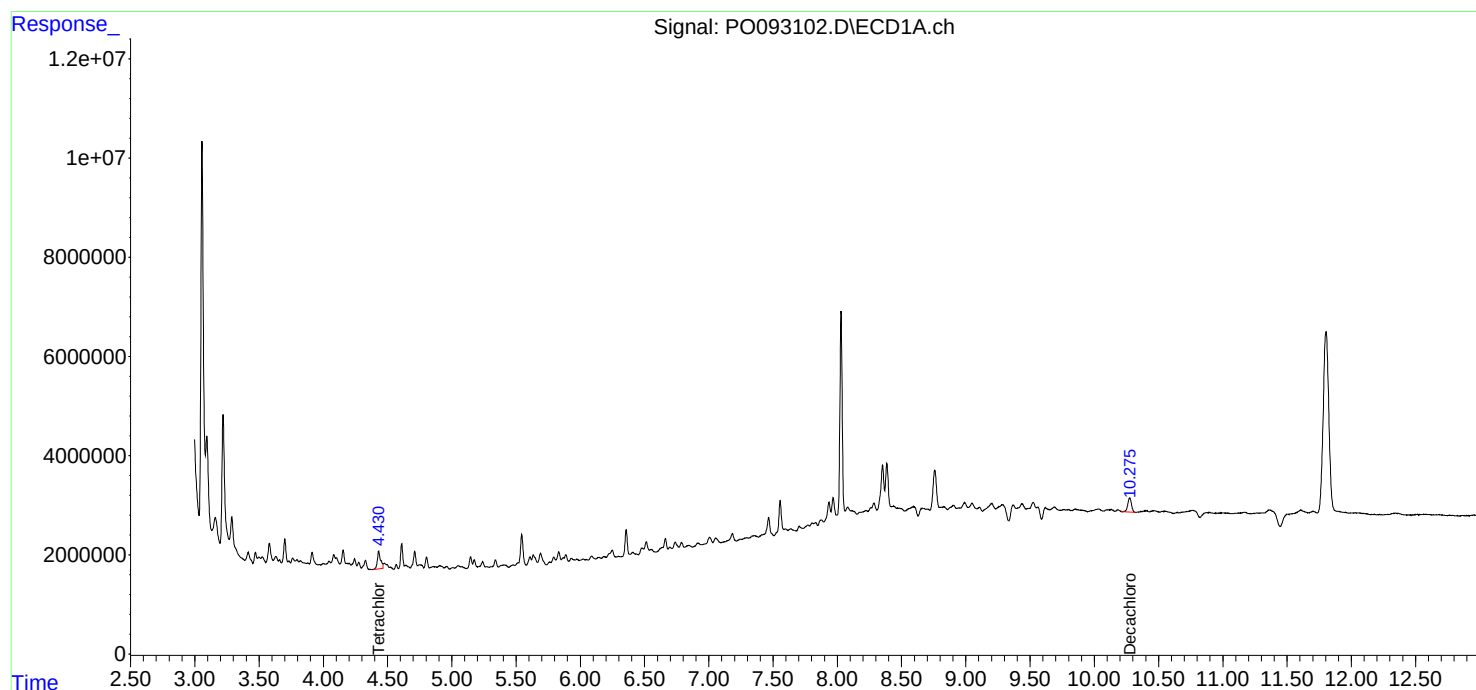

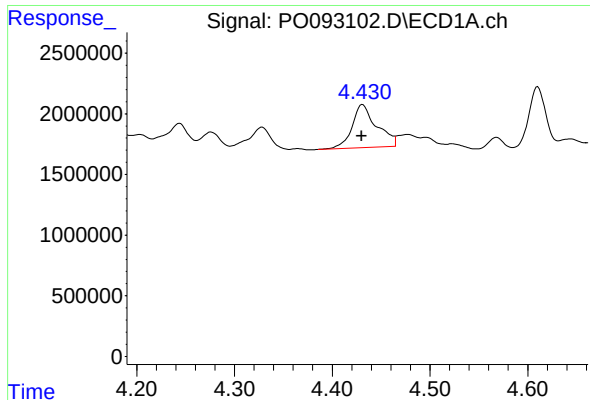


#1 Tetrachloro-m-xylene

R.T.: 4.431 min
Delta R.T.: 0.001 min
Response: 6255552
Conc: 2.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
103122


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2023
Supervised By :Ankita Jodhani 03/15/2023

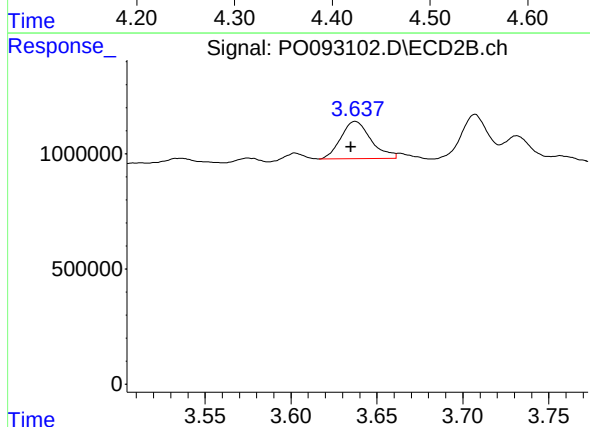


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: 0.002 min
Response: 1973175
Conc: 1.75 ng/ml

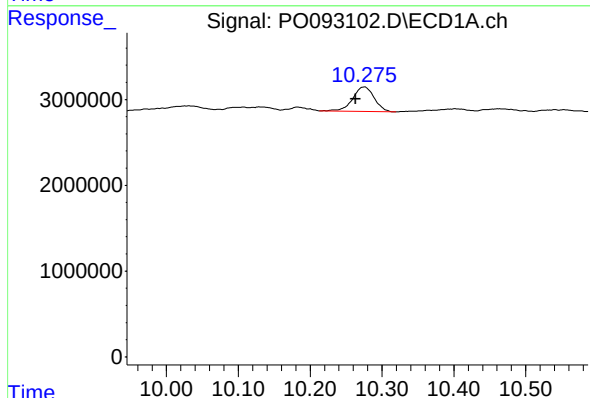

#2 Decachlorobiphenyl

R.T.: 10.275 min
Delta R.T.: 0.012 min
Response: 5837645
Conc: 2.70 ng/ml

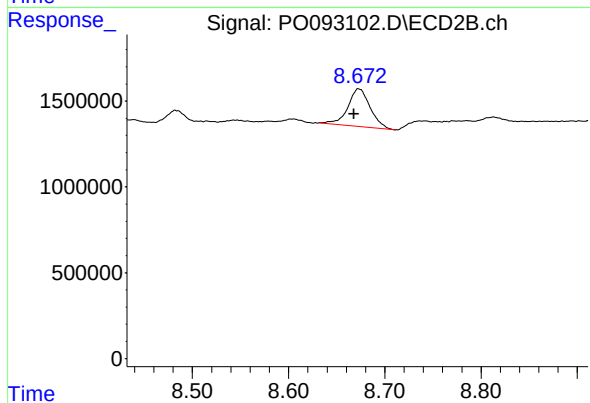

#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: 0.005 min
Response: 3523653
Conc: 3.60 ng/ml