

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031423\
 Data File : P0093103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2023 14:26
 Operator : YP/AJ
 Sample : 01898-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SAMPLE-1-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/15/2023
 Supervised By :Ankita Jodhani 03/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 21:36:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.431	3.636	67422451	22824675	21.530	20.237m
2) SA Decachlor...	10.272	8.672	45595231	21484635	21.067	21.942

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031423\
Data File : PO093103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2023 14:26
Operator : YP/AJ
Sample : 01898-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SAMPLE-1-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2023
Supervised By :Ankita Jodhani 03/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 21:36:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

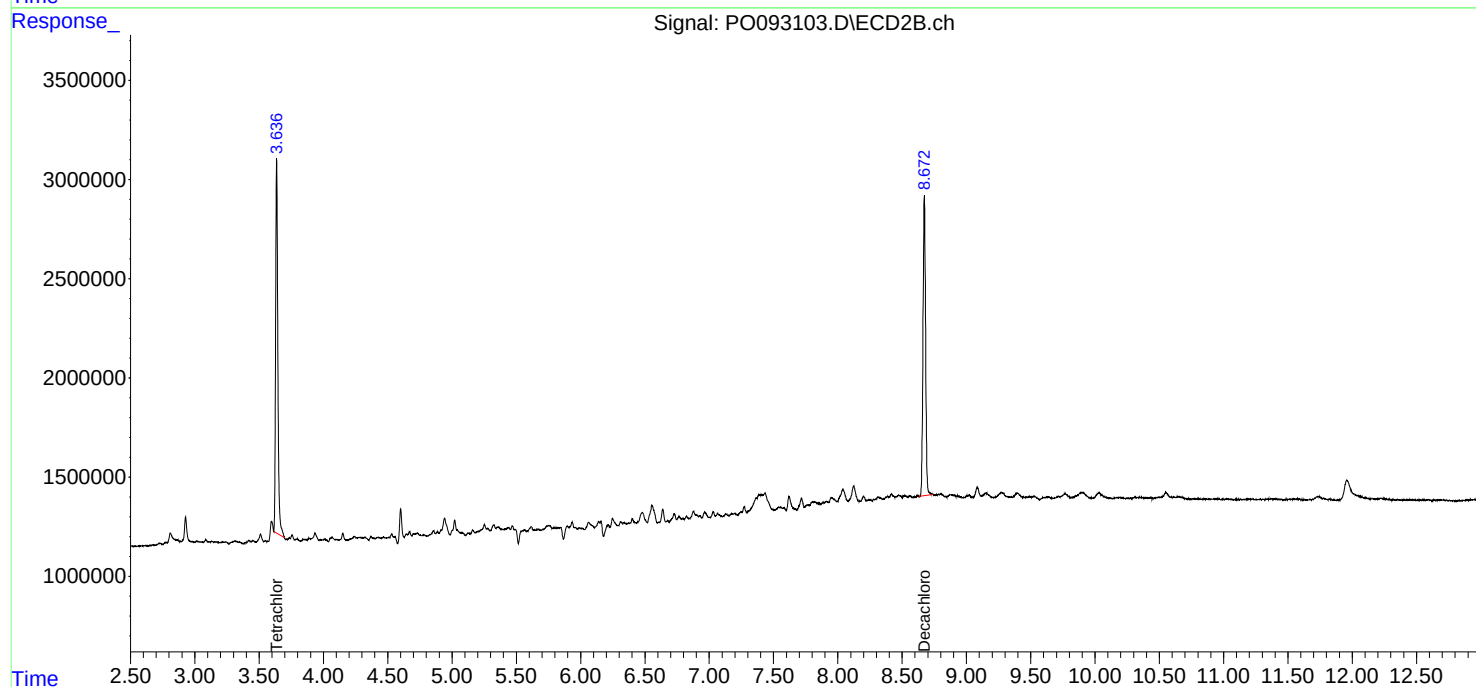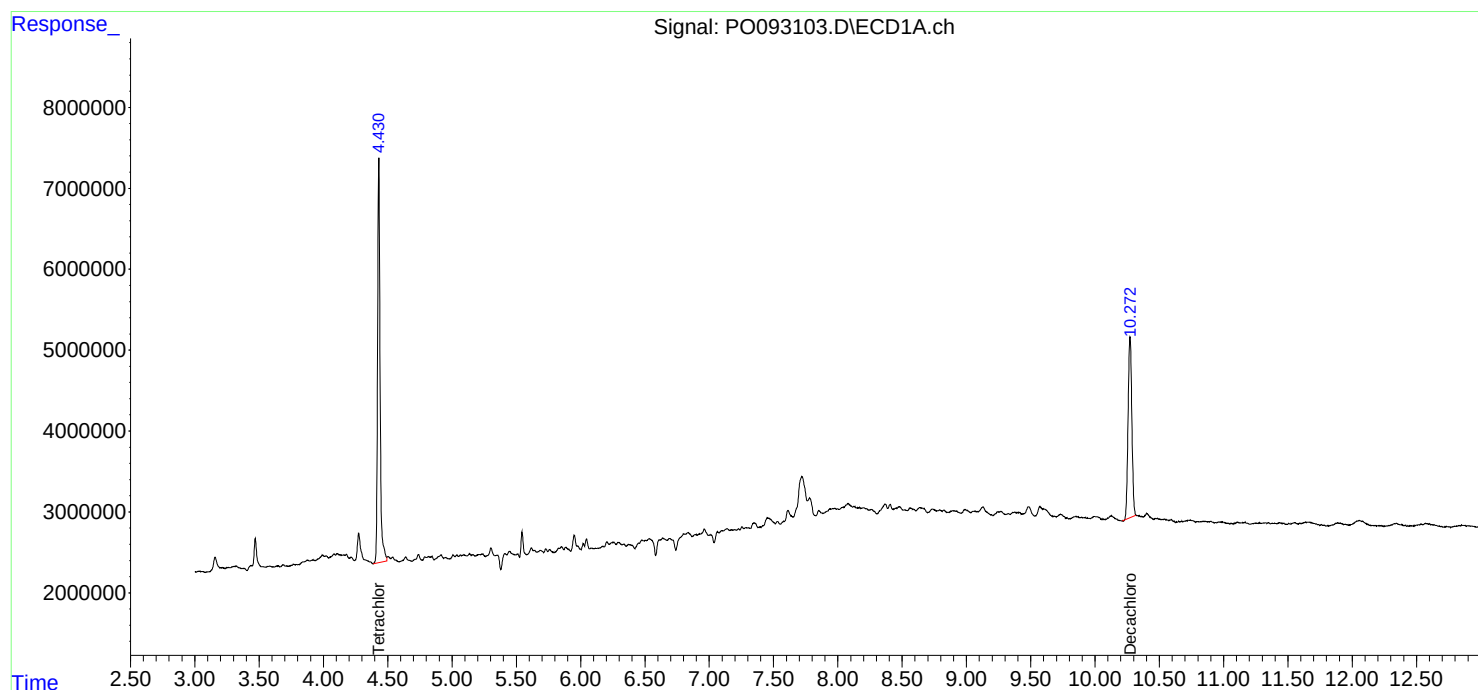

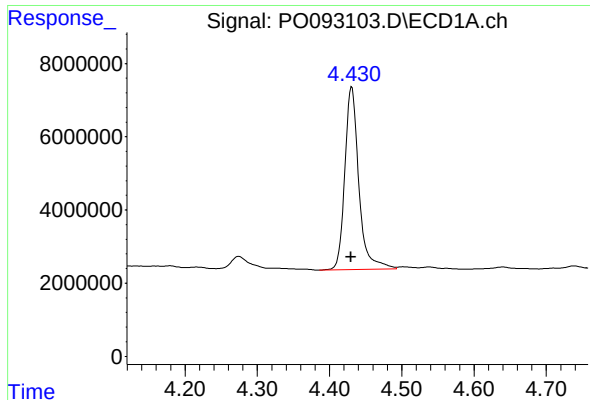


#1 Tetrachloro-m-xylene

R.T.: 4.431 min
Delta R.T.: 0.000 min
Response: 67422451
Conc: 21.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
SAMPLE-1-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2023
Supervised By :Ankita Jodhani 03/15/2023

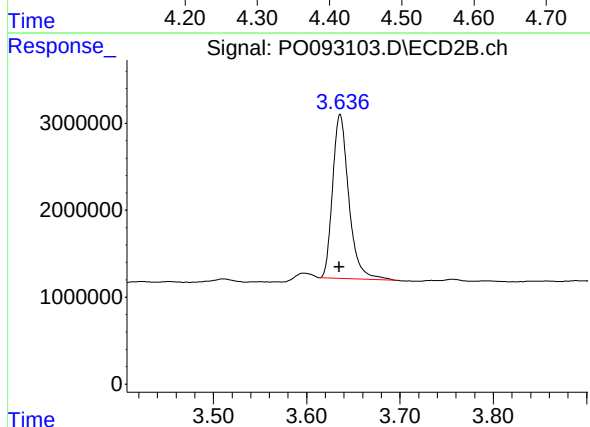


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 22824675
Conc: 20.24 ng/ml

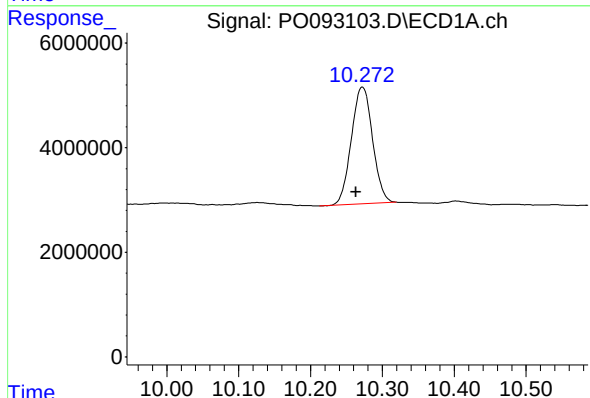

#2 Decachlorobiphenyl

R.T.: 10.272 min
Delta R.T.: 0.009 min
Response: 45595231
Conc: 21.07 ng/ml

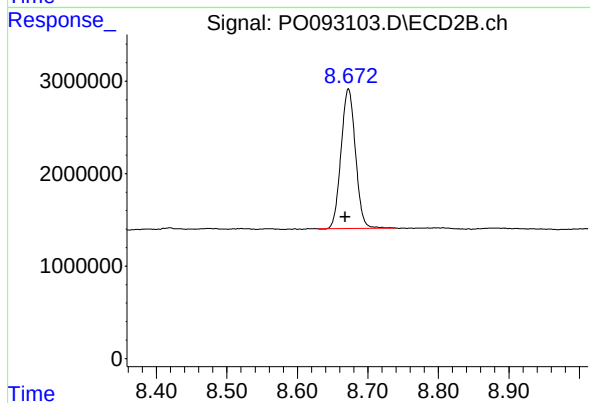

#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: 0.004 min
Response: 21484635
Conc: 21.94 ng/ml