

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031424\
 Data File : P0102497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2024 14:54
 Operator : YP/AJ
 Sample : P1746-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-01-4.0-6.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/15/2024
 Supervised By :Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 20:17:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 13 04:51:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.269	3.384	69888201	45560430	17.050	16.260m
2) SA Decachlor...	9.810	8.250	39199555	26140759	20.644	21.204

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031424\
Data File : PO102497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2024 14:54
Operator : YP/AJ
Sample : P1746-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-01-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2024
Supervised By :Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 20:17:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031224.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 13 04:51:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

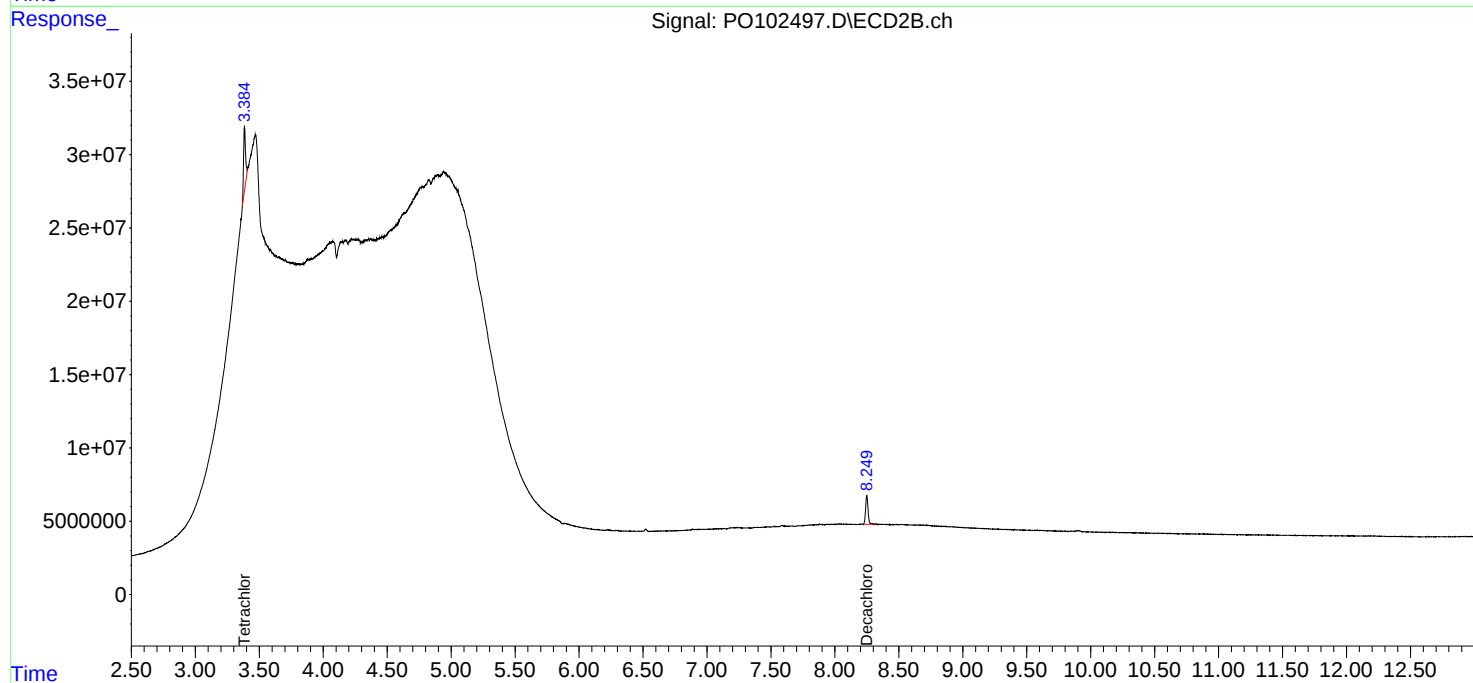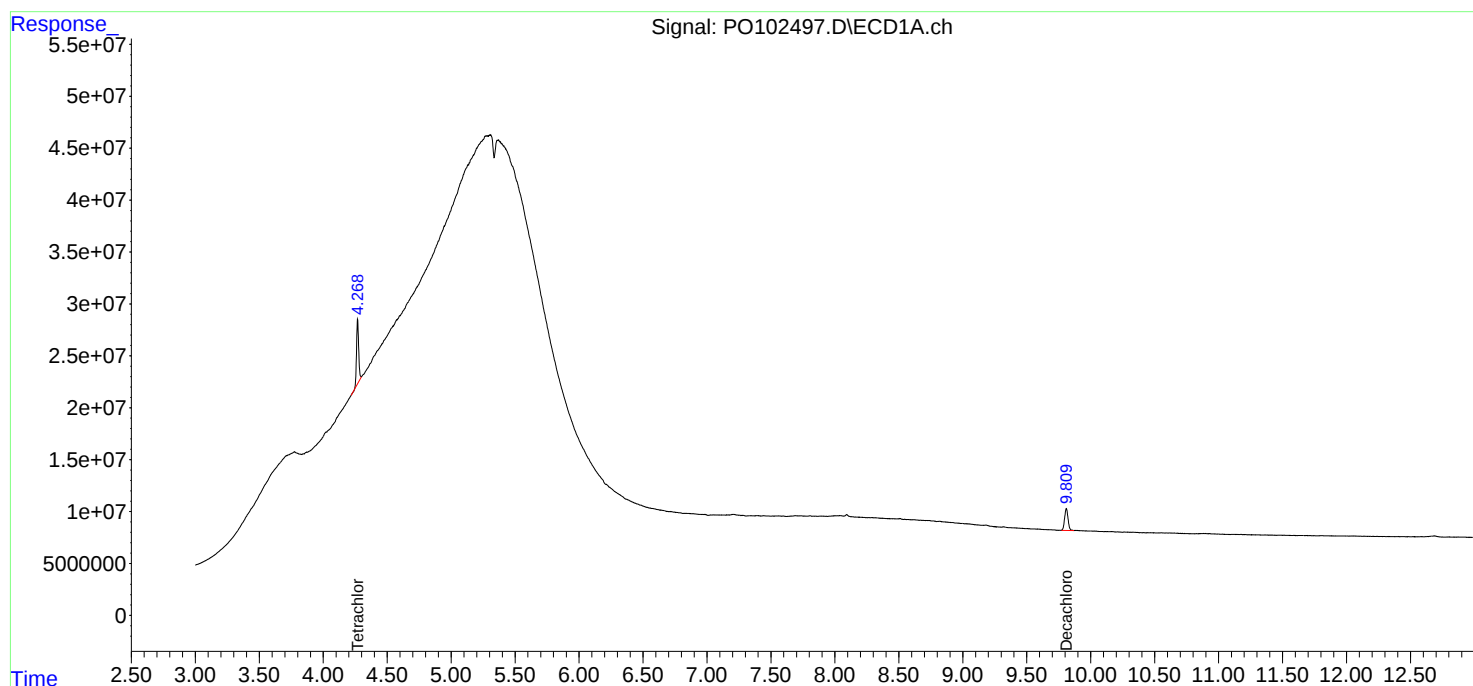

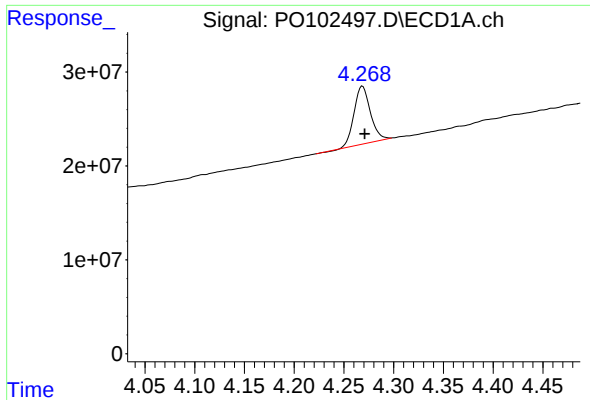


#1 Tetrachloro-m-xylene

R.T.: 4.269 min
Delta R.T.: -0.002 min
Response: 69888201
Conc: 17.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-4.0-6.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2024
Supervised By :Ankita Jodhani 03/15/2024

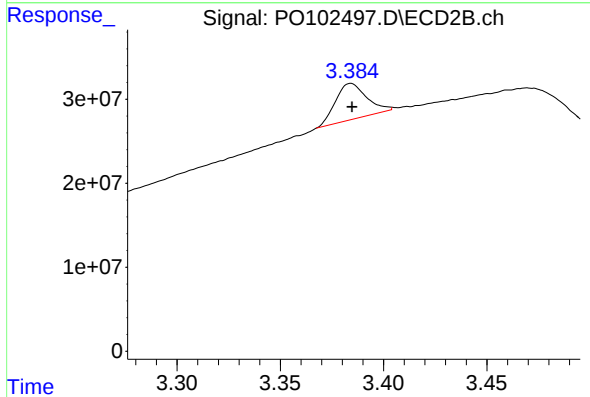


#1 Tetrachloro-m-xylene

R.T.: 3.384 min
Delta R.T.: -0.001 min
Response: 45560430
Conc: 16.26 ng/ml m

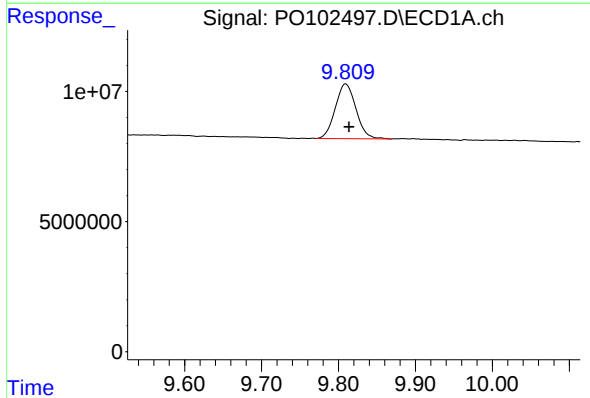

#2 Decachlorobiphenyl

R.T.: 9.810 min
Delta R.T.: -0.004 min
Response: 39199555
Conc: 20.64 ng/ml

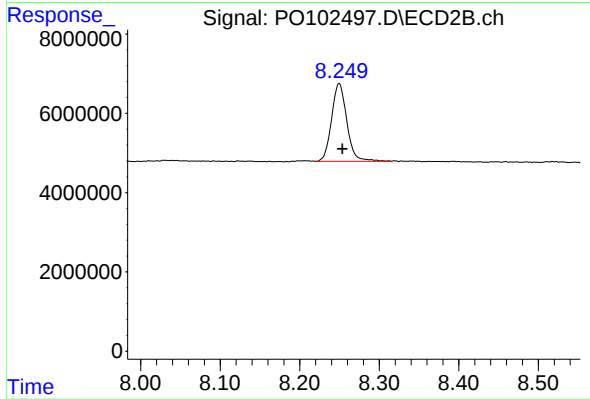

#2 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: -0.004 min
Response: 26140759
Conc: 21.20 ng/ml