

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031424\
 Data File : P0102503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2024 16:37
 Operator : YP/AJ
 Sample : P1746-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-03-0-2.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/15/2024
 Supervised By :Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 20:21:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 13 04:51:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.269	3.383	76910883	51875180	18.764	18.514
2) SA Decachlor...	9.809	8.248	34999196	23676129	18.432	19.205m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO031424\
Data File : PO102503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2024 16:37
Operator : YP/AJ
Sample : P1746-08
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-03-0-2.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2024
Supervised By :Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 20:21:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO031224.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 13 04:51:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

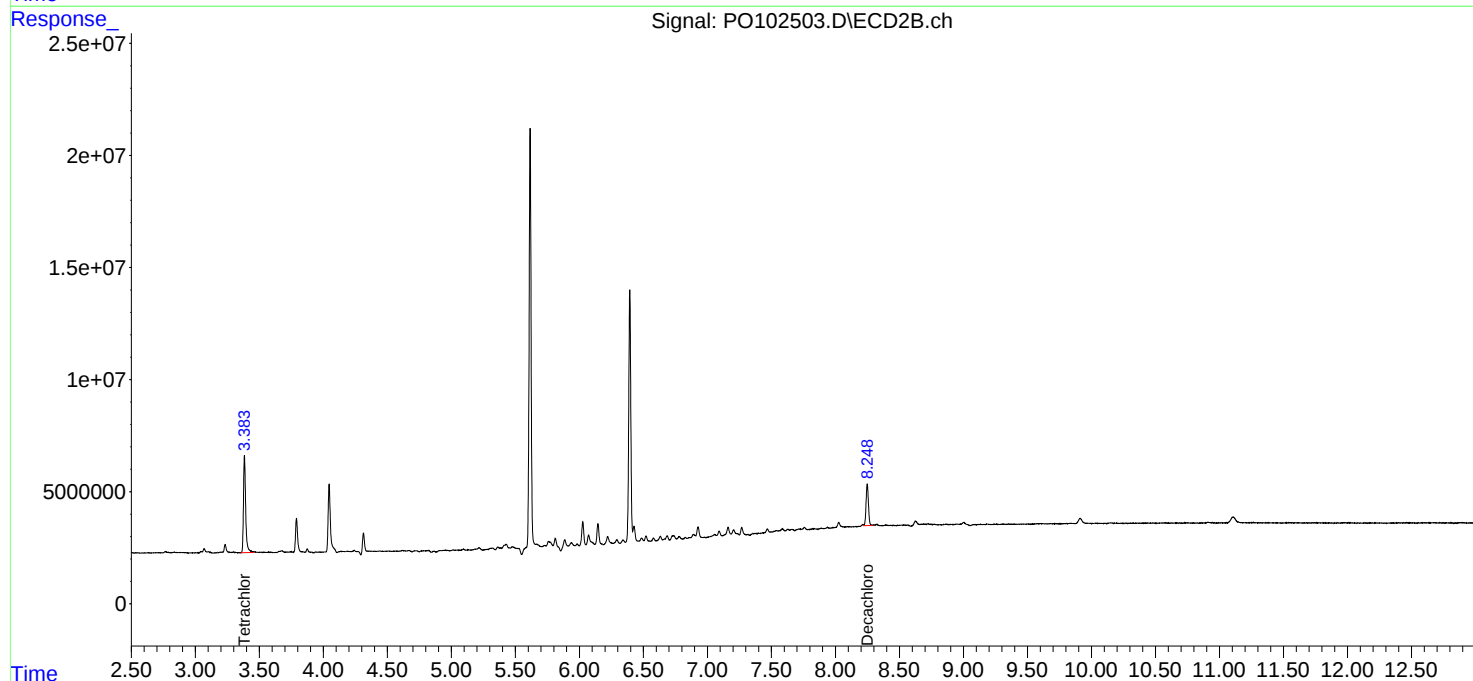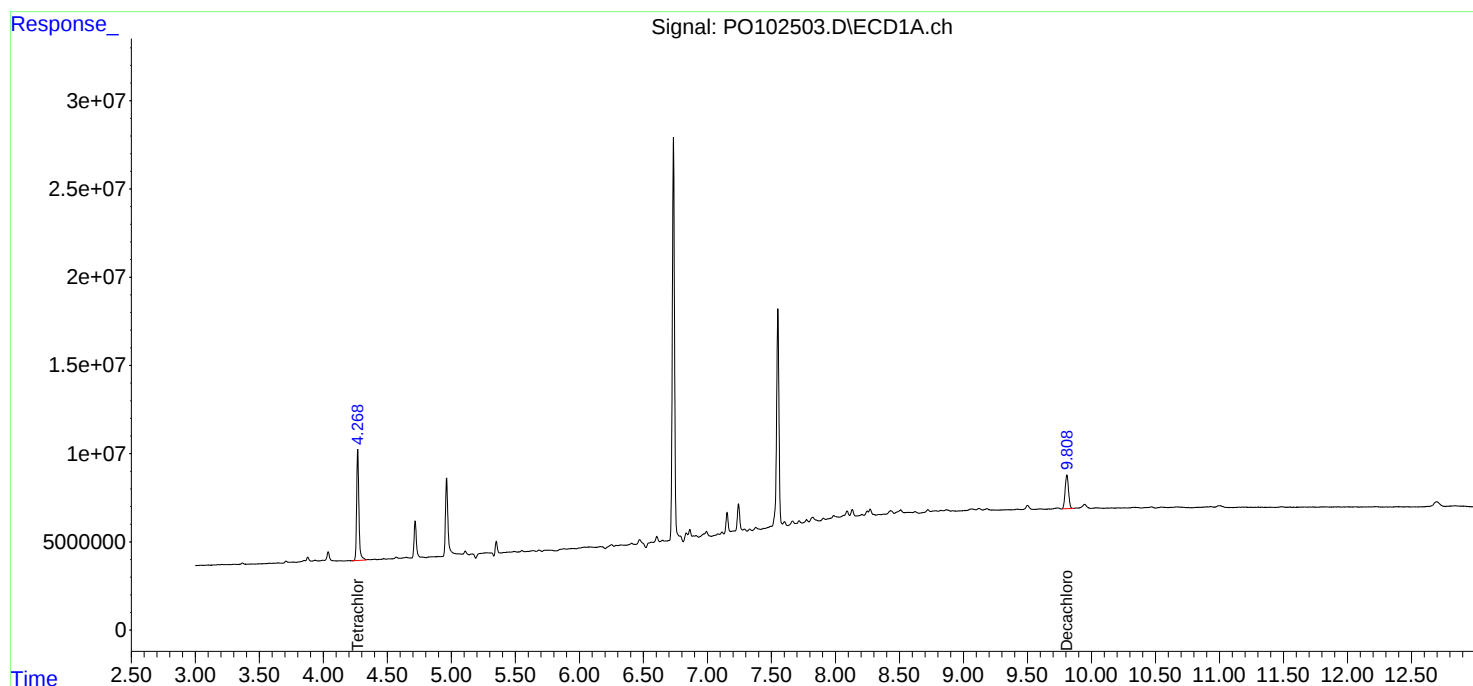

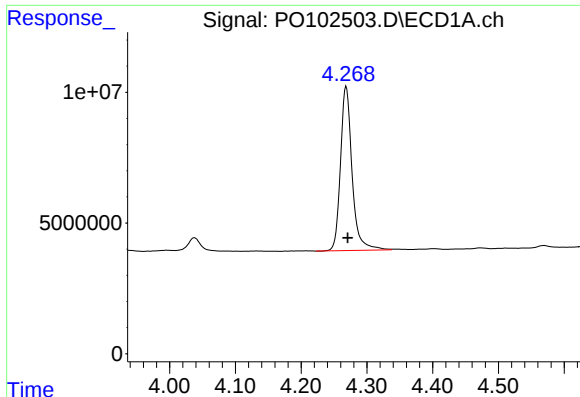


#1 Tetrachloro-m-xylene

R.T.: 4.269 min
Delta R.T.: -0.002 min
Response: 76910883
Conc: 18.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-0-2.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2024
Supervised By :Ankita Jodhani 03/15/2024

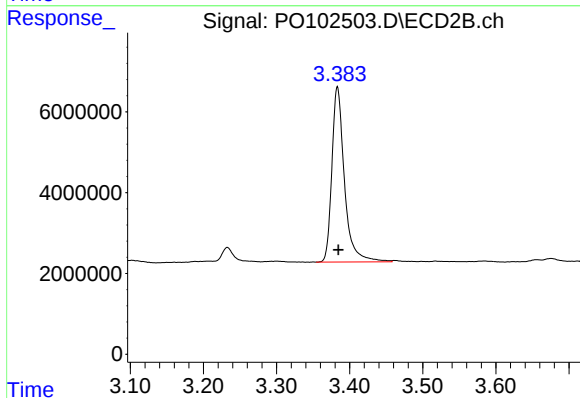


#1 Tetrachloro-m-xylene

R.T.: 3.383 min
Delta R.T.: -0.001 min
Response: 51875180
Conc: 18.51 ng/ml

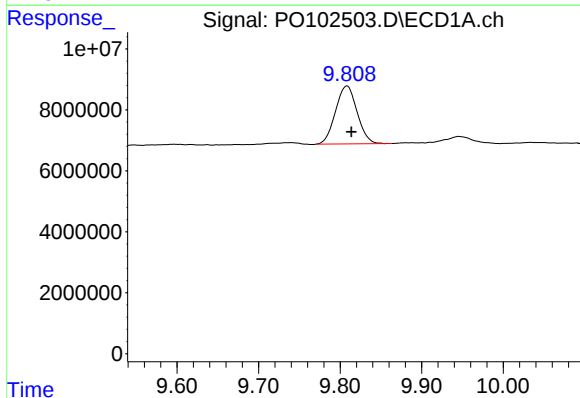

#2 Decachlorobiphenyl

R.T.: 9.809 min
Delta R.T.: -0.005 min
Response: 34999196
Conc: 18.43 ng/ml

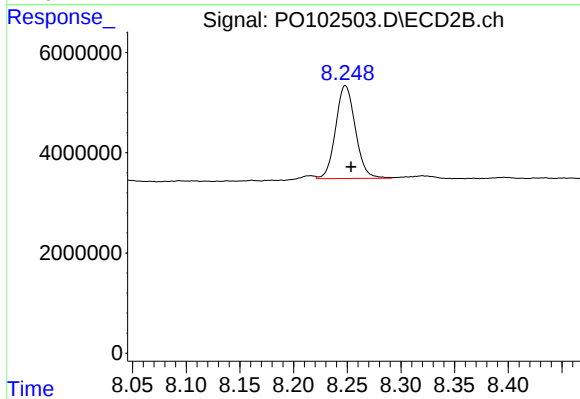

#2 Decachlorobiphenyl

R.T.: 8.248 min
Delta R.T.: -0.006 min
Response: 23676129
Conc: 19.20 ng/ml m