

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031424\
 Data File : P0102526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2024 23:26
 Operator : YP/AJ
 Sample : P1758-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB031224RB04

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/15/2024
 Supervised By :Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 00:30:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 13 04:51:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.266	3.382	81266560	50382092	19.826m	17.981m
2) SA Decachlor...	9.806	8.248	49562235	34895134	26.101	28.305

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031424\
Data File : PO102526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2024 23:26
Operator : YP/AJ
Sample : P1758-04
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB031224RB04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2024
Supervised By :Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 00:30:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031224.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 13 04:51:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

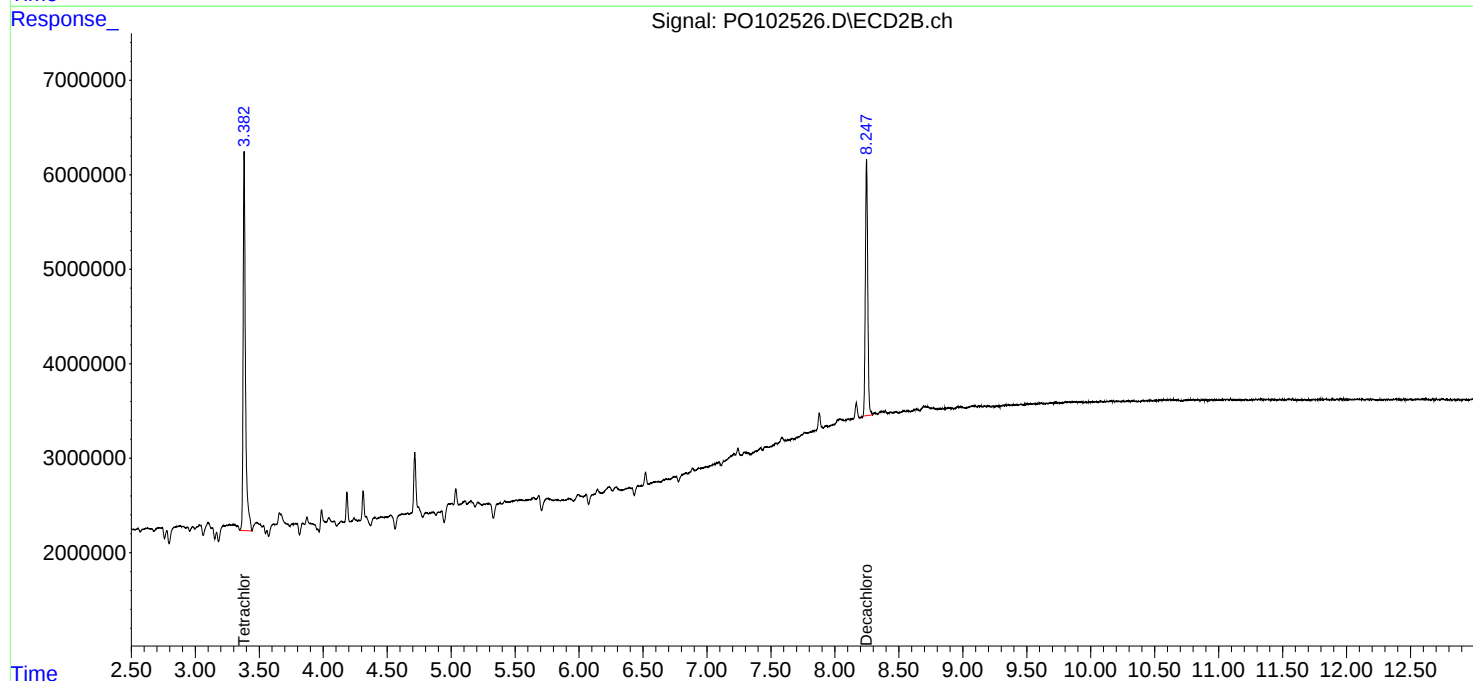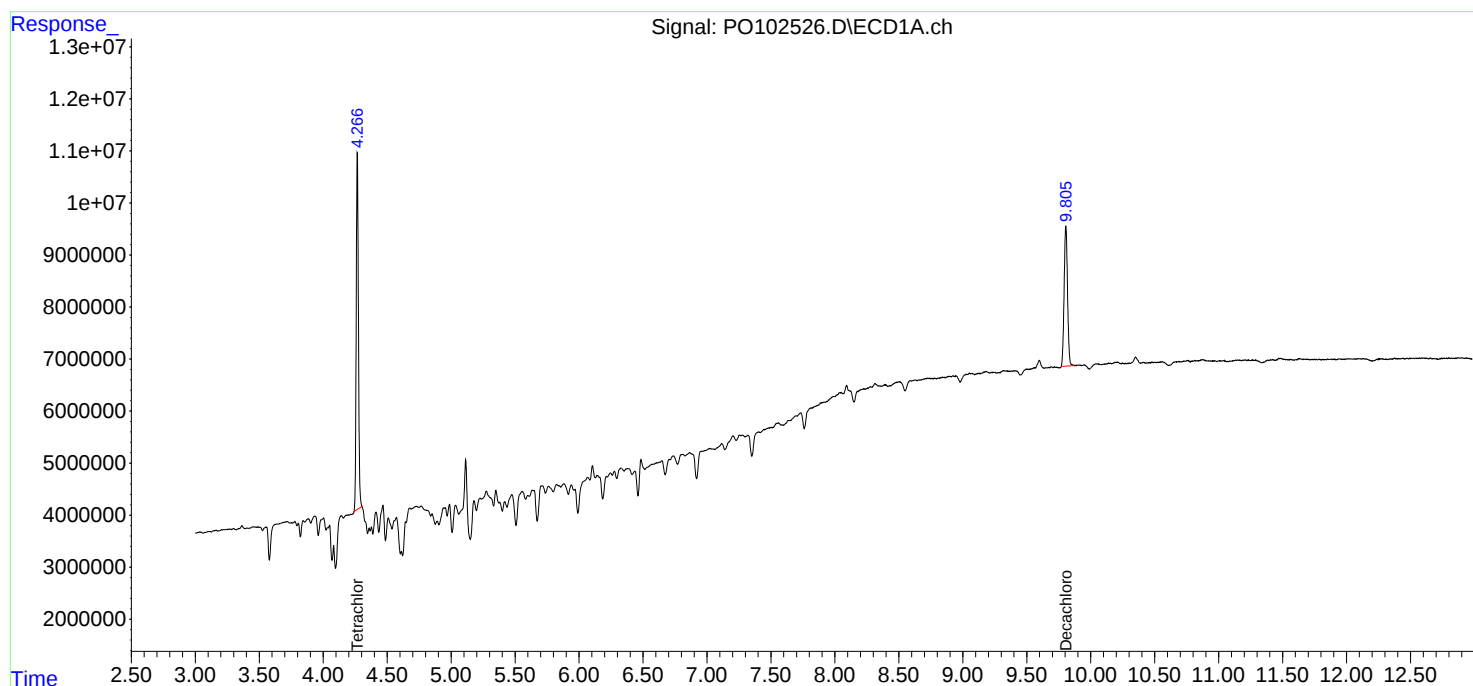

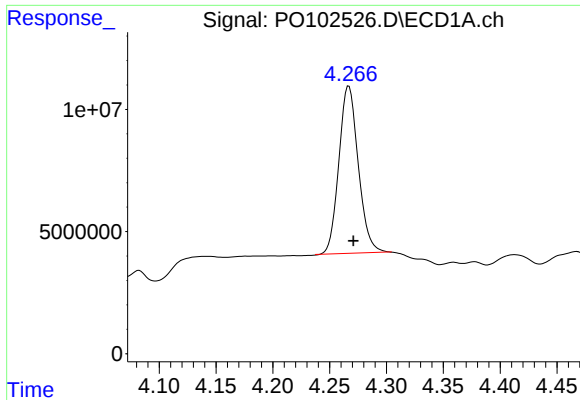


#1 Tetrachloro-m-xylene

R.T.: 4.266 min
Delta R.T.: -0.005 min
Response: 81266560
Conc: 19.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB031224RB04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/15/2024
Supervised By :Ankita Jodhani 03/15/2024

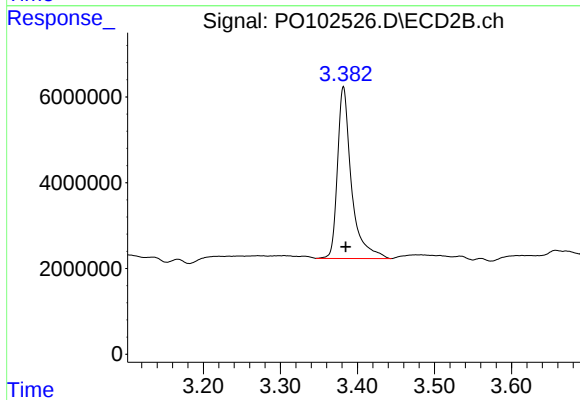


#1 Tetrachloro-m-xylene

R.T.: 3.382 min
Delta R.T.: -0.003 min
Response: 50382092
Conc: 17.98 ng/ml m

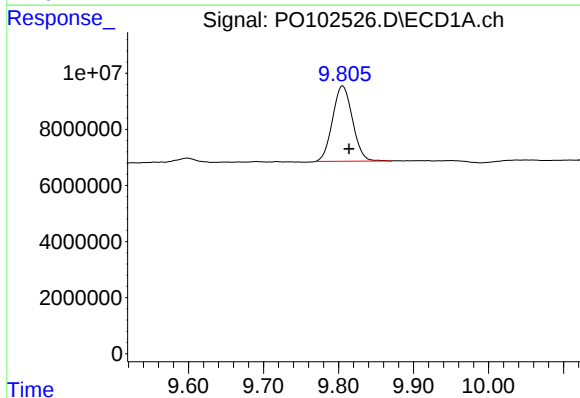

#2 Decachlorobiphenyl

R.T.: 9.806 min
Delta R.T.: -0.008 min
Response: 49562235
Conc: 26.10 ng/ml

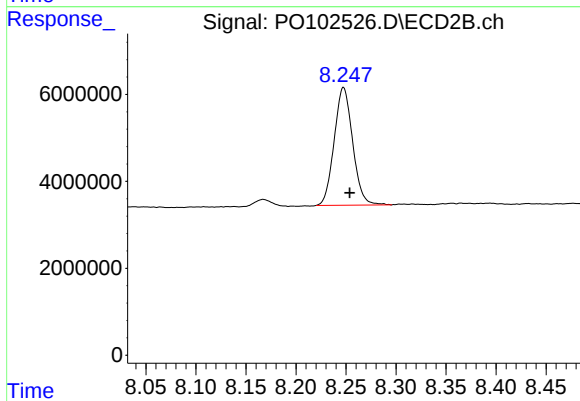

#2 Decachlorobiphenyl

R.T.: 8.248 min
Delta R.T.: -0.006 min
Response: 34895134
Conc: 28.30 ng/ml