

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031521\
 Data File : P0076173.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2021 23:37
 Operator : DD\AJ
 Sample : AR1262ICC050
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC050

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:16:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 06:36:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 06:35:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.935	298144	217641	5.016	5.239
2) SA Decachlor...	10.921	9.201	204169	225182	5.169	5.985
Target Compounds						
36) L8 AR-1262-1	8.567	7.292	152959	83773	51.606	58.303
37) L8 AR-1262-2	9.123	7.844	247578	272835	50.895m	56.016m
38) L8 AR-1262-3	9.432	8.128	170722	121887	51.162	57.757m
39) L8 AR-1262-4	9.525	8.192	129286	209585	50.039	56.101
40) L8 AR-1262-5	10.185	8.689	87259	91379	52.776	52.610

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031521\
Data File : P0076173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2021 23:37
Operator : DD\AJ
Sample : AR1262ICC050
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1262ICC050


Manual Integrations
APPROVED

Ankita
3/16/2021 11:16:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 06:36:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 06:35:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

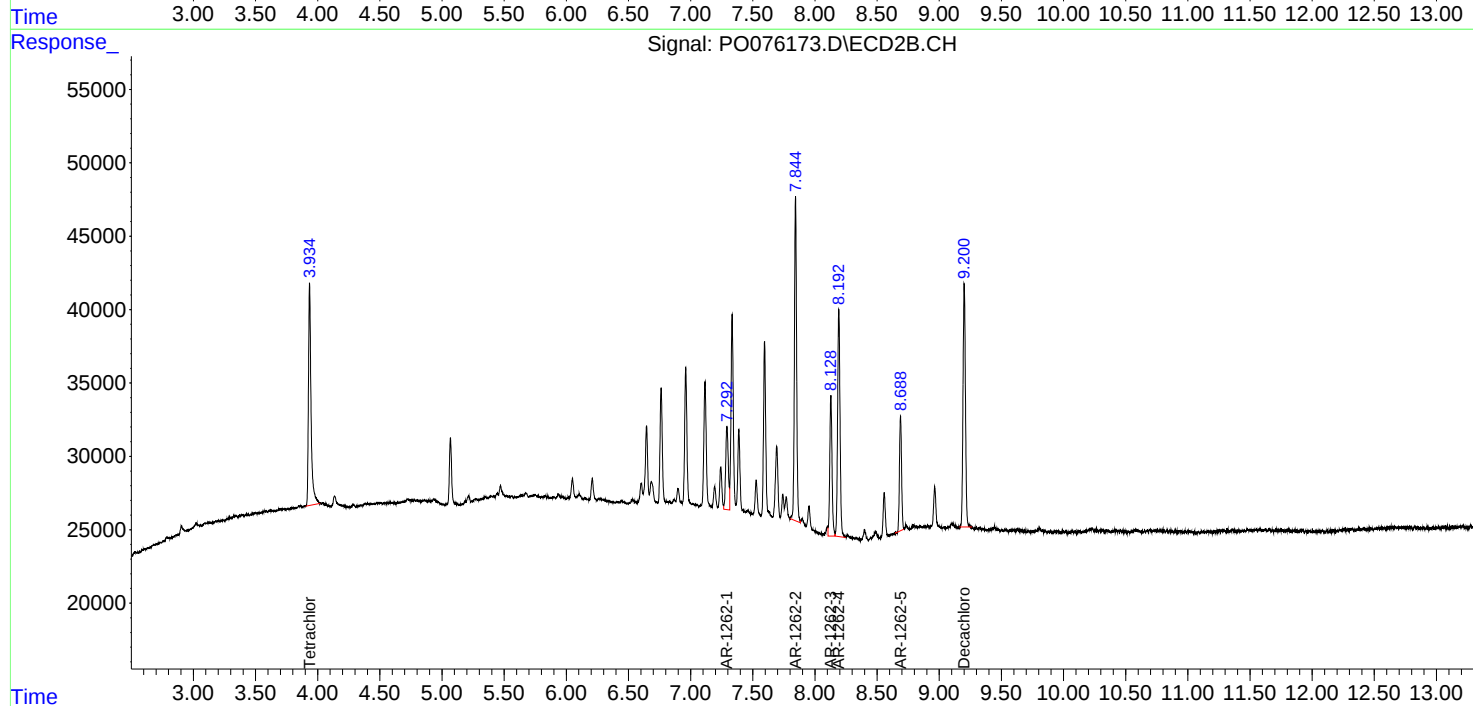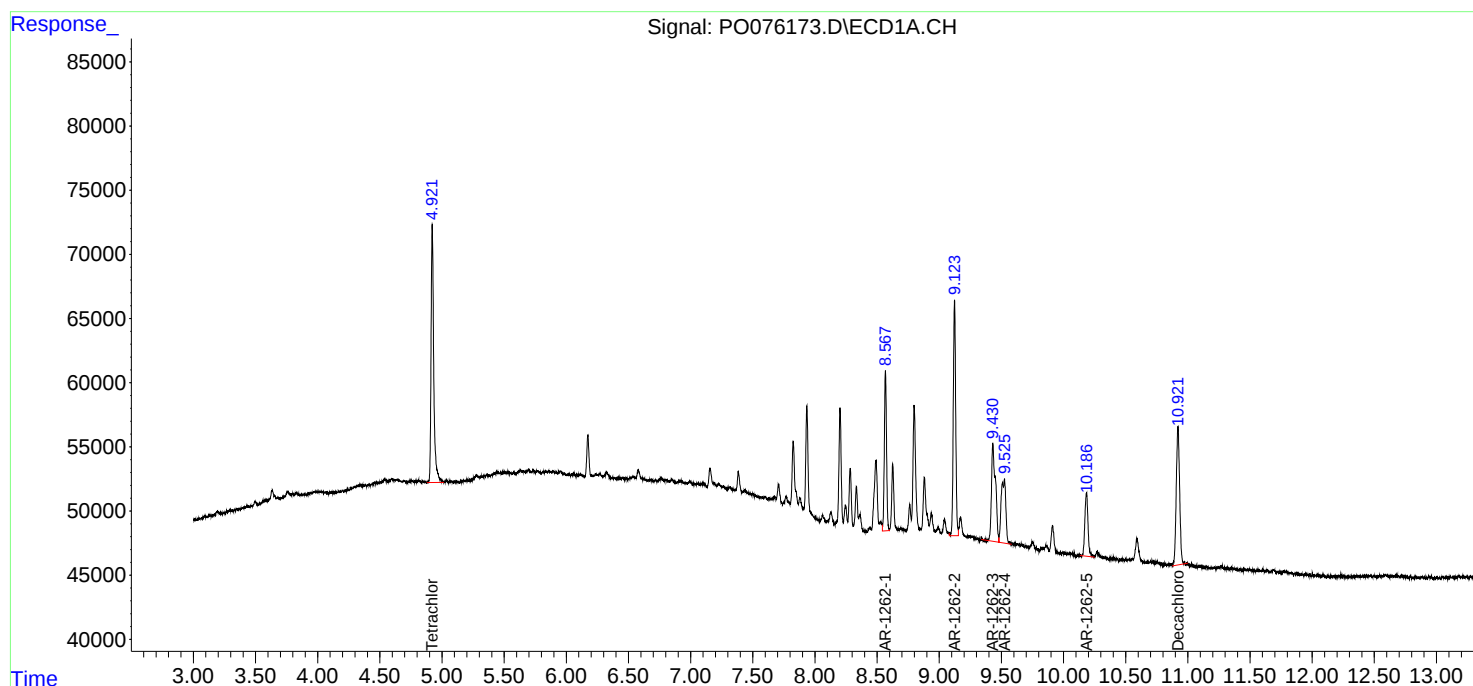

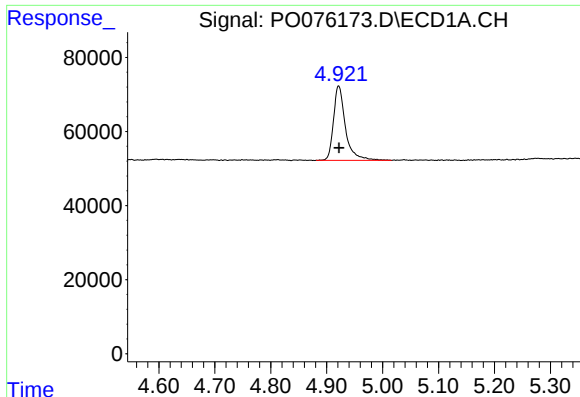


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 298144
Conc: 5.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262ICC050


Manual Integrations
APPROVED

Ankita
3/16/2021 11:16:35 AM

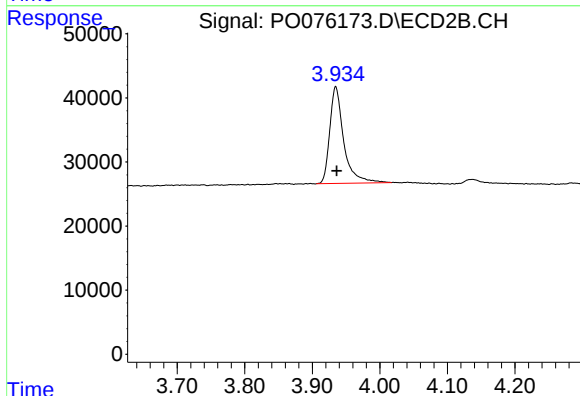


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 217641
Conc: 5.24 ng/ml

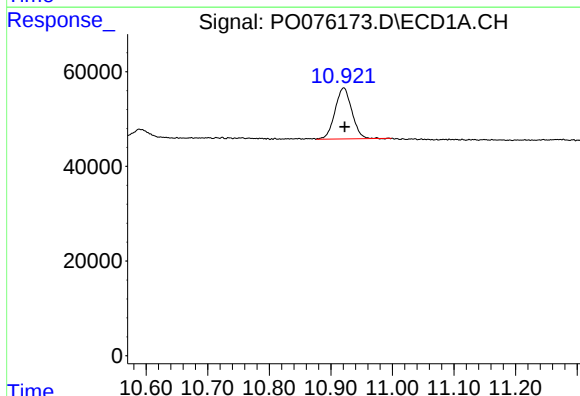


#2 Decachlorobiphenyl

R.T.: 10.921 min
Delta R.T.: -0.002 min
Response: 204169
Conc: 5.17 ng/ml

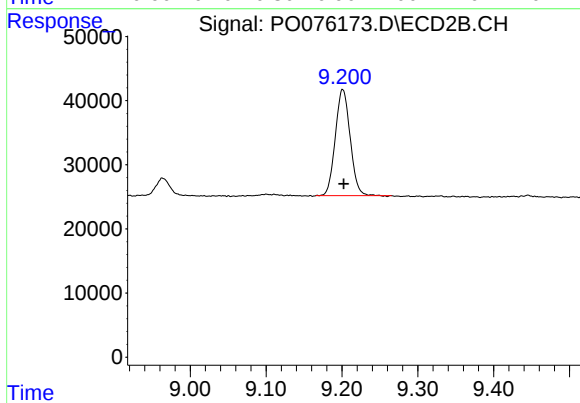

#2 Decachlorobiphenyl

R.T.: 9.201 min
Delta R.T.: -0.001 min
Response: 225182
Conc: 5.99 ng/ml

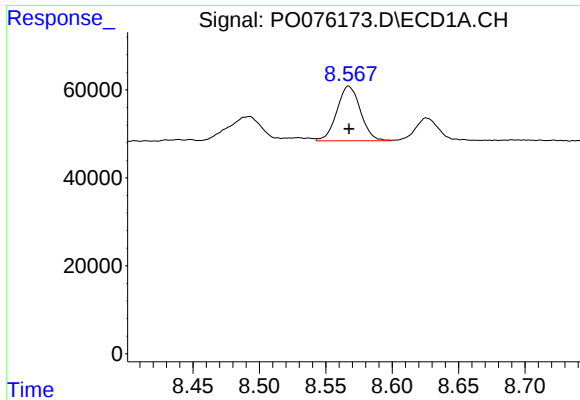


#36 AR-1262-1

R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 152959
Conc: 51.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262ICC050


Manual Integrations
APPROVED

Ankita
3/16/2021 11:16:35 AM

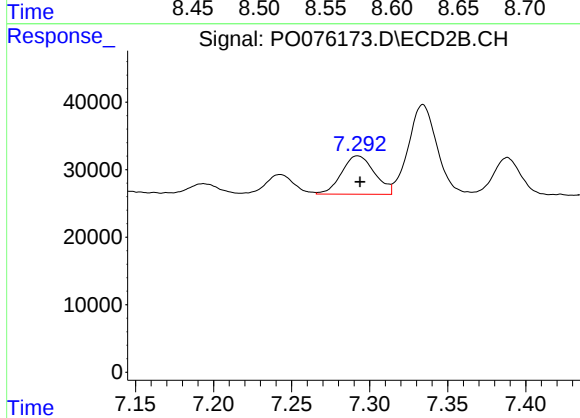


#36 AR-1262-1

R.T.: 7.292 min
Delta R.T.: -0.002 min
Response: 83773
Conc: 58.30 ng/ml

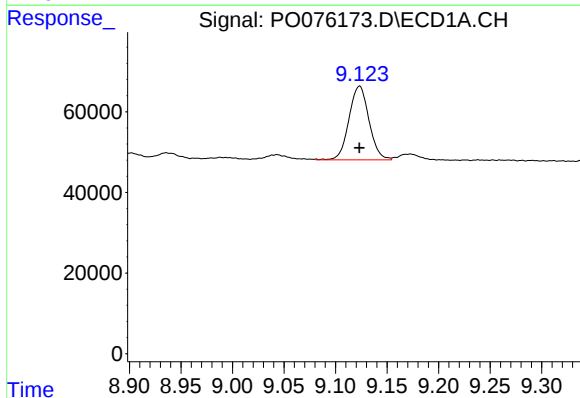


#37 AR-1262-2

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 247578
Conc: 50.89 ng/ml m

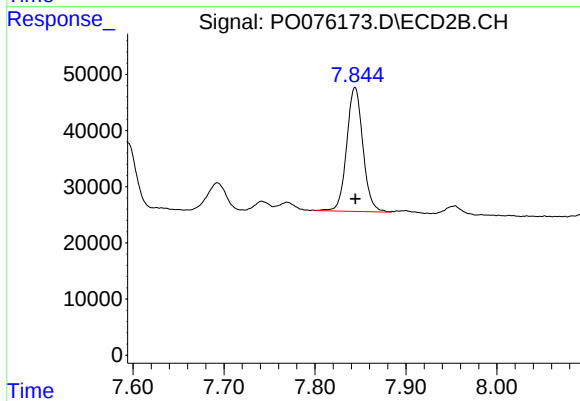

#37 AR-1262-2

R.T.: 7.844 min
Delta R.T.: 0.000 min
Response: 272835
Conc: 56.02 ng/ml m

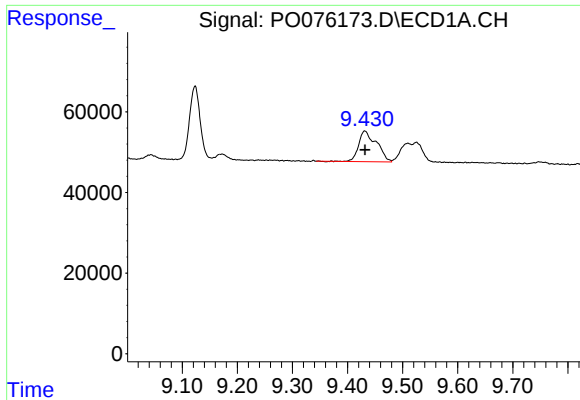


#38 AR-1262-3

R.T.: 9.432 min
Delta R.T.: 0.000 min
Response: 170722
Conc: 51.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262ICC050


Manual Integrations
APPROVED

Ankita
3/16/2021 11:16:35 AM

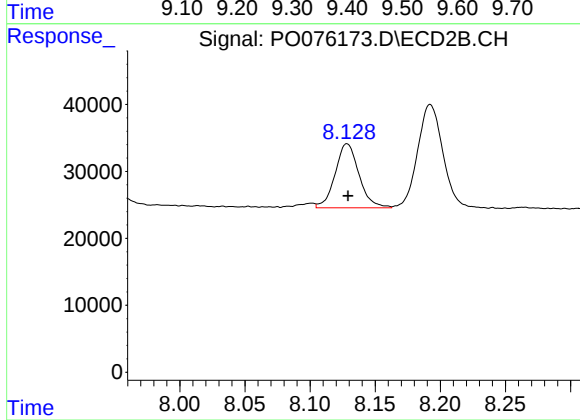


#38 AR-1262-3

R.T.: 8.128 min
Delta R.T.: -0.001 min
Response: 121887
Conc: 57.76 ng/ml m

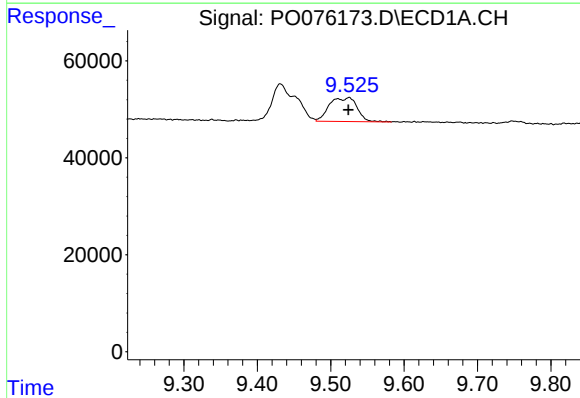


#39 AR-1262-4

R.T.: 9.525 min
Delta R.T.: 0.000 min
Response: 129286
Conc: 50.04 ng/ml

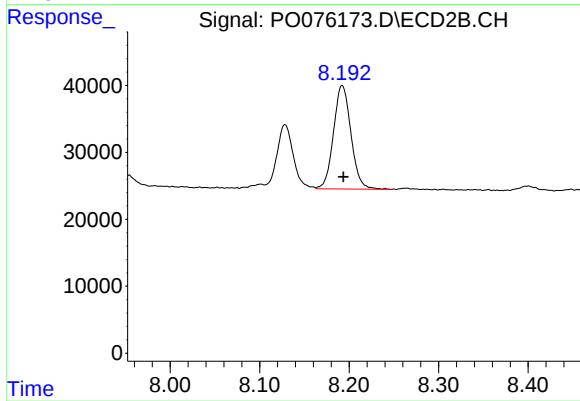

#39 AR-1262-4

R.T.: 8.192 min
Delta R.T.: -0.001 min
Response: 209585
Conc: 56.10 ng/ml

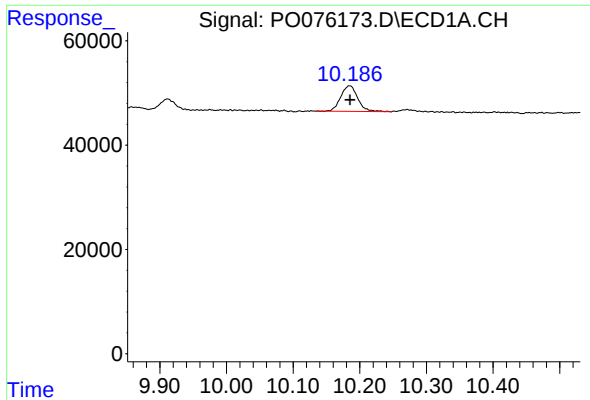


#40 AR-1262-5

R.T.: 10.185 min
Delta R.T.: -0.001 min
Response: 87259
Conc: 52.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262ICC050

Manual Integrations
APPROVED

Ankita
3/16/2021 11:16:35 AM

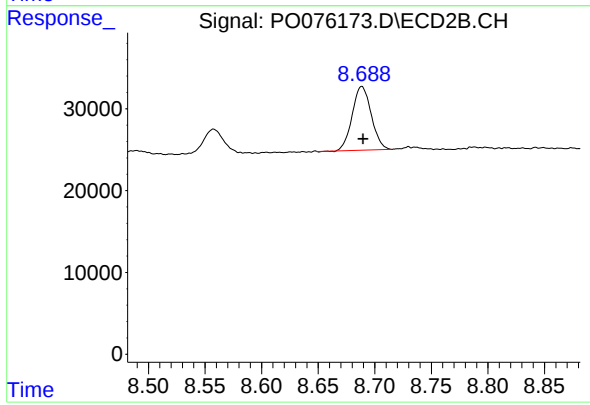

#40 AR-1262-5

R.T.: 8.689 min
Delta R.T.: -0.001 min
Response: 91379
Conc: 52.61 ng/ml