

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031522\
 Data File : P0085343.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Mar 2022 20:46
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2022
 Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:27:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 02:27:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.588	1015198	226503	4.532	4.830
2) SA Decachlor...	10.392	8.605	583245	207332	4.647	5.266
Target Compounds						
16) L4 AR-1242-1	5.679	4.677	246429	70848	48.818m	54.222
17) L4 AR-1242-2	5.703	4.695	349208	98459	47.570m	53.278
18) L4 AR-1242-3	5.765	4.871	208807	53357	47.515	52.769
19) L4 AR-1242-4	5.865	4.956	186434	57387	51.378	55.209
20) L4 AR-1242-5	6.613	5.480	170915	63067	48.099	49.984

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031522\
Data File : P0085343.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Mar 2022 20:46
Operator : YP\AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:27:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 02:27:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

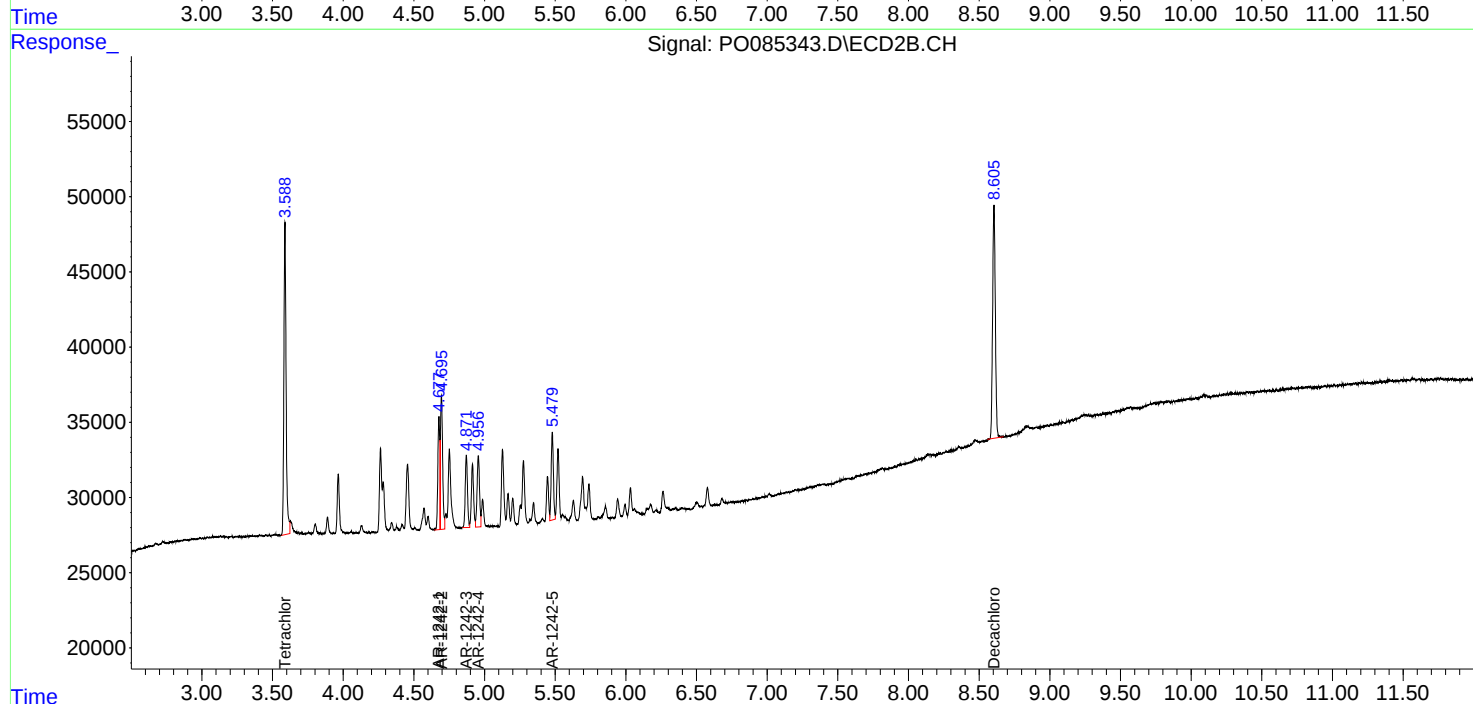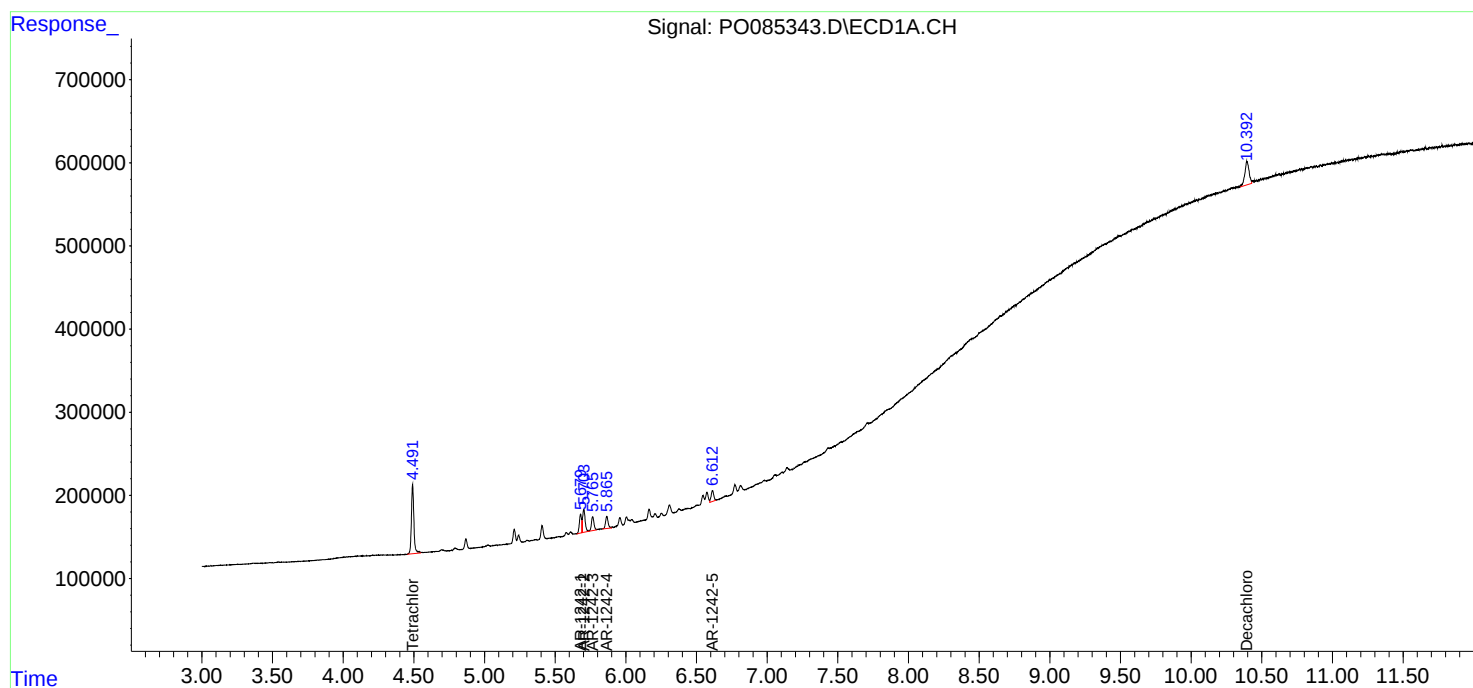

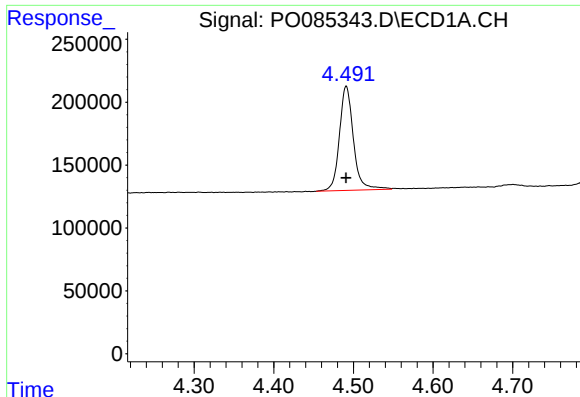


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: 0.000 min
Response: 1015198
Conc: 4.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242IC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

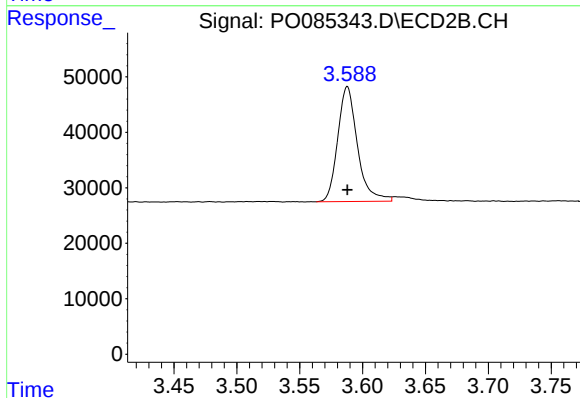


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: 0.000 min
Response: 226503
Conc: 4.83 ng/ml

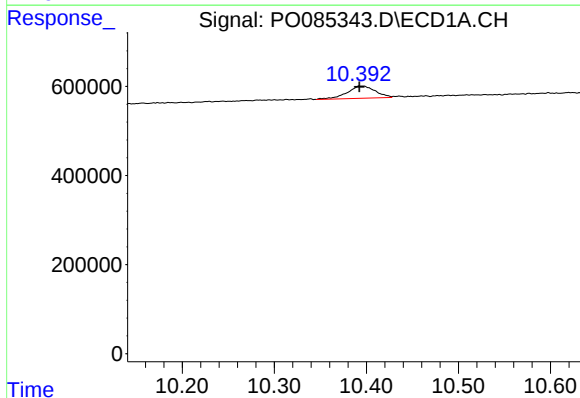


#2 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.000 min
Response: 583245
Conc: 4.65 ng/ml

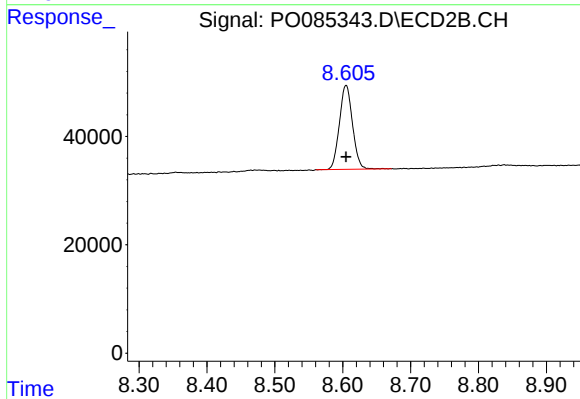

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: 0.000 min
Response: 207332
Conc: 5.27 ng/ml

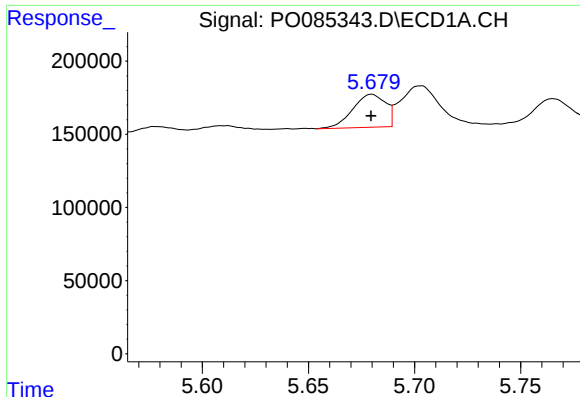


#16 AR-1242-1

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 246429
Conc: 48.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

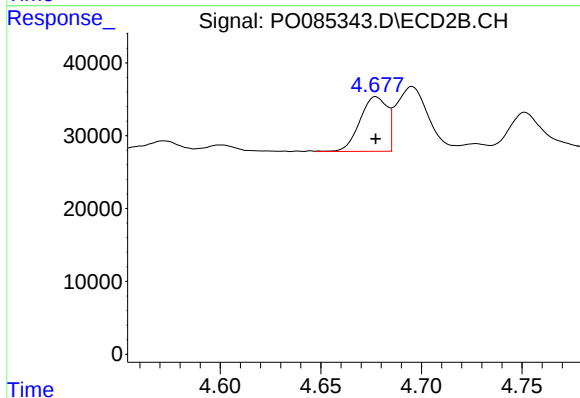


#16 AR-1242-1

R.T.: 4.677 min
Delta R.T.: 0.000 min
Response: 70848
Conc: 54.22 ng/ml

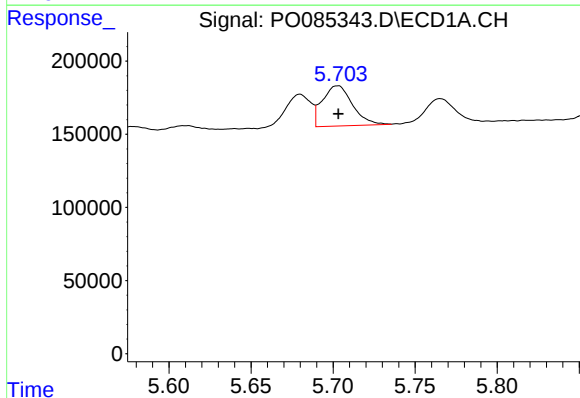


#17 AR-1242-2

R.T.: 5.703 min
Delta R.T.: 0.000 min
Response: 349208
Conc: 47.57 ng/ml m

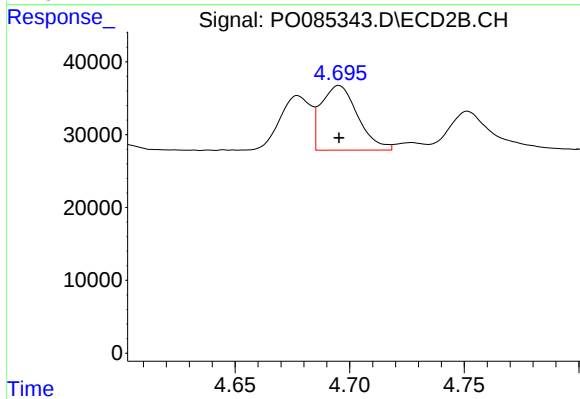

#17 AR-1242-2

R.T.: 4.695 min
Delta R.T.: 0.000 min
Response: 98459
Conc: 53.28 ng/ml

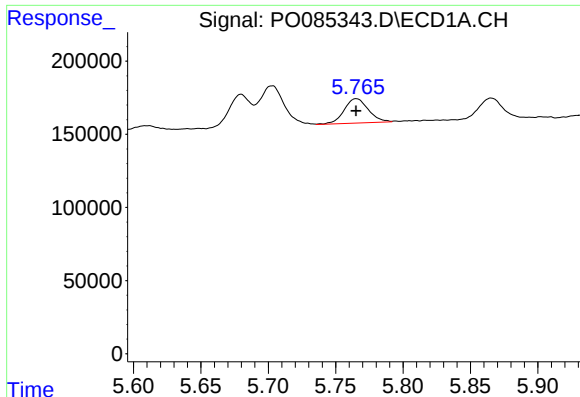


#18 AR-1242-3

R.T.: 5.765 min
Delta R.T.: 0.000 min
Response: 208807
Conc: 47.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

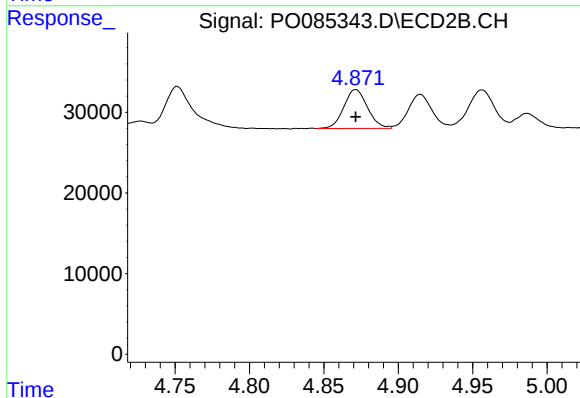


#18 AR-1242-3

R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 53357
Conc: 52.77 ng/ml

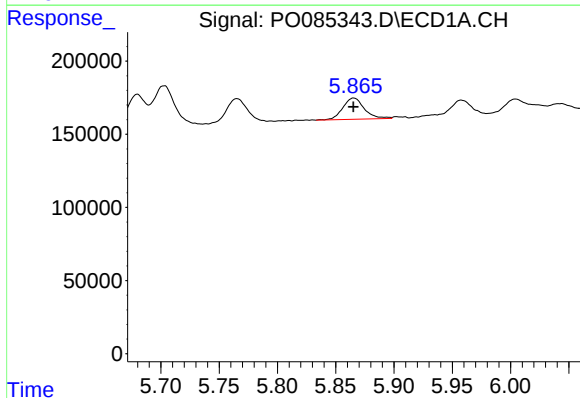


#19 AR-1242-4

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 186434
Conc: 51.38 ng/ml

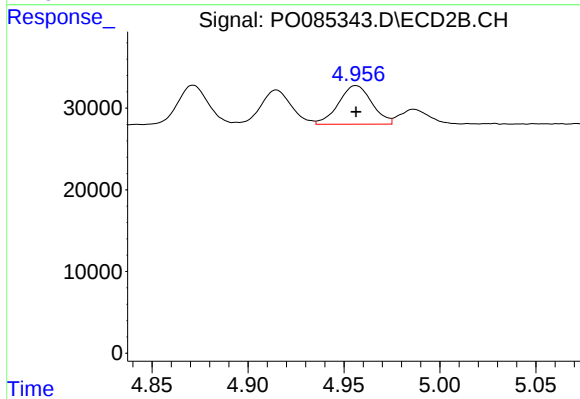

#19 AR-1242-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 57387
Conc: 55.21 ng/ml

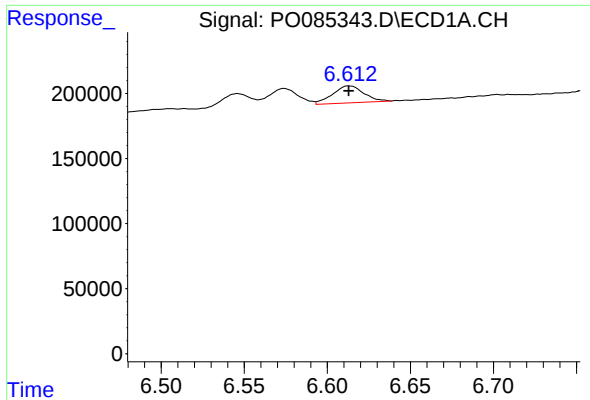


#20 AR-1242-5

R.T.: 6.613 min
Delta R.T.: 0.000 min
Response: 170915
Conc: 48.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

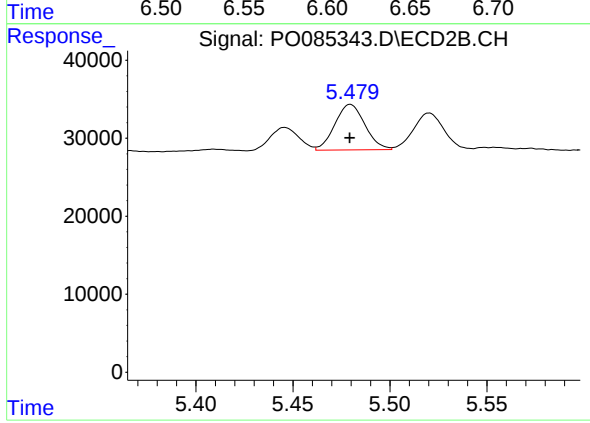

#20 AR-1242-5

R.T.: 5.480 min
Delta R.T.: 0.000 min
Response: 63067
Conc: 49.98 ng/ml