

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031522\
 Data File : P0085388.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2022 11:29
 Operator : YP\AJ
 Sample : N1905-15
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-14A-1A-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2022
 Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 13:48:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.497	3.600	1824810	740981	8.924	17.295m#
2) SA Decachlor...	10.419	8.632	3009749	524841	25.038	13.670m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031522\
Data File : P0085388.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2022 11:29
Operator : YP\AJ
Sample : N1905-15
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
WC-14A-1A-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 13:48:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

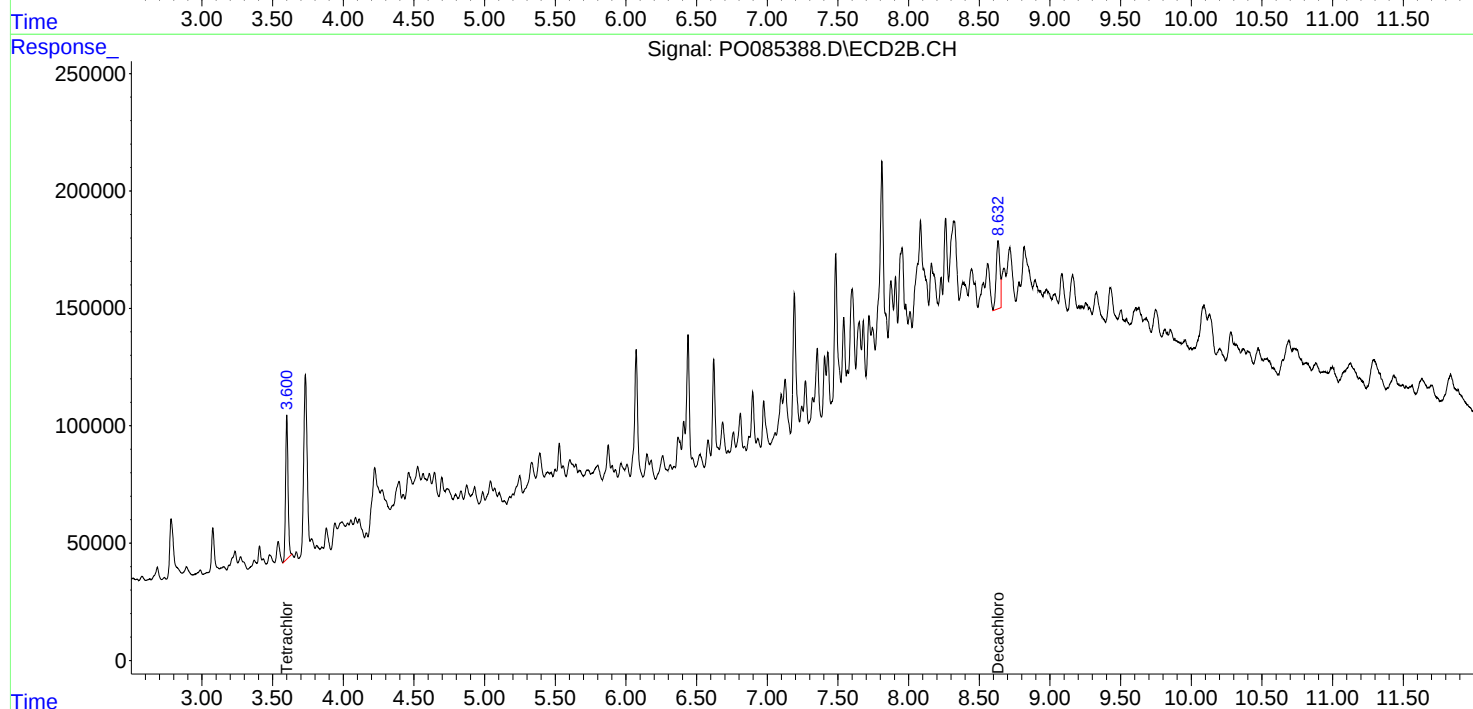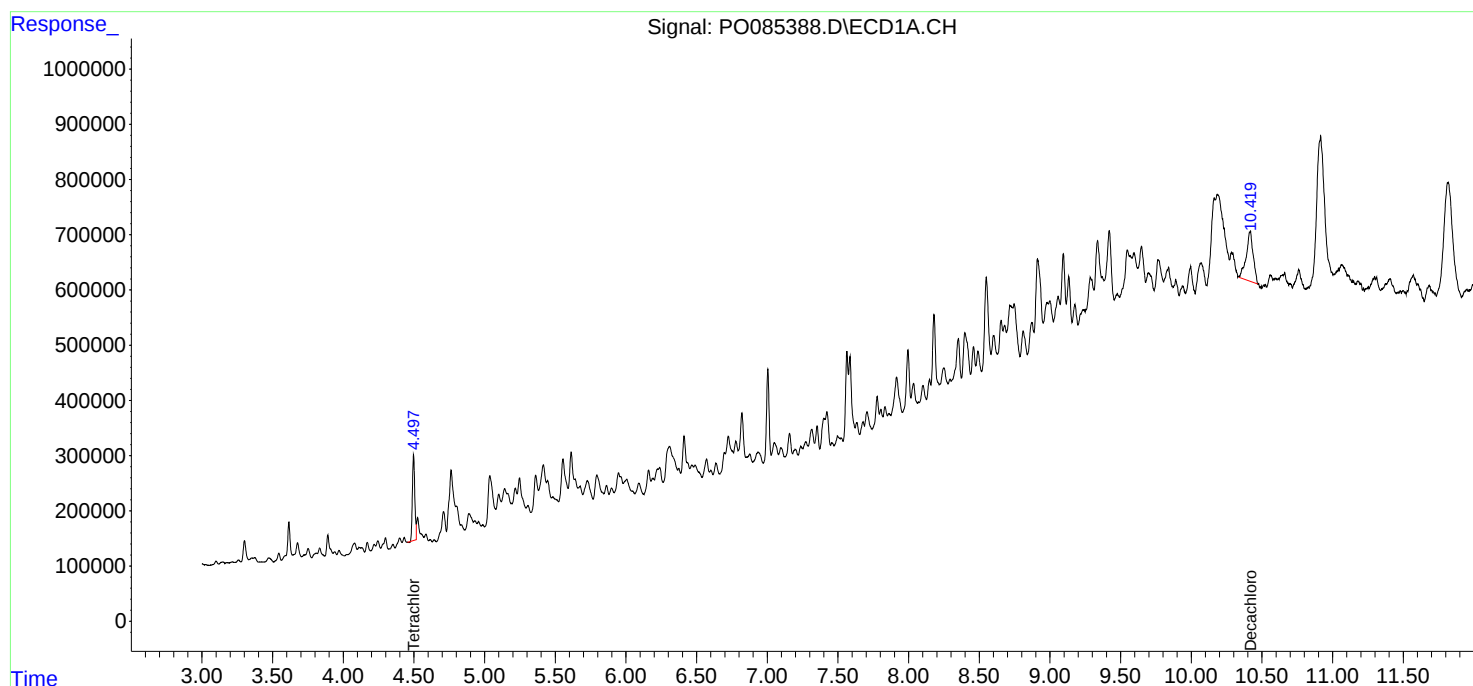

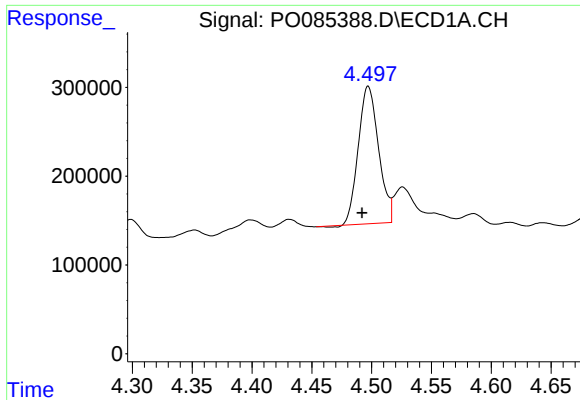


#1 Tetrachloro-m-xylene

R.T.: 4.497 min
Delta R.T.: 0.005 min
Response: 1824810
Conc: 8.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-14A-1A-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

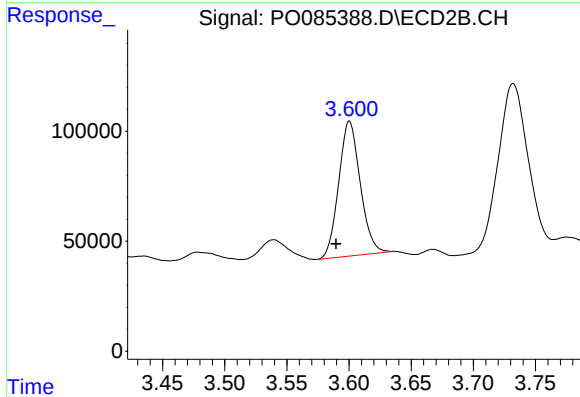


#1 Tetrachloro-m-xylene

R.T.: 3.600 min
Delta R.T.: 0.010 min
Response: 740981
Conc: 17.30 ng/ml m

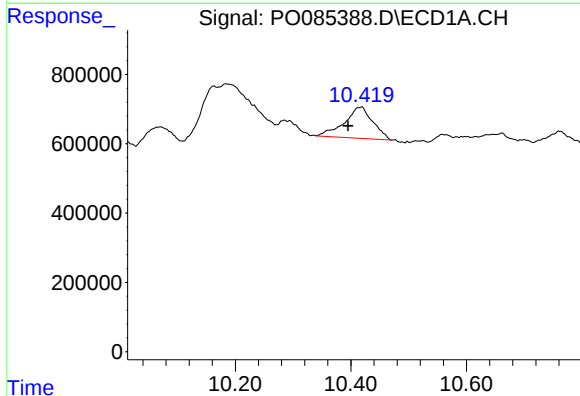

#2 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: 0.023 min
Response: 3009749
Conc: 25.04 ng/ml

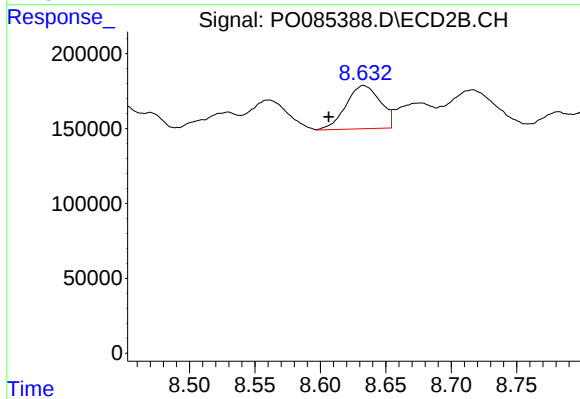

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: 0.026 min
Response: 524841
Conc: 13.67 ng/ml m