

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031522\
 Data File : P0085390.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2022 12:00
 Operator : YP\AJ
 Sample : N1950-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 31406

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 13:48:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.495	3.594	1807343	697876	8.839	16.289 #
2) SA Decachlor...	10.398	8.607	899375	246765	7.482	6.427m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031522\
 Data File : P0085390.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2022 12:00
 Operator : YP\AJ
 Sample : N1950-03
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31406

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 13:48:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

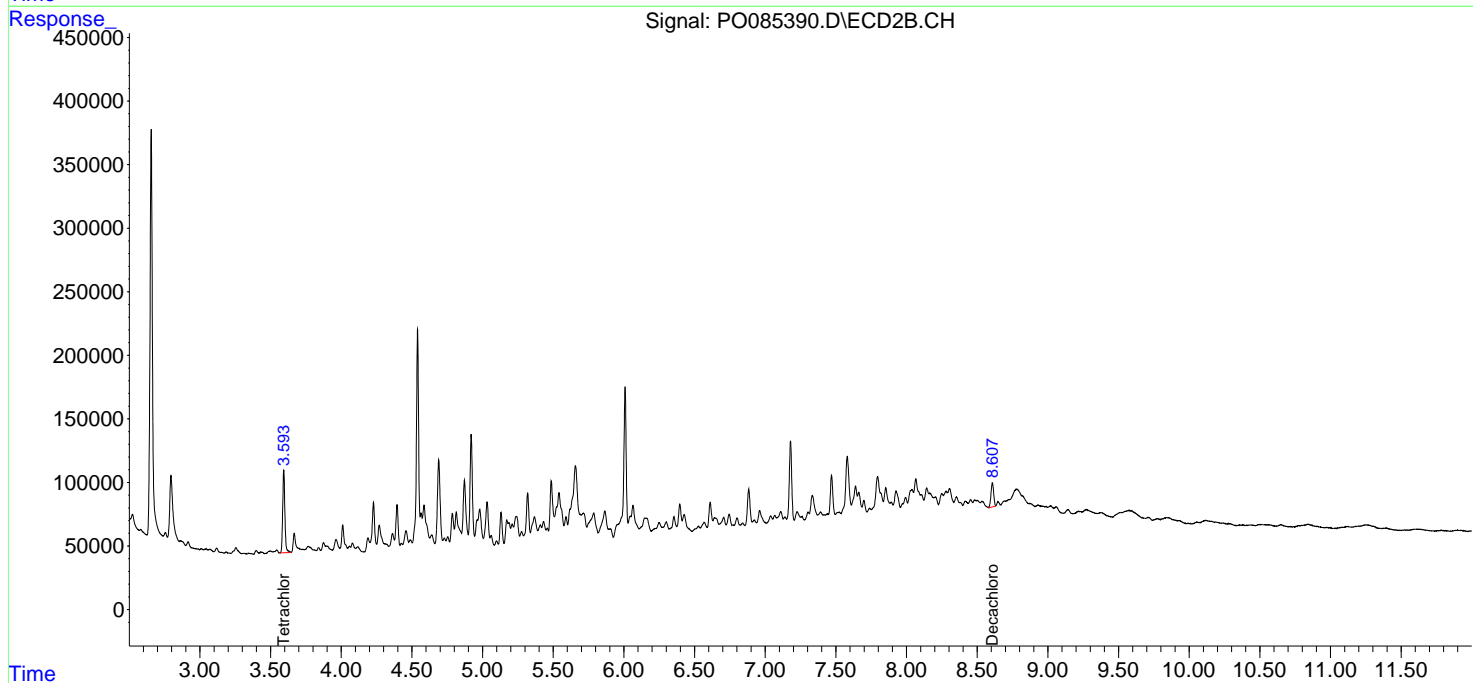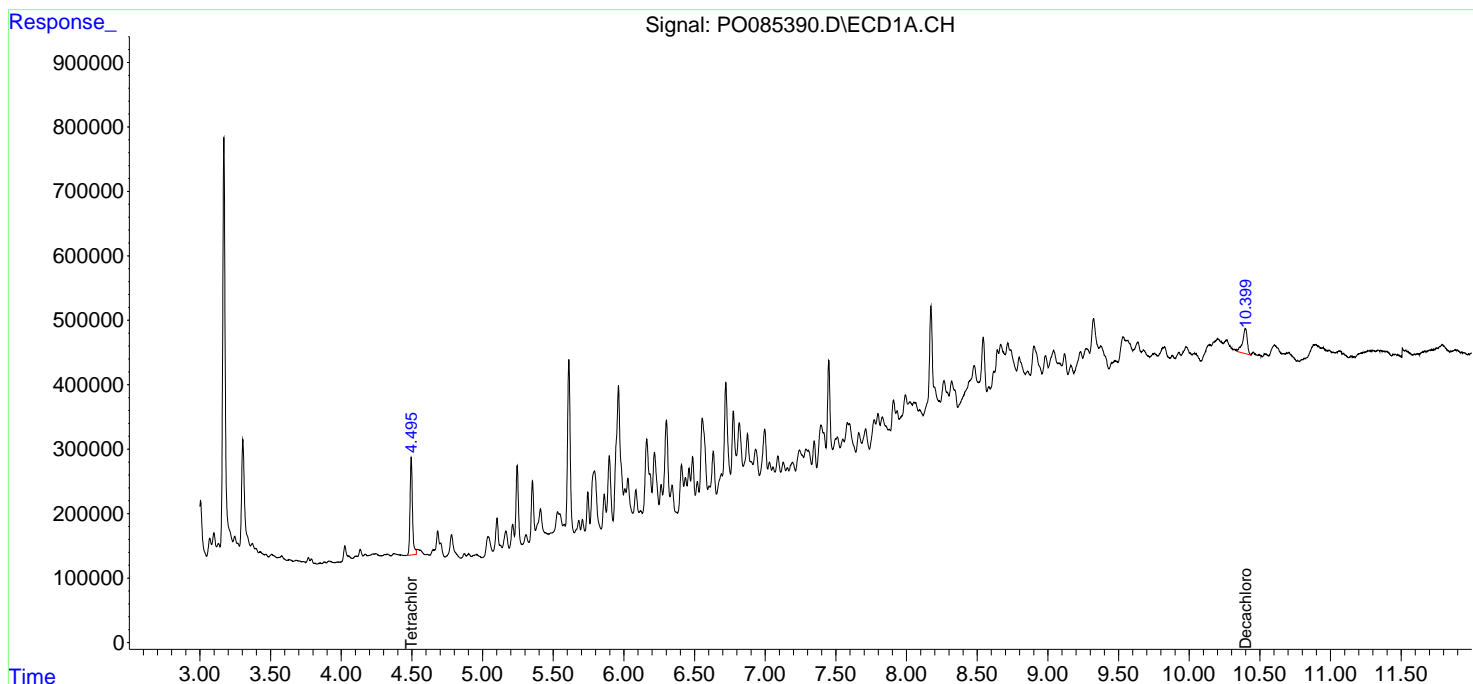


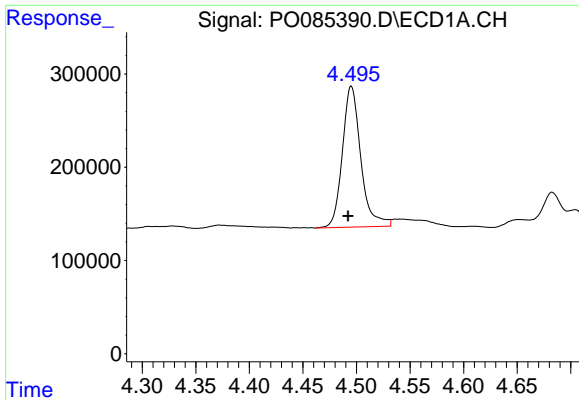

#1 Tetrachloro-m-xylene


R.T.: 4.495 min
 Delta R.T.: 0.003 min
 Response: 1807343
 Conc: 8.84 ng/ml

Instrument :
 ECD_O
 ClientSampleId :
 31406

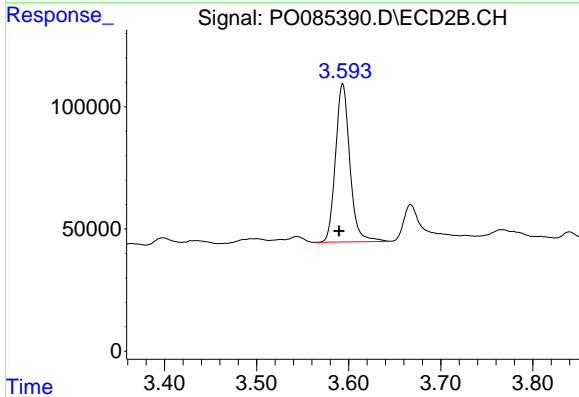


#1 Tetrachloro-m-xylene

R.T.: 3.594 min
 Delta R.T.: 0.004 min
 Response: 697876
 Conc: 16.29 ng/ml

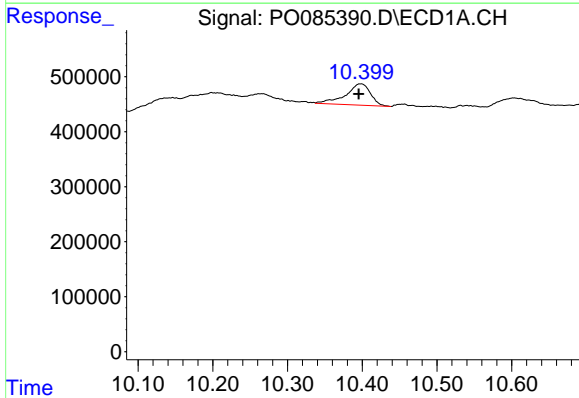

#2 Decachlorobiphenyl

R.T.: 10.398 min
 Delta R.T.: 0.003 min
 Response: 899375
 Conc: 7.48 ng/ml

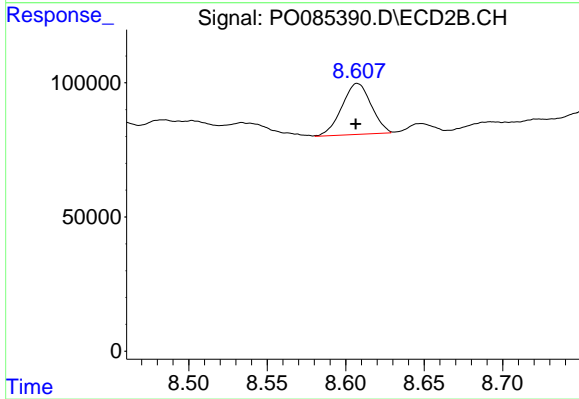

#2 Decachlorobiphenyl

R.T.: 8.607 min
 Delta R.T.: 0.000 min
 Response: 246765
 Conc: 6.43 ng/ml m