

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0031523\  
 Data File : P0093154.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 15 Mar 2023 10:09  
 Operator : YP/AJ  
 Sample : 01912-03DL 100X  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 04-A-04-B-04-CDL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 03/16/2023  
 Supervised By :Ankita Jodhani 03/16/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 15 21:59:22 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031323.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 14 05:32:59 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

Target Compounds

|     |    |           |       |       |          |          |          |         |
|-----|----|-----------|-------|-------|----------|----------|----------|---------|
| 26) | L6 | AR-1254-1 | 6.469 | 5.523 | 41492741 | 26328730 | 355.063  | 419.490 |
| 27) | L6 | AR-1254-2 | 6.689 | 5.671 | 82416351 | 29876418 | 482.340  | 530.177 |
| 28) | L6 | AR-1254-3 | 7.058 | 6.076 | 102.7E6  | 54299083 | 617.746  | 630.695 |
| 29) | L6 | AR-1254-4 | 7.345 | 6.306 | 81608792 | 34974455 | 765.571m | 764.789 |
| 30) | L6 | AR-1254-5 | 7.769 | 6.726 | 117.2E6  | 68421328 | 865.320m | 926.466 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO031523\  
Data File : PO093154.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 15 Mar 2023 10:09  
Operator : YP/AJ  
Sample : 01912-03DL 100X  
Misc :  
ALS Vial : 9 Sample Multiplier: 1



Instrument :  
ECD\_O  
ClientSampleId :  
04-A-04-B-04-CDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/16/2023  
Supervised By :Ankita Jodhani 03/16/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 15 21:59:22 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO031323.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Mar 14 05:32:59 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

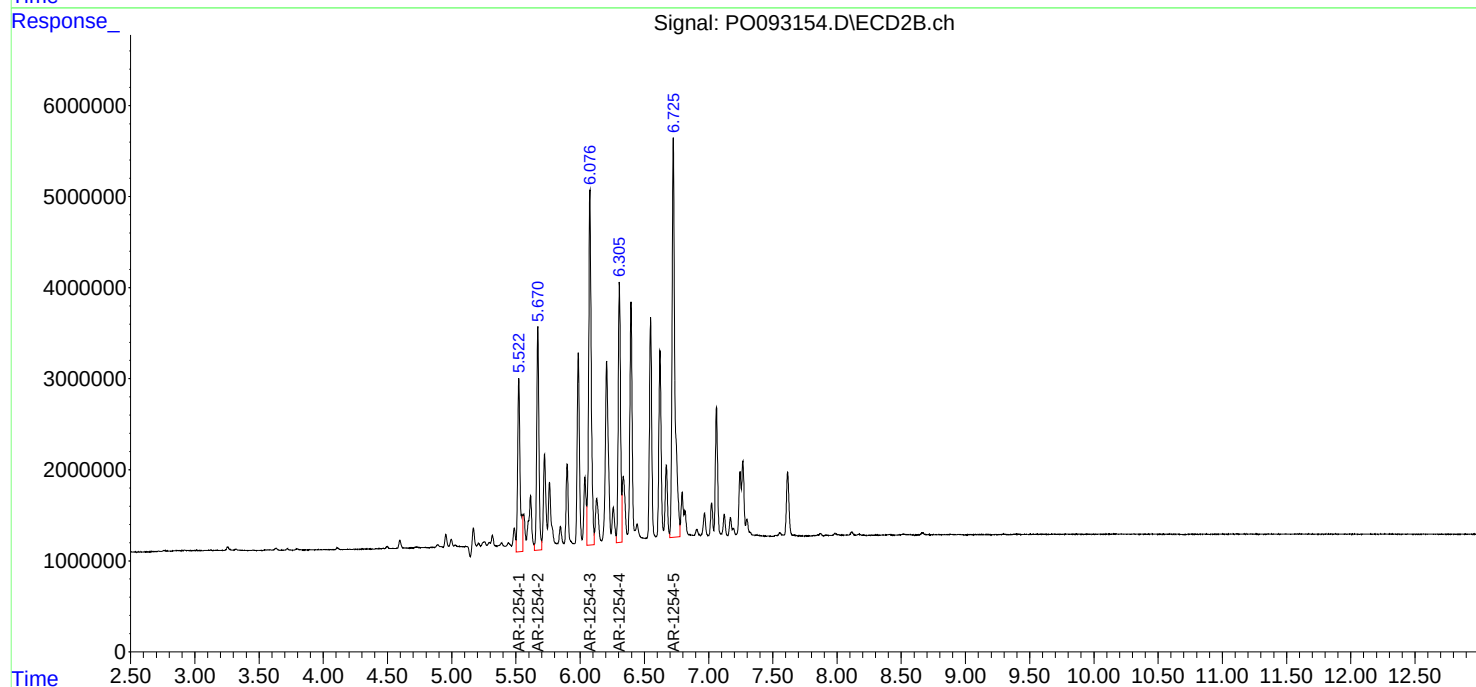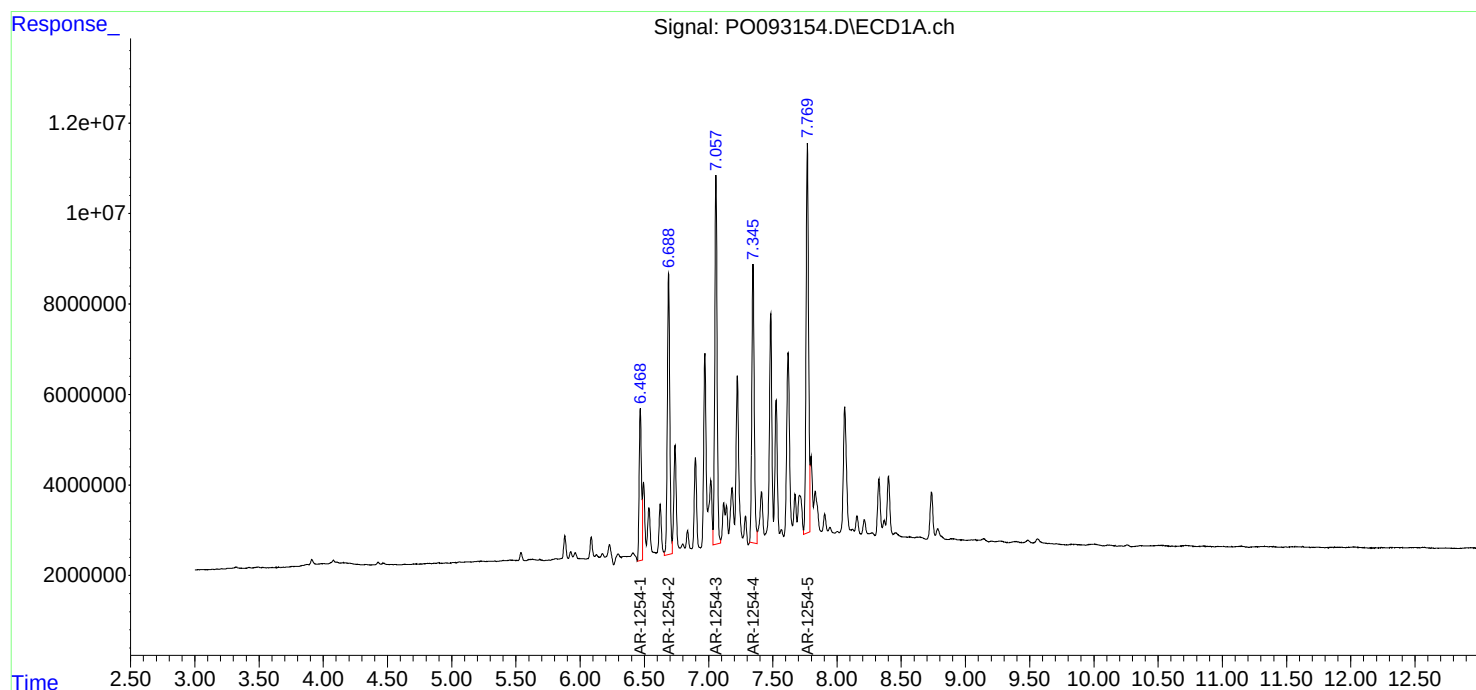

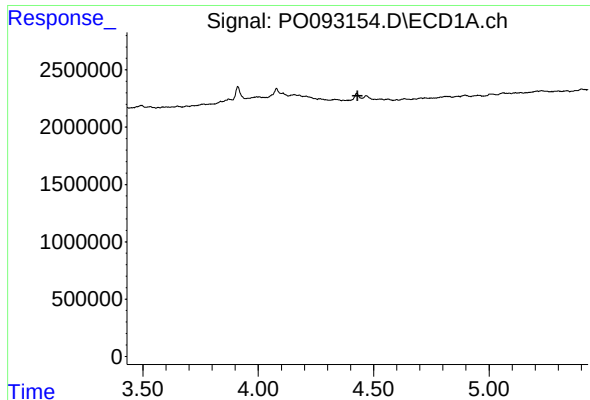

#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T.: 4.430 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_O  
ClientSampleId :  
04-A-04-B-04-CDL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/16/2023  
Supervised By :Ankita Jodhani 03/16/2023

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T.: 3.635 min  
Response: 0  
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T.: 10.263 min  
Response: 0  
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T.: 8.668 min  
Response: 0  
Conc: N.D.

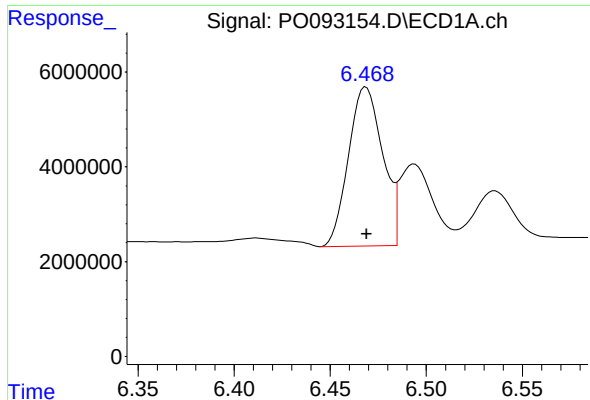


#26 AR-1254-1

R.T.: 6.469 min  
Delta R.T.: 0.000 min  
Response: 41492741  
Conc: 355.06 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
04-A-04-B-04-CDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/16/2023  
Supervised By :Ankita Jodhani 03/16/2023

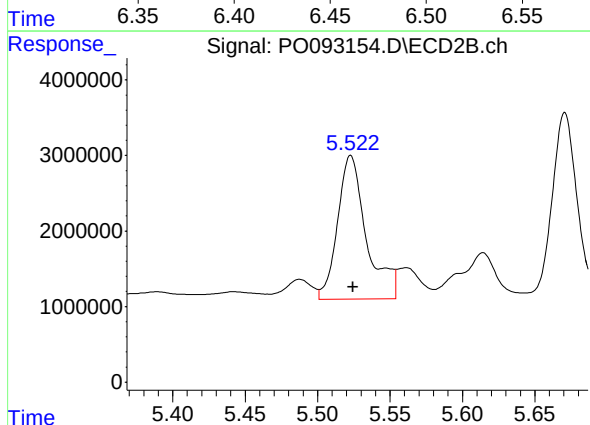


#26 AR-1254-1

R.T.: 5.523 min  
Delta R.T.: -0.002 min  
Response: 26328730  
Conc: 419.49 ng/ml

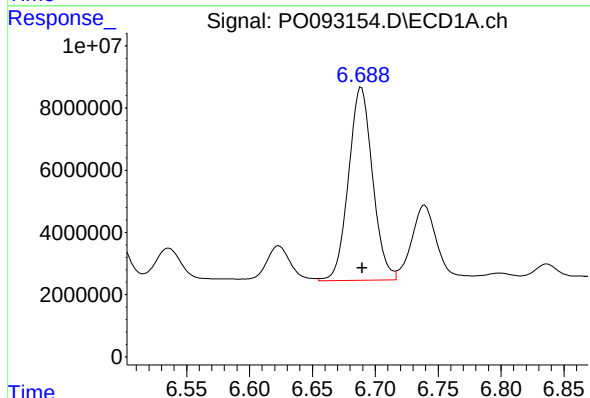


#27 AR-1254-2

R.T.: 6.689 min  
Delta R.T.: 0.000 min  
Response: 82416351  
Conc: 482.34 ng/ml

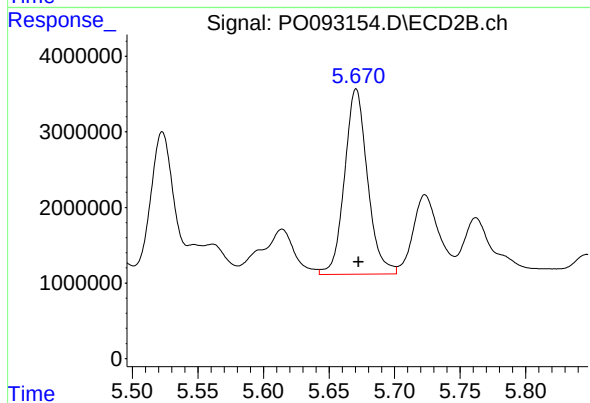

#27 AR-1254-2

R.T.: 5.671 min  
Delta R.T.: -0.002 min  
Response: 29876418  
Conc: 530.18 ng/ml

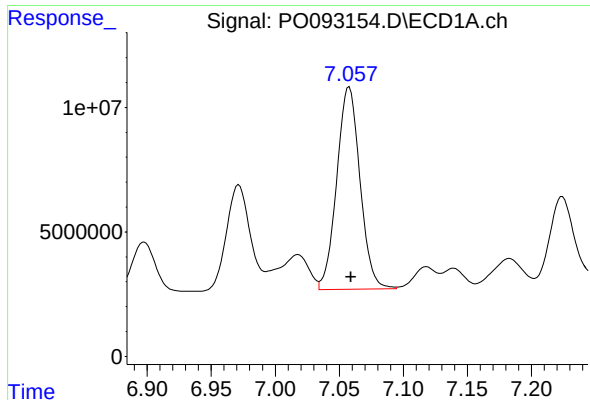


#28 AR-1254-3

R.T.: 7.058 min  
Delta R.T.: -0.002 min  
Response: 102692727  
Conc: 617.75 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
04-A-04-B-04-CDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/16/2023  
Supervised By :Ankita Jodhani 03/16/2023

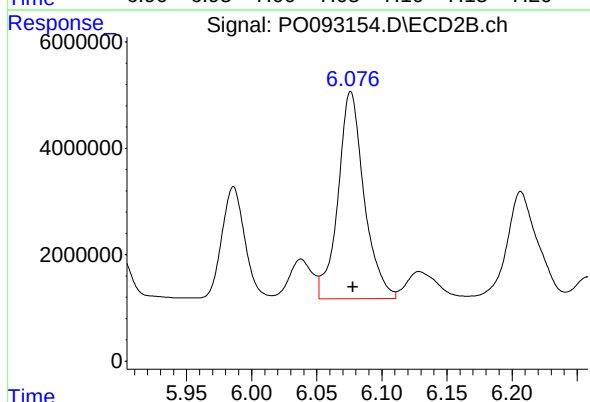


#28 AR-1254-3

R.T.: 6.076 min  
Delta R.T.: -0.002 min  
Response: 54299083  
Conc: 630.70 ng/ml

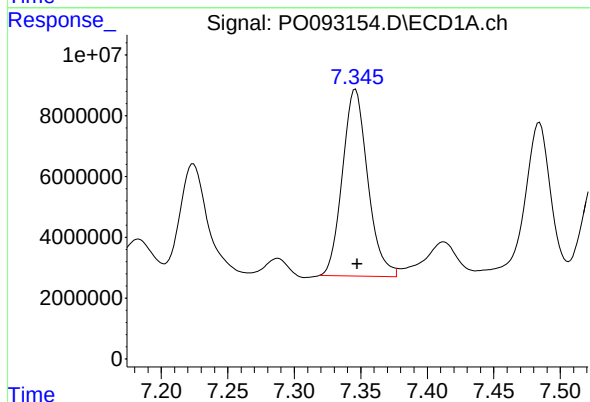


#29 AR-1254-4

R.T.: 7.345 min  
Delta R.T.: -0.002 min  
Response: 81608792  
Conc: 765.57 ng/ml m

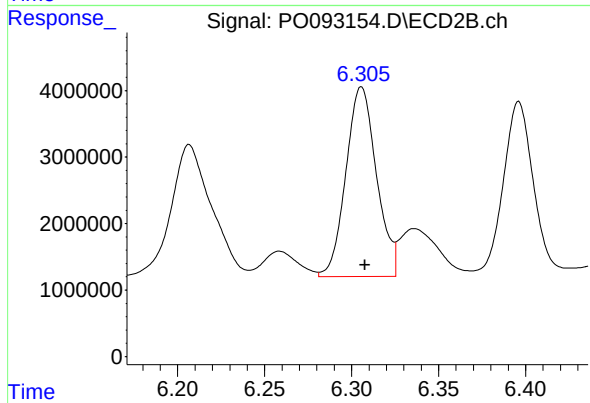

#29 AR-1254-4

R.T.: 6.306 min  
Delta R.T.: -0.002 min  
Response: 34974455  
Conc: 764.79 ng/ml

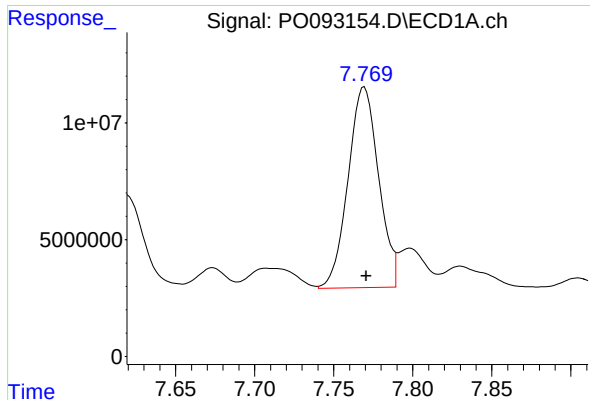


#30 AR-1254-5

R.T.: 7.769 min  
Delta R.T.: -0.002 min  
Response: 117171935  
Conc: 865.32 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
04-A-04-B-04-CDL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/16/2023  
Supervised By :Ankita Jodhani 03/16/2023

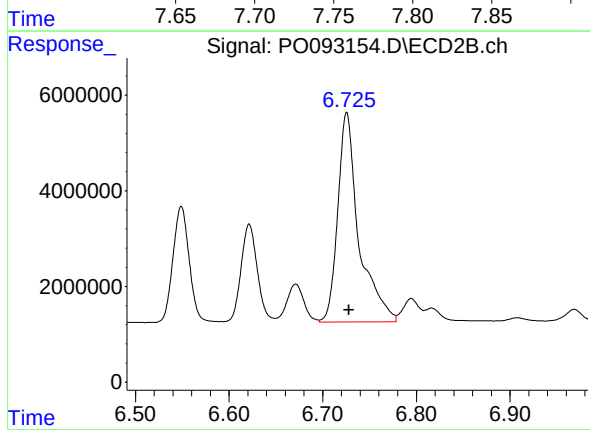

#30 AR-1254-5

R.T.: 6.726 min  
Delta R.T.: -0.002 min  
Response: 68421328  
Conc: 926.47 ng/ml