

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031523\
 Data File : P0093182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 19:44
 Operator : YP/AJ
 Sample : 01907-06DL 2X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33961DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/16/2023
 Supervised By :Ankita Jodhani 03/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:16:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.633	33800241	12752790	10.794	11.307
2) SA Decachlor...	10.263	8.667	32617750	15860319	15.071	16.198
Target Compounds						
21) L5 AR-1248-1	5.605	4.719	45268076	17208275	728.205	739.451
22) L5 AR-1248-2	5.882	4.957	45457462	18649096	475.945m	514.592
23) L5 AR-1248-3	6.088	4.998	80452151	21605755	773.139	575.745 #
24) L5 AR-1248-4	6.496	5.170	88661995	31311169	870.676	727.804
25) L5 AR-1248-5	6.534	5.564	81054441	37204612	791.862	1011.616 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031523\
Data File : PO093182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 19:44
Operator : YP/AJ
Sample : 01907-06DL 2X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
33961DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/16/2023
Supervised By :Ankita Jodhani 03/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:16:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

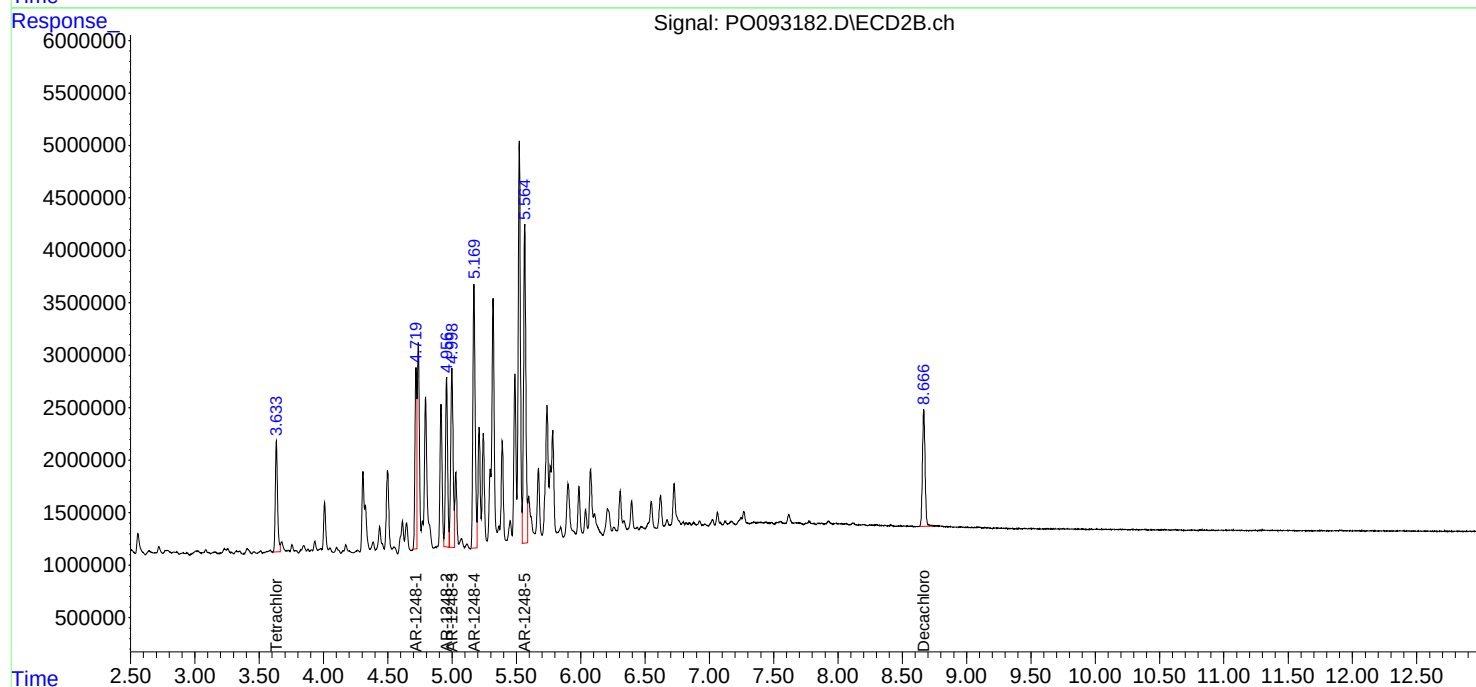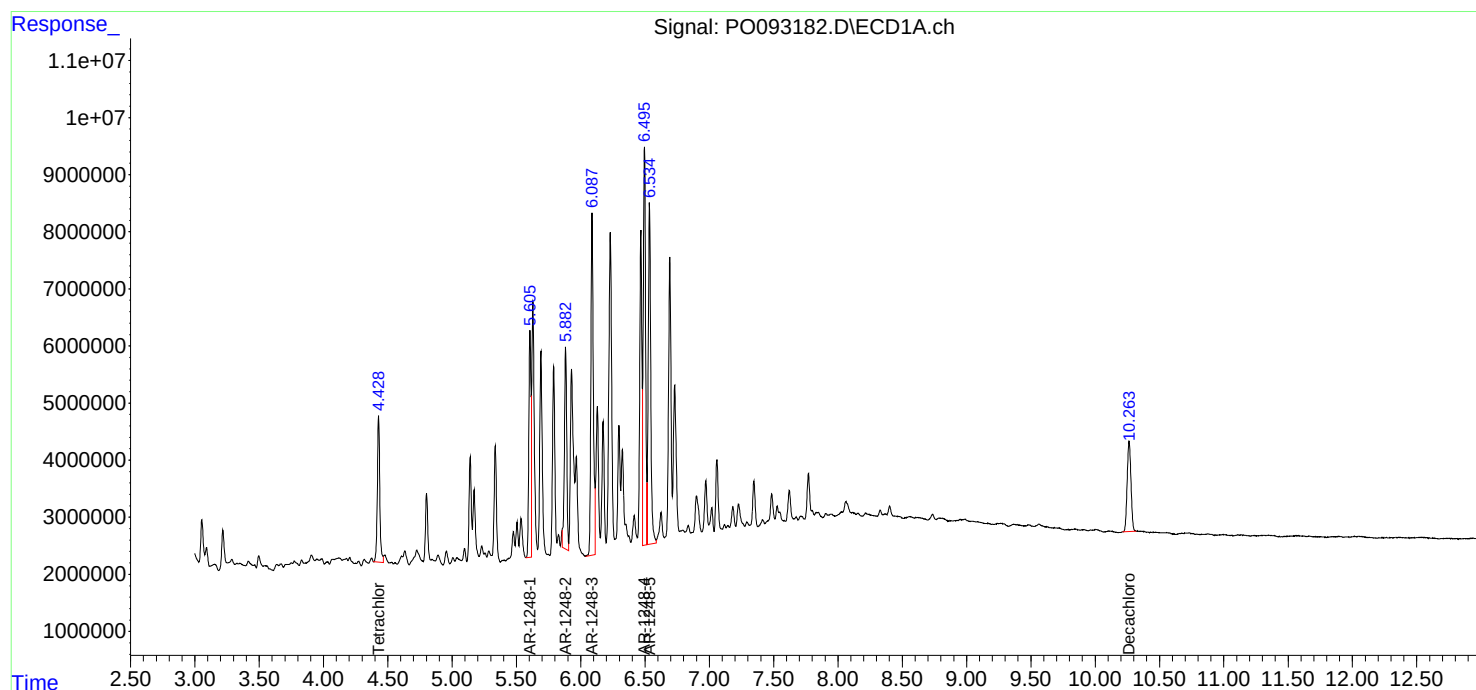

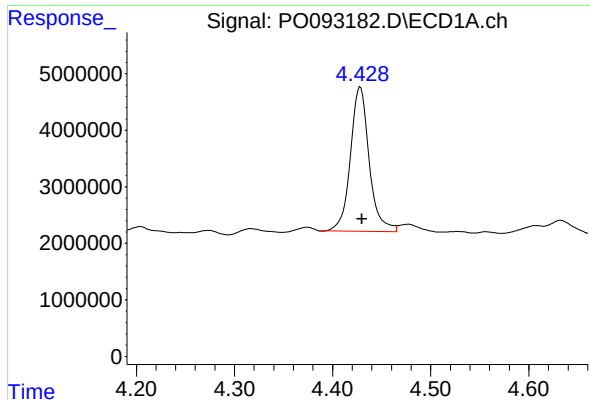


#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: -0.002 min
Response: 33800241
Conc: 10.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
33961DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/16/2023
Supervised By :Ankita Jodhani 03/16/2023

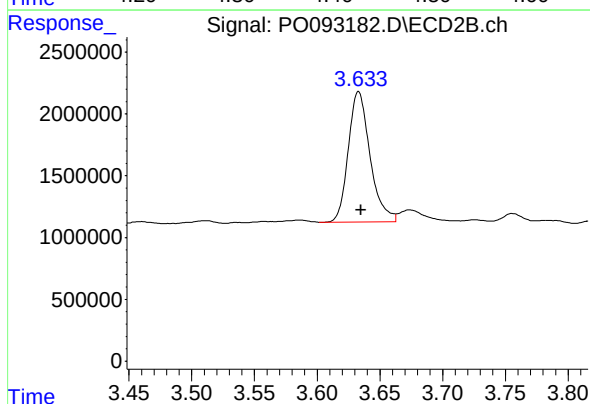


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.002 min
Response: 12752790
Conc: 11.31 ng/ml

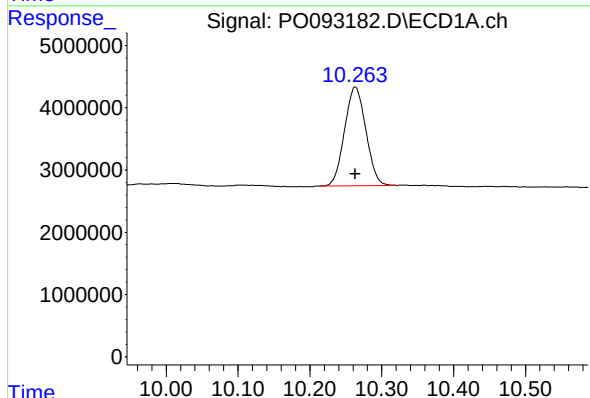


#2 Decachlorobiphenyl

R.T.: 10.263 min
Delta R.T.: 0.000 min
Response: 32617750
Conc: 15.07 ng/ml

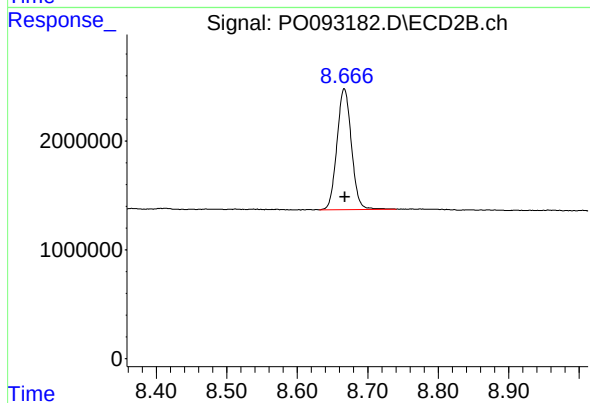

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.001 min
Response: 15860319
Conc: 16.20 ng/ml

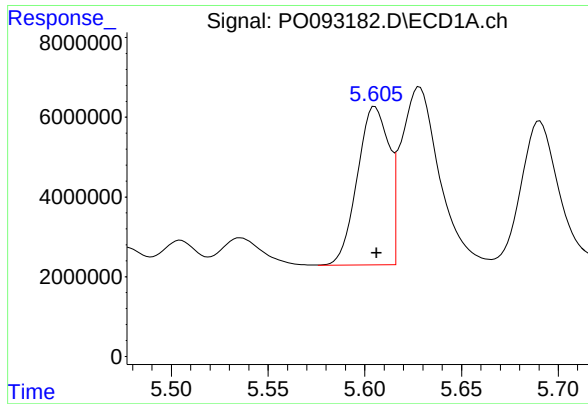


#21 AR-1248-1

R.T.: 5.605 min
Delta R.T.: 0.000 min
Response: 45268076
Conc: 728.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
33961DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/16/2023
Supervised By :Ankita Jodhani 03/16/2023

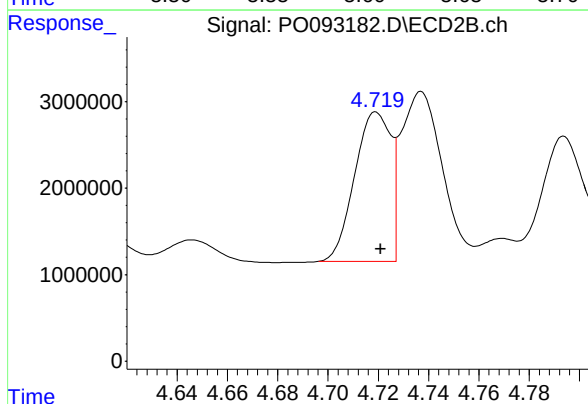


#21 AR-1248-1

R.T.: 4.719 min
Delta R.T.: -0.002 min
Response: 17208275
Conc: 739.45 ng/ml

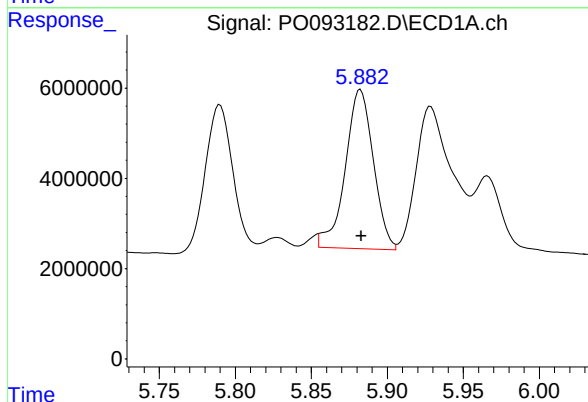


#22 AR-1248-2

R.T.: 5.882 min
Delta R.T.: -0.001 min
Response: 45457462
Conc: 475.95 ng/ml m

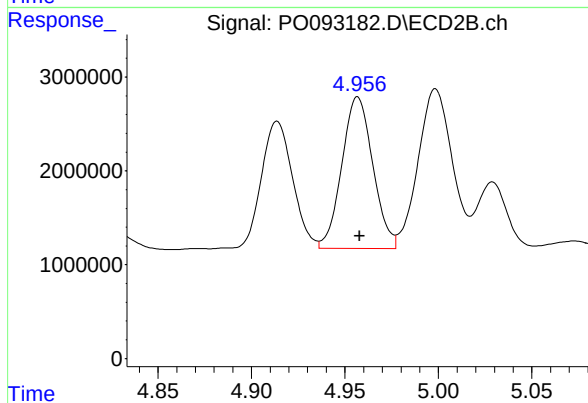

#22 AR-1248-2

R.T.: 4.957 min
Delta R.T.: -0.001 min
Response: 18649096
Conc: 514.59 ng/ml

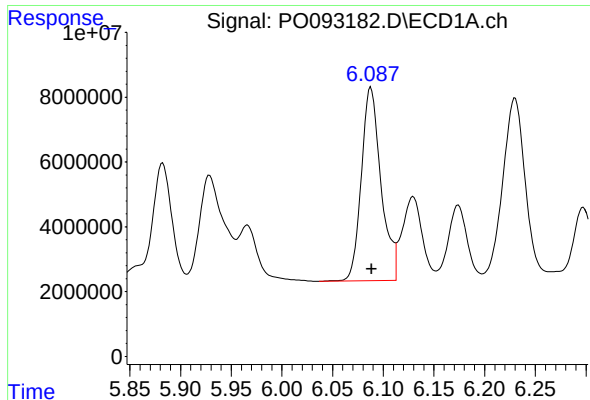


#23 AR-1248-3

R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 80452151
Conc: 773.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
33961DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/16/2023
Supervised By :Ankita Jodhani 03/16/2023

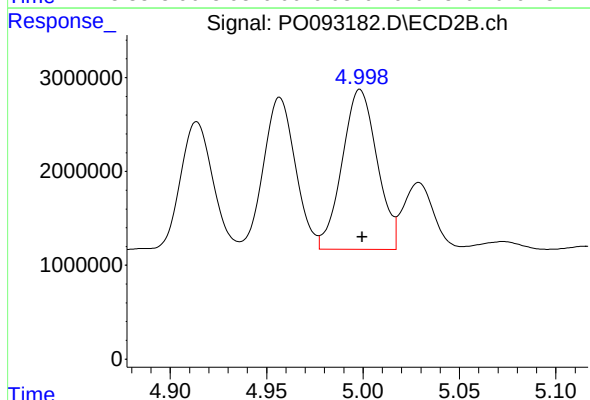


#23 AR-1248-3

R.T.: 4.998 min
Delta R.T.: -0.001 min
Response: 21605755
Conc: 575.74 ng/ml

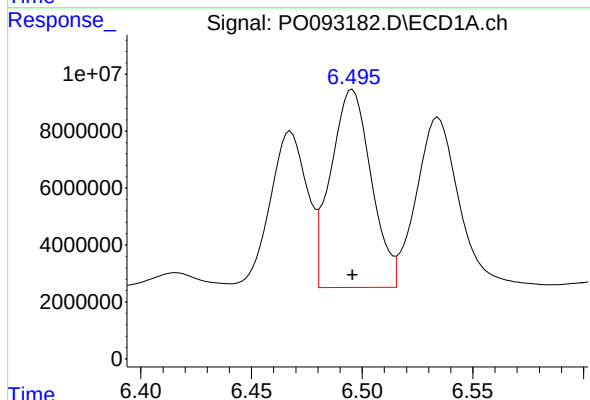


#24 AR-1248-4

R.T.: 6.496 min
Delta R.T.: 0.000 min
Response: 88661995
Conc: 870.68 ng/ml

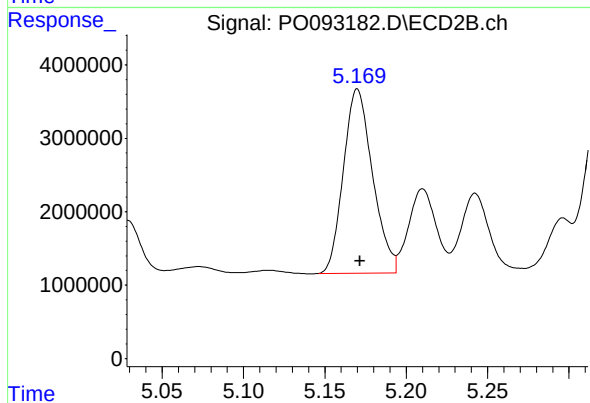

#24 AR-1248-4

R.T.: 5.170 min
Delta R.T.: -0.002 min
Response: 31311169
Conc: 727.80 ng/ml

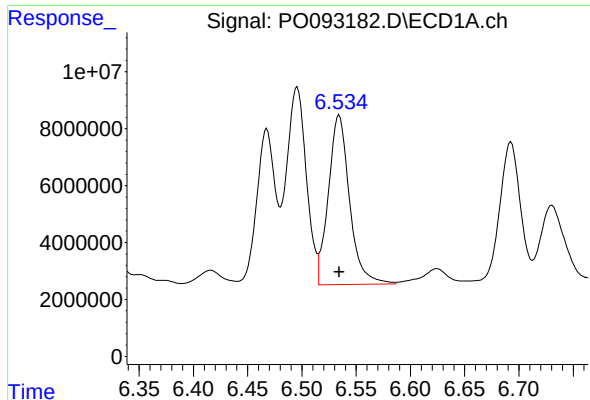


#25 AR-1248-5

R.T.: 6.534 min
Delta R.T.: 0.000 min
Response: 81054441
Conc: 791.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
33961DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/16/2023
Supervised By :Ankita Jodhani 03/16/2023

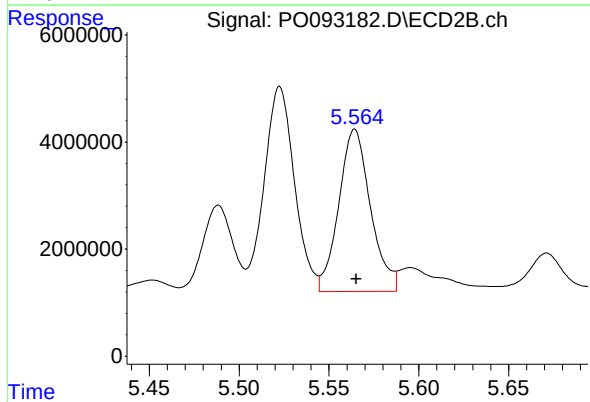

#25 AR-1248-5

R.T.: 5.564 min
Delta R.T.: 0.000 min
Response: 37204612
Conc: 1011.62 ng/ml