

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031523\
 Data File : P0093187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2023 21:10
 Operator : YP/AJ
 Sample : 01921-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RT3249

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/16/2023
 Supervised By :Ankita Jodhani 03/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 22:18:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.633	40773063	10279092	13.020	9.114m#
2) SA Decachlor...	10.262	8.663	47980518	21649997	22.169	22.111

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031523\
Data File : PO093187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2023 21:10
Operator : YP/AJ
Sample : 01921-02
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RT3249


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/16/2023
Supervised By :Ankita Jodhani 03/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 22:18:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

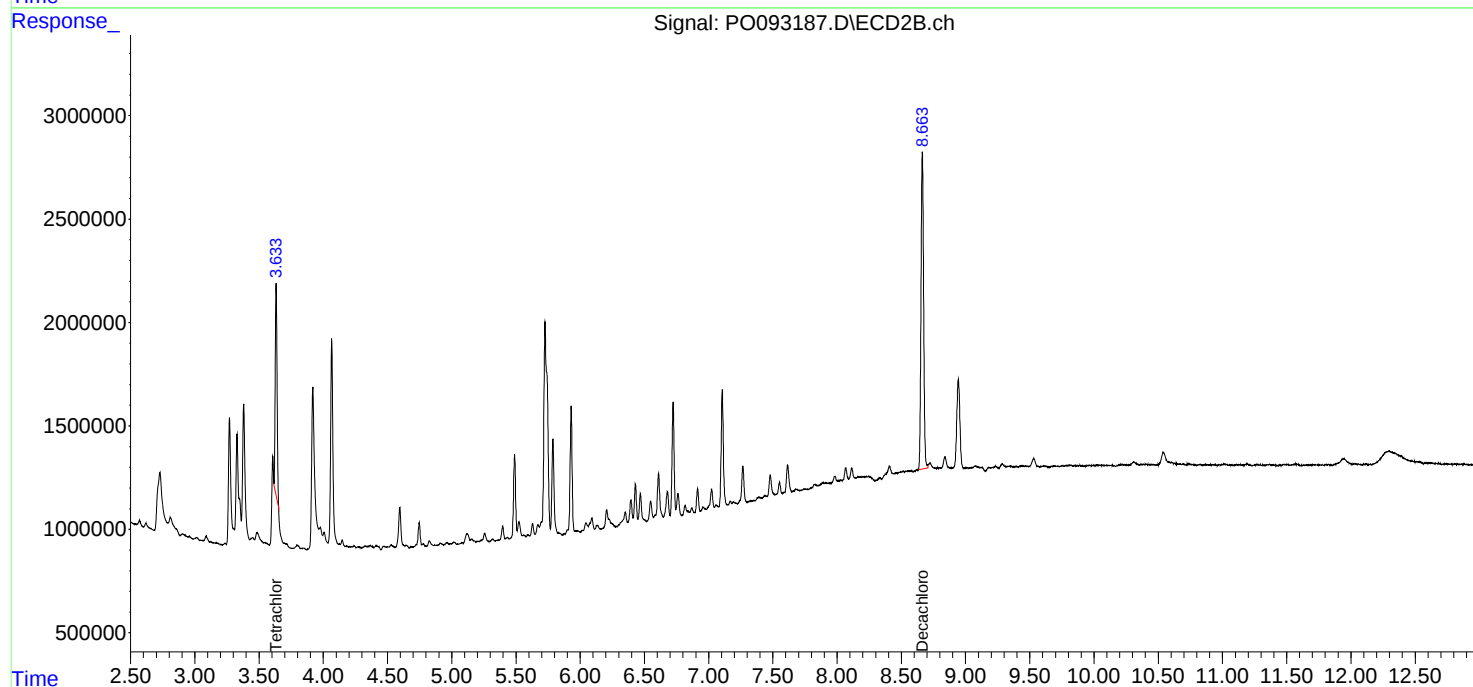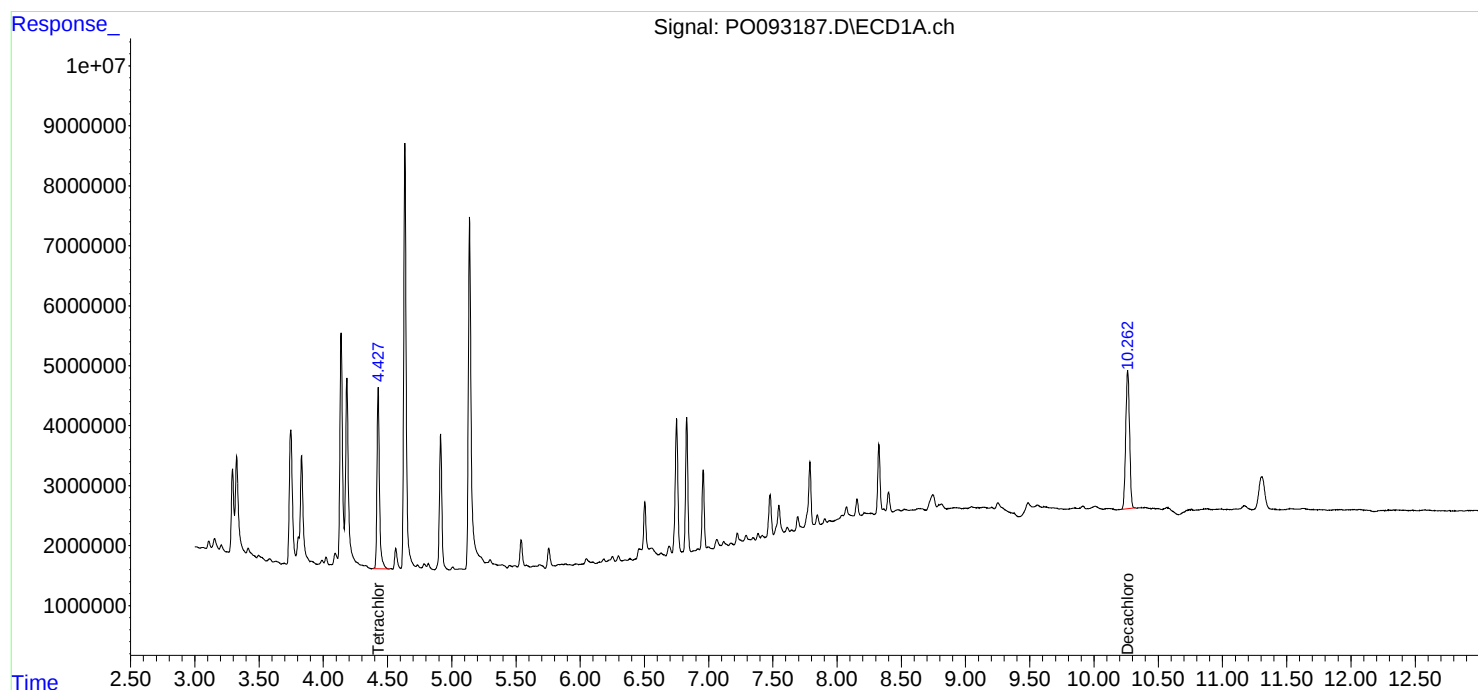

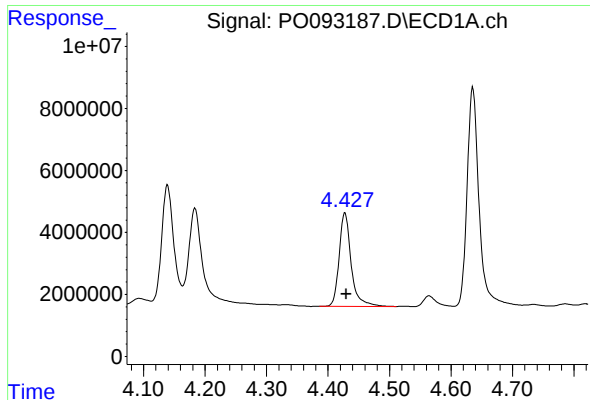


#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: -0.002 min
Response: 40773063
Conc: 13.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT3249


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/16/2023
Supervised By :Ankita Jodhani 03/16/2023

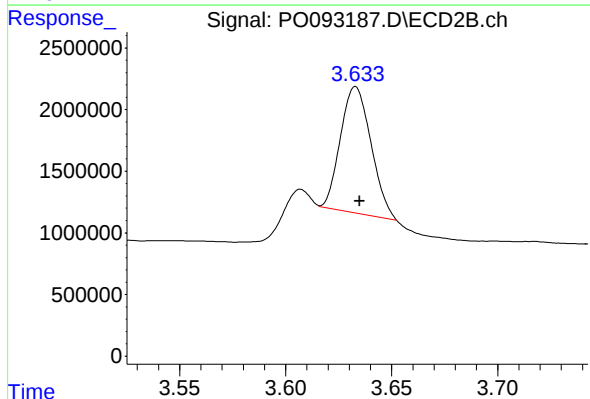


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.002 min
Response: 10279092
Conc: 9.11 ng/ml

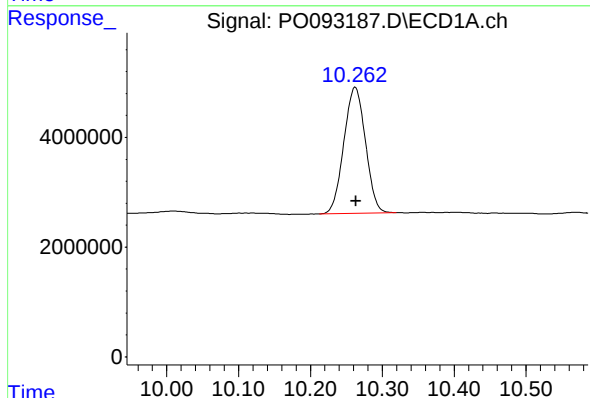

#2 Decachlorobiphenyl

R.T.: 10.262 min
Delta R.T.: 0.000 min
Response: 47980518
Conc: 22.17 ng/ml

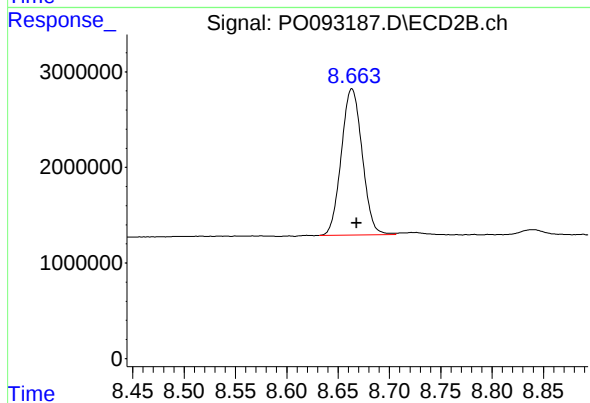

#2 Decachlorobiphenyl

R.T.: 8.663 min
Delta R.T.: -0.005 min
Response: 21649997
Conc: 22.11 ng/ml