

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031621\
 Data File : P0076201.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2021 13:47
 Operator : DD\AJ
 Sample : AR1262CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262CCC500

Manual Integrations
 APPROVED

Ankita
 3/17/2021 2:21:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 17:31:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.936	3248564	2300060	57.184	55.129
2) SA Decachlor...	10.921	9.202	2048866	1824004	53.268	47.503
Target Compounds						
36) L8 AR-1262-1	8.567	7.292	1344160	715370	454.316	489.847
37) L8 AR-1262-2	9.123	7.844	2329945	2402844	481.293	485.070
38) L8 AR-1262-3	9.431	8.130	1589612	1011169	480.994	470.667
39) L8 AR-1262-4	9.524	8.193	1204396	1803684	468.518m	476.881
40) L8 AR-1262-5	10.183	8.689	842040	829097	511.896	478.944

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031621\
Data File : P0076201.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2021 13:47
Operator : DD\AJ
Sample : AR1262CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/17/2021 2:21:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 17:31:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

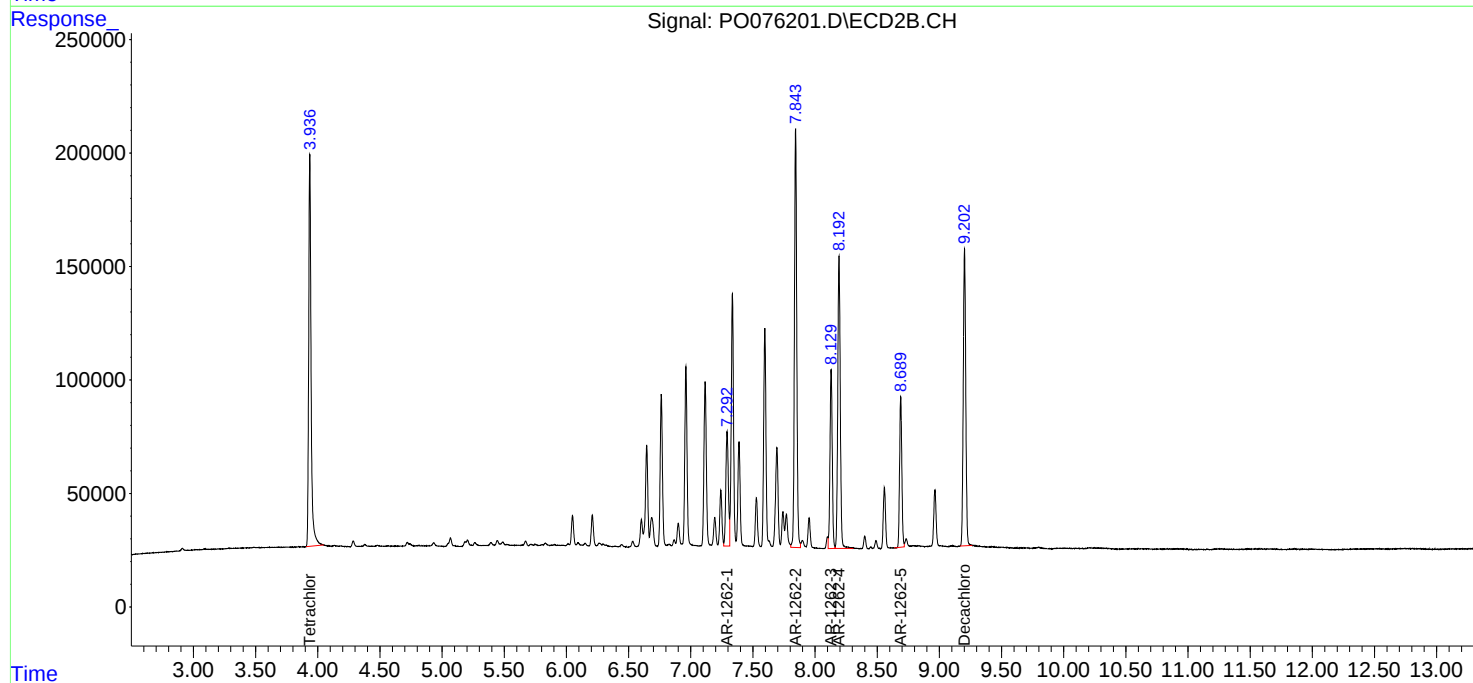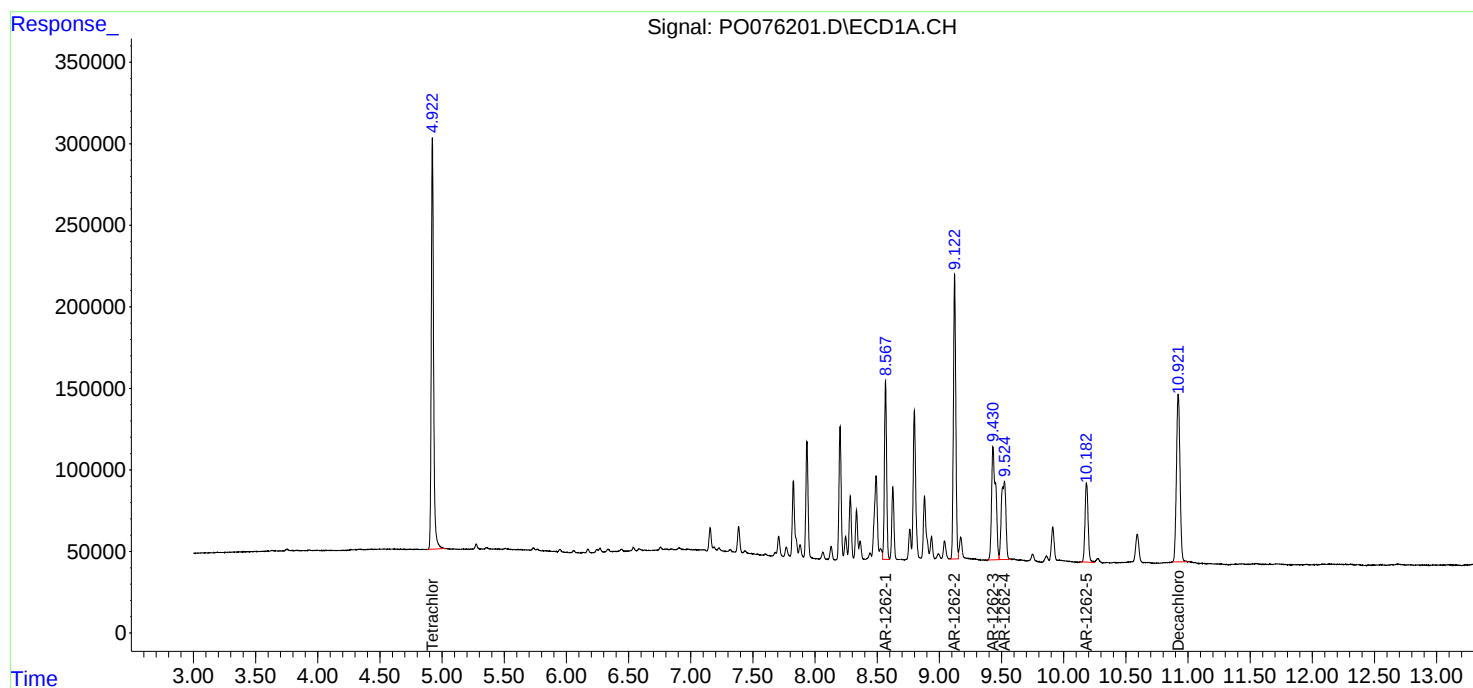

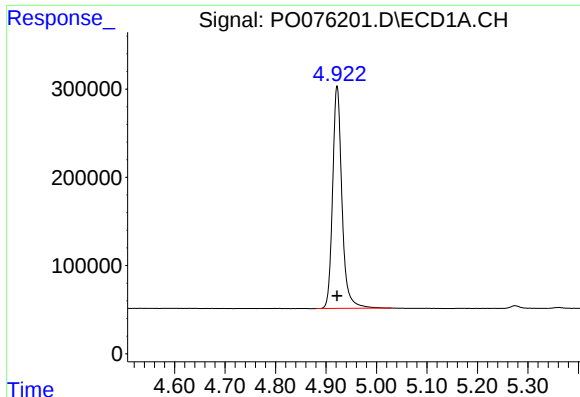


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 3248564
Conc: 57.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/17/2021 2:21:55 PM

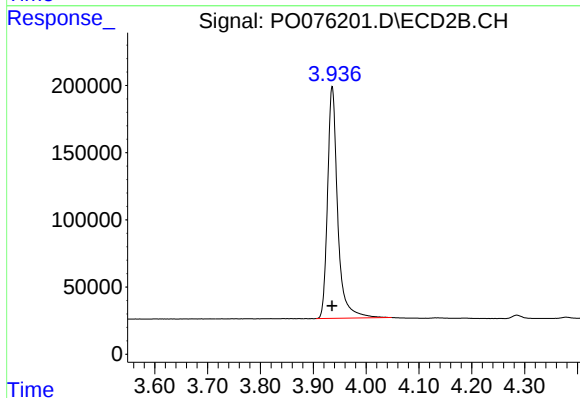


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 2300060
Conc: 55.13 ng/ml

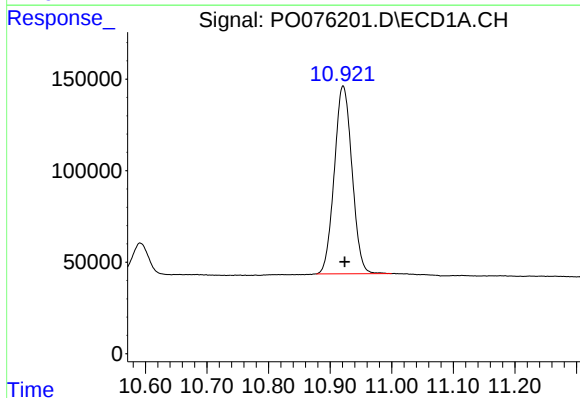


#2 Decachlorobiphenyl

R.T.: 10.921 min
Delta R.T.: -0.003 min
Response: 2048866
Conc: 53.27 ng/ml

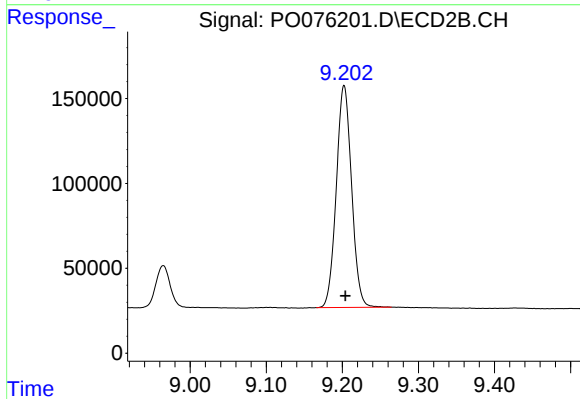

#2 Decachlorobiphenyl

R.T.: 9.202 min
Delta R.T.: -0.002 min
Response: 1824004
Conc: 47.50 ng/ml

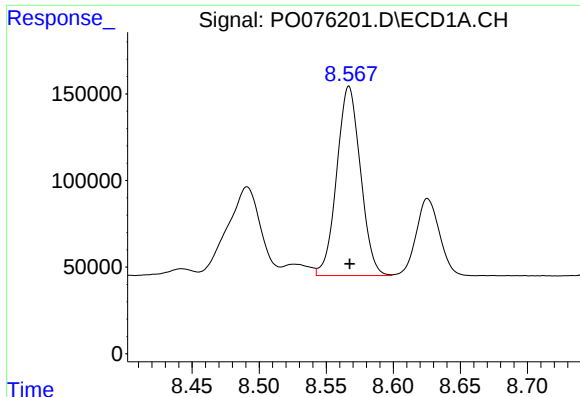


#36 AR-1262-1

R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 1344160
Conc: 454.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/17/2021 2:21:55 PM

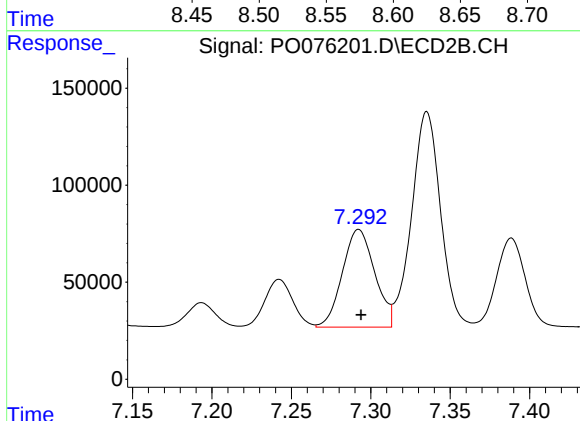


#36 AR-1262-1

R.T.: 7.292 min
Delta R.T.: -0.001 min
Response: 715370
Conc: 489.85 ng/ml

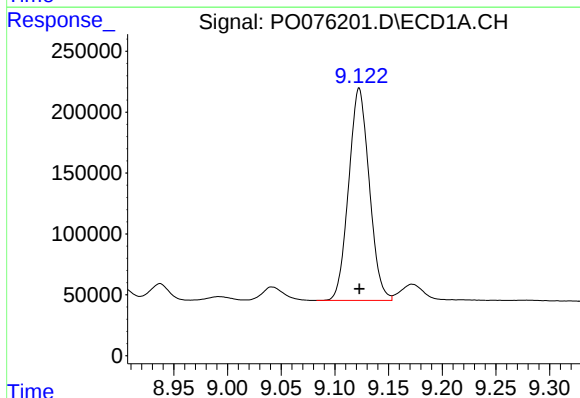


#37 AR-1262-2

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 2329945
Conc: 481.29 ng/ml

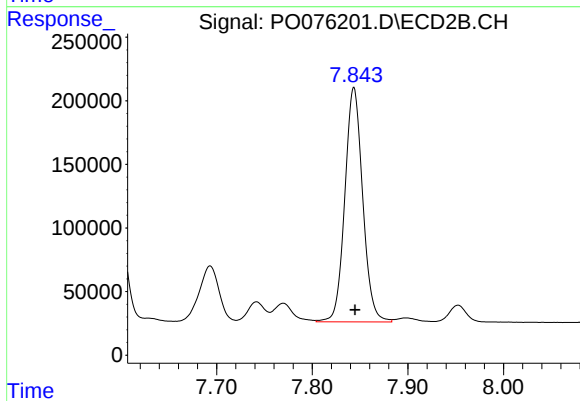

#37 AR-1262-2

R.T.: 7.844 min
Delta R.T.: -0.001 min
Response: 2402844
Conc: 485.07 ng/ml

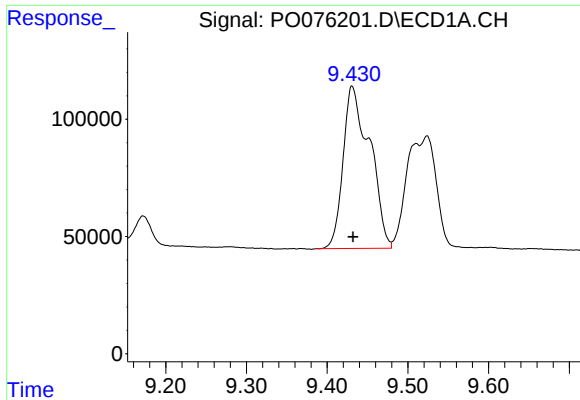


#38 AR-1262-3

R.T.: 9.431 min
Delta R.T.: -0.001 min
Response: 1589612
Conc: 480.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500


Manual Integrations
APPROVED

Ankita
3/17/2021 2:21:55 PM

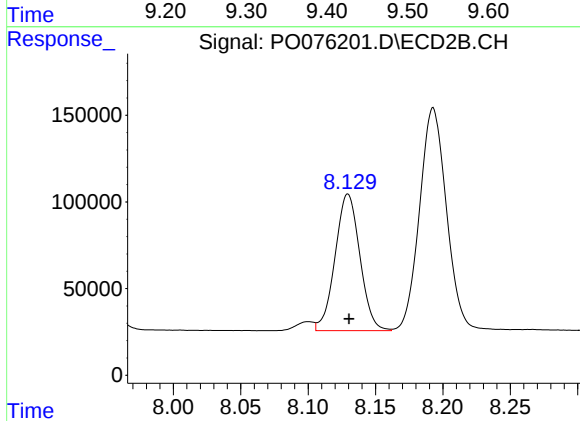


#38 AR-1262-3

R.T.: 8.130 min
Delta R.T.: 0.000 min
Response: 1011169
Conc: 470.67 ng/ml

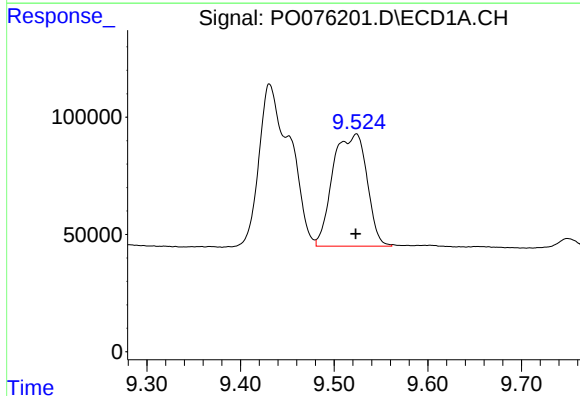


#39 AR-1262-4

R.T.: 9.524 min
Delta R.T.: 0.000 min
Response: 1204396
Conc: 468.52 ng/ml m

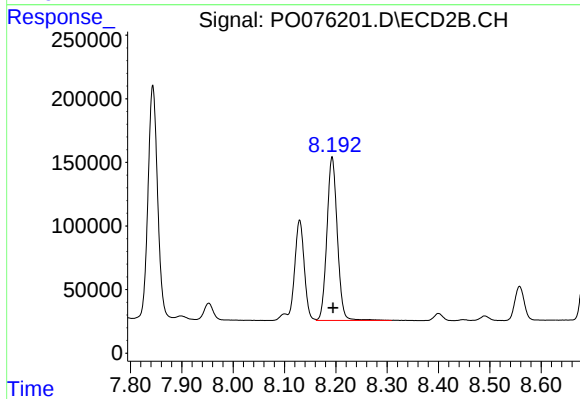

#39 AR-1262-4

R.T.: 8.193 min
Delta R.T.: -0.001 min
Response: 1803684
Conc: 476.88 ng/ml

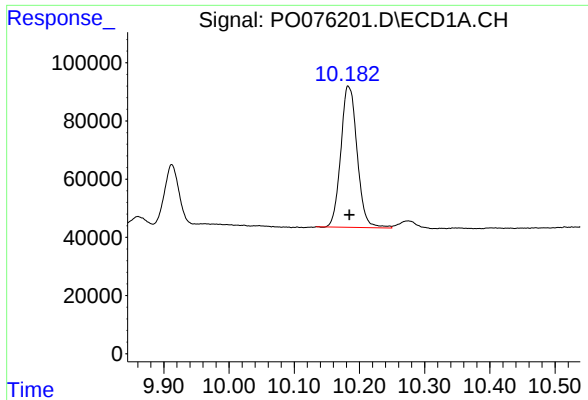


#40 AR-1262-5

R.T.: 10.183 min
Delta R.T.: -0.002 min
Response: 842040
Conc: 511.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262CCC500

Manual Integrations
APPROVED

Ankita
3/17/2021 2:21:55 PM

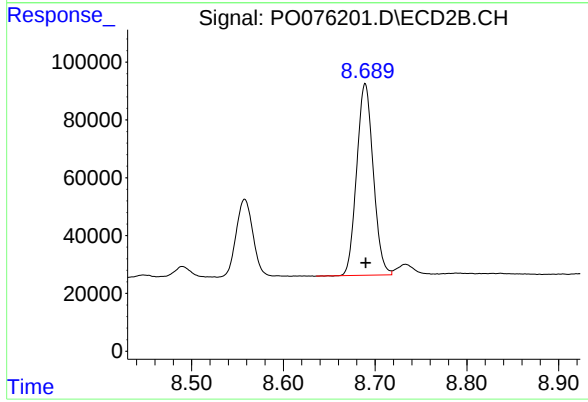

#40 AR-1262-5

R.T.: 8.689 min
Delta R.T.: 0.000 min
Response: 829097
Conc: 478.94 ng/ml