

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031622\
 Data File : P0085422.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2022 23:14
 Operator : YP\AJ
 Sample : N1943-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DF1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:09:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.590	4306259	1059104	21.060	24.721
2) SA Decachlor...	10.394	8.604	2295576	725441	19.097	18.895

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031622\
Data File : P0085422.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2022 23:14
Operator : YP\AJ
Sample : N1943-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DF1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:09:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

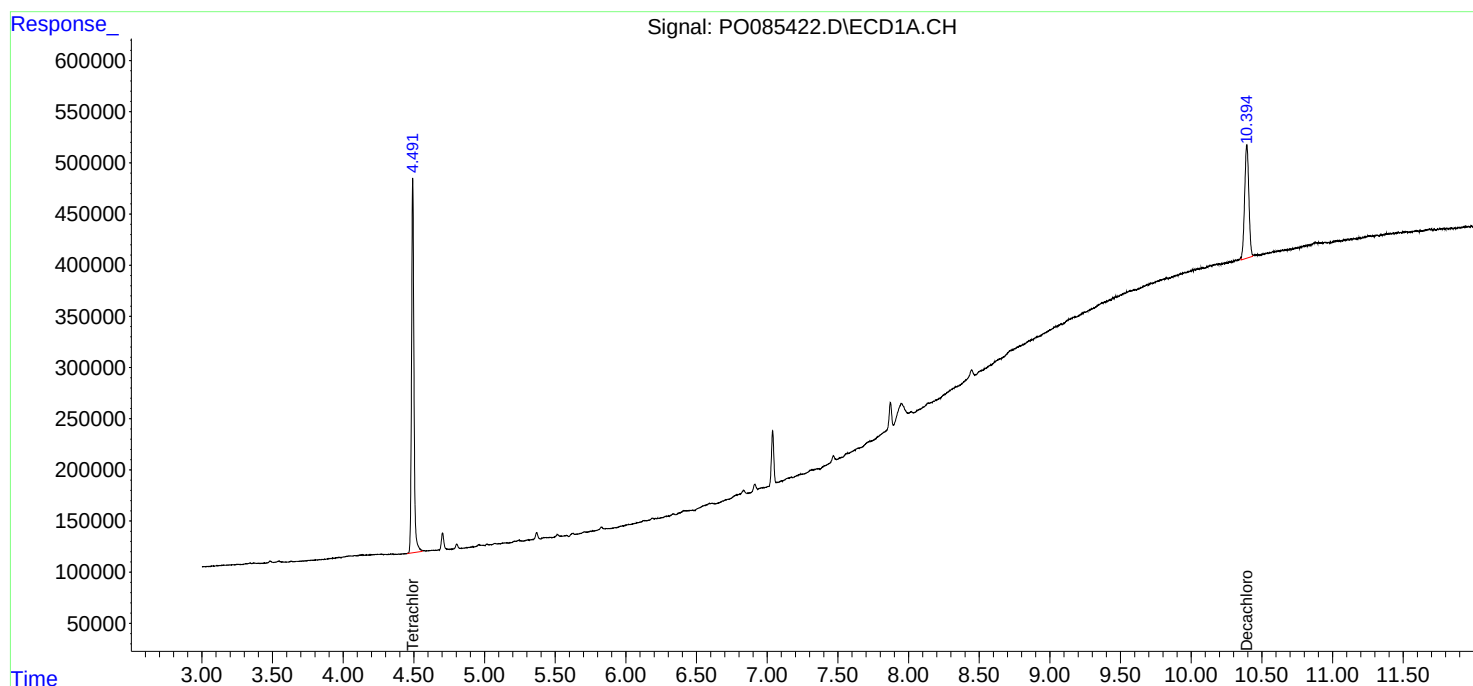


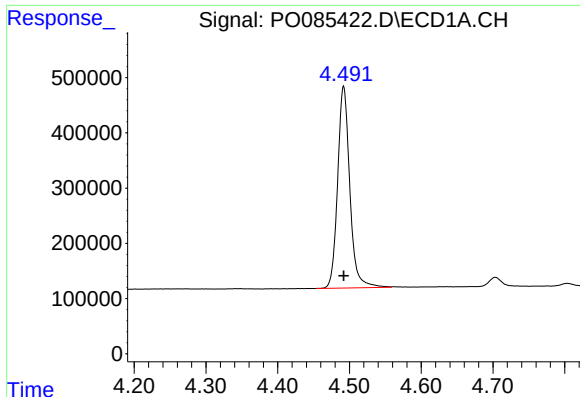

#1 Tetrachloro-m-xylene


R.T.: 4.492 min
Delta R.T.: 0.000 min
Response: 4306259
Conc: 21.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
DF1

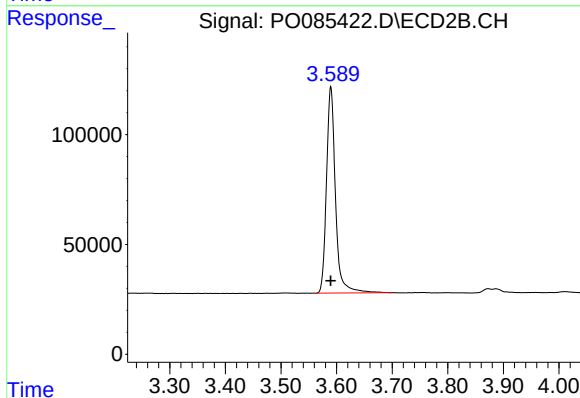


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: 0.000 min
Response: 1059104
Conc: 24.72 ng/ml

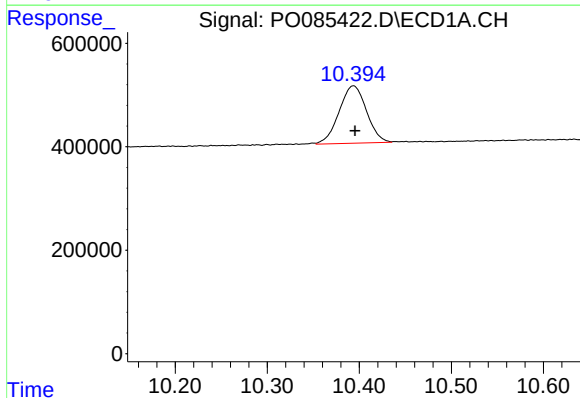

#2 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: -0.002 min
Response: 2295576
Conc: 19.10 ng/ml

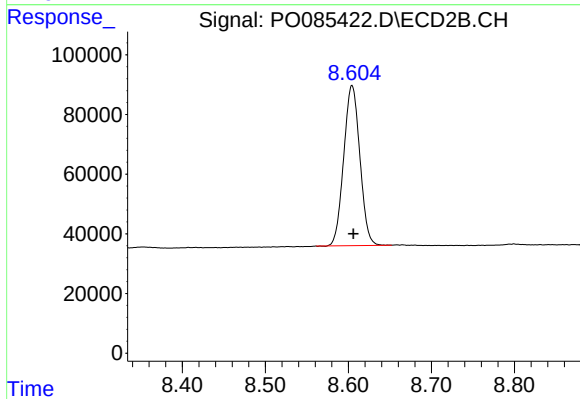

#2 Decachlorobiphenyl

R.T.: 8.604 min
Delta R.T.: -0.002 min
Response: 725441
Conc: 18.90 ng/ml