

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031622\
 Data File : P0085424.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Mar 2022 23:46
 Operator : YP\AJ
 Sample : N1956-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TPK-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2022
 Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:10:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.590	4271398	1078243	20.889	25.167
2) SA Decachlor...	10.393	8.605	2535808	715784	21.095	18.644
Target Compounds						
31) L7 AR-1260-1	7.305	6.163	1193749	449000	173.007	189.385
32) L7 AR-1260-2	7.564	6.353	1482269	546242	189.485	195.674
33) L7 AR-1260-3	7.930	6.505	1722938	441077	293.335m	167.762 #
34) L7 AR-1260-4	8.159	6.979	1107201	337130	160.301	150.517
35) L7 AR-1260-5	8.492	7.223	1961639	731227	139.627	145.148

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031622\
Data File : P0085424.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Mar 2022 23:46
Operator : YP\AJ
Sample : N1956-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TPK-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:10:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

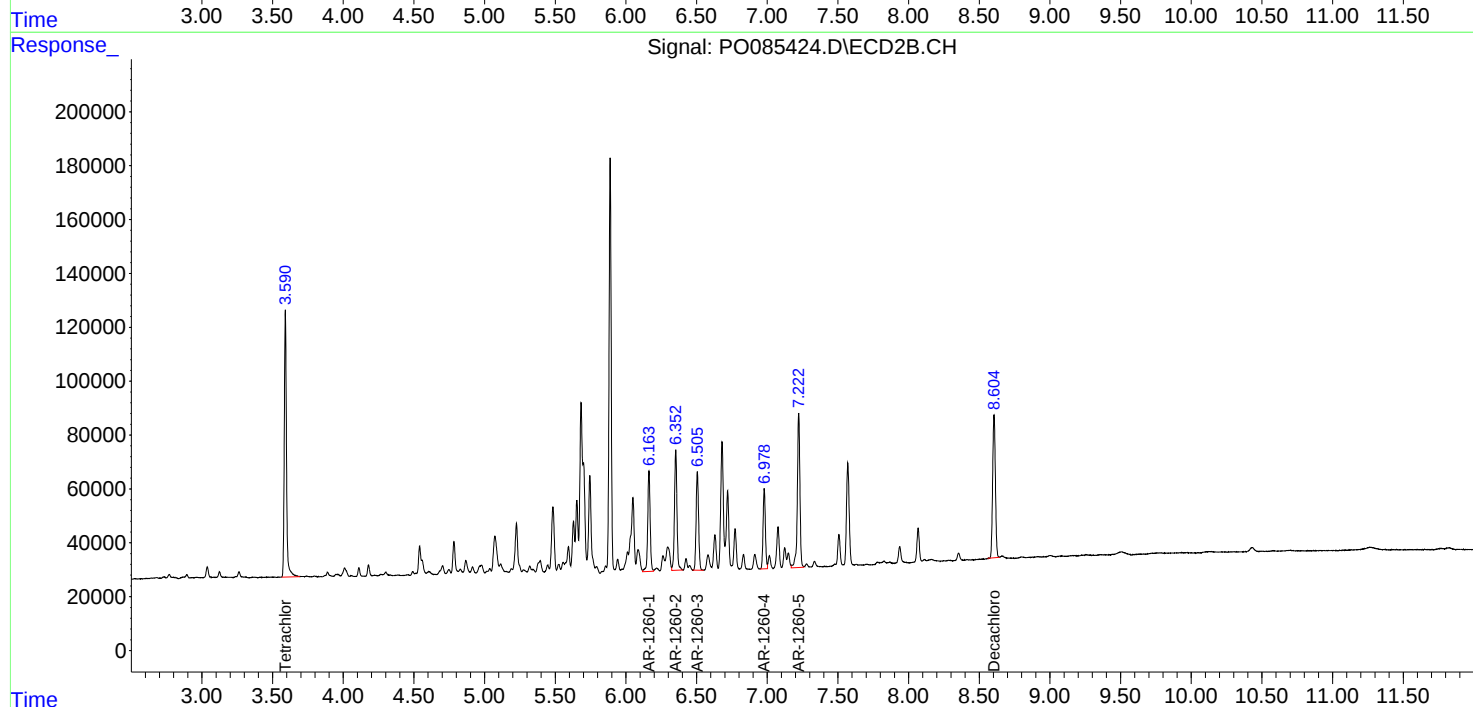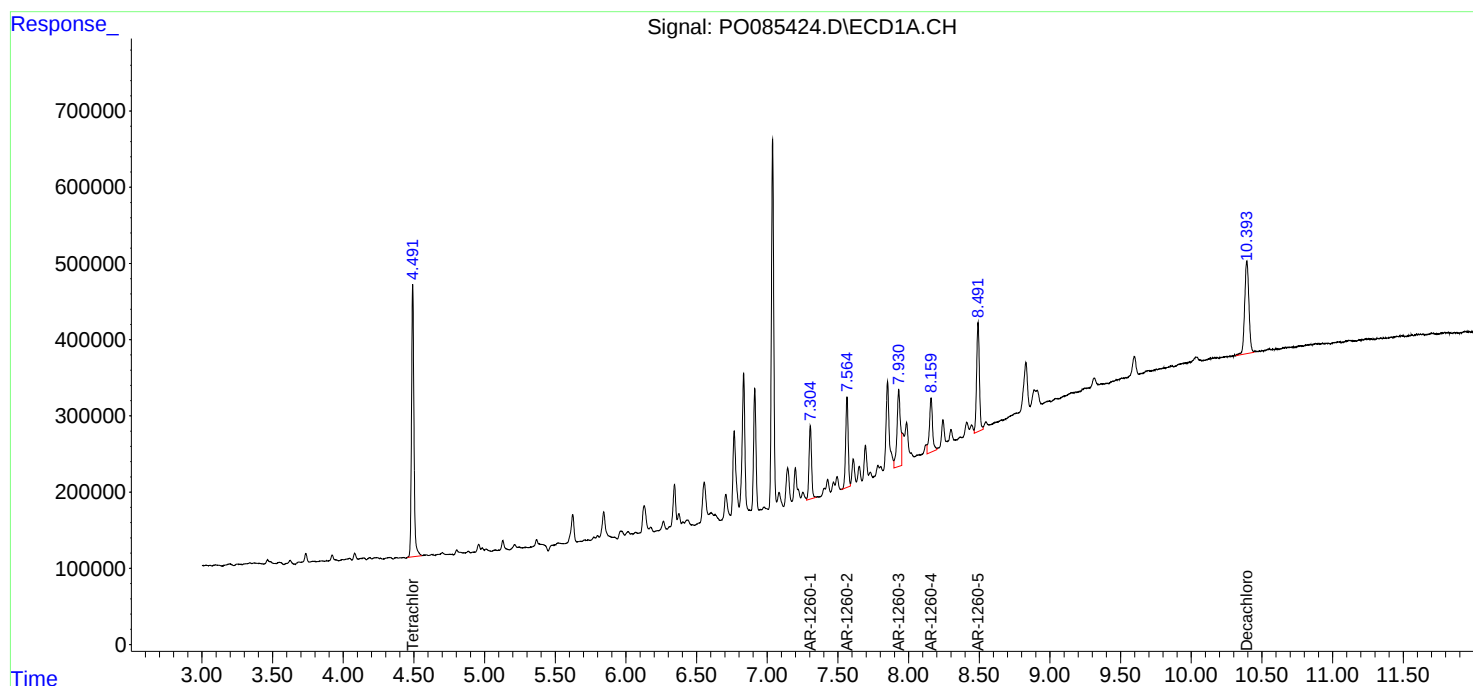

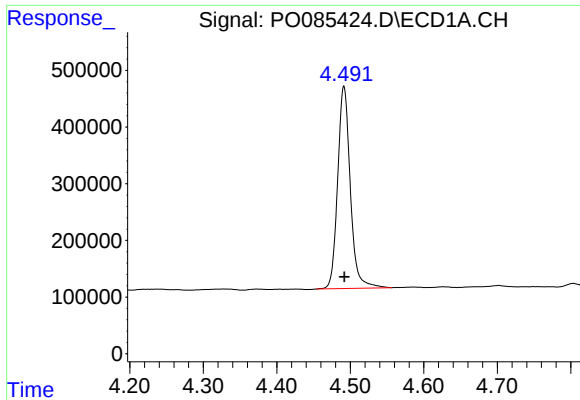


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: 0.000 min
Response: 4271398
Conc: 20.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

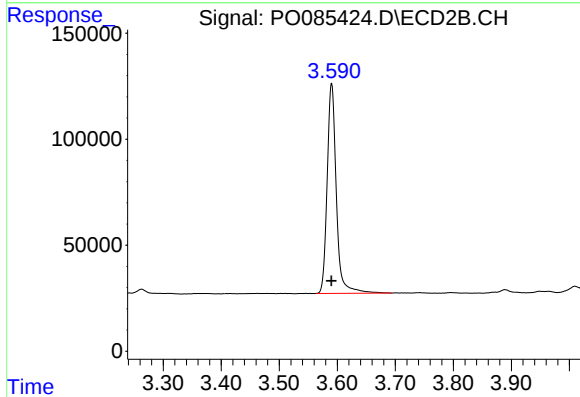


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: 0.000 min
Response: 1078243
Conc: 25.17 ng/ml

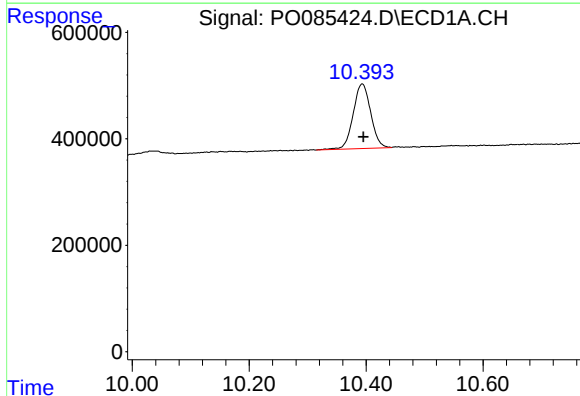


#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: -0.002 min
Response: 2535808
Conc: 21.10 ng/ml

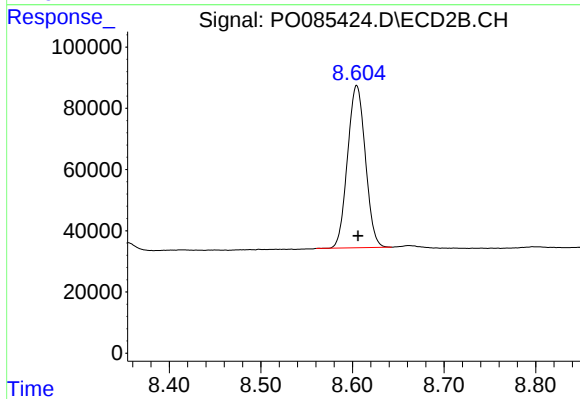

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: -0.002 min
Response: 715784
Conc: 18.64 ng/ml

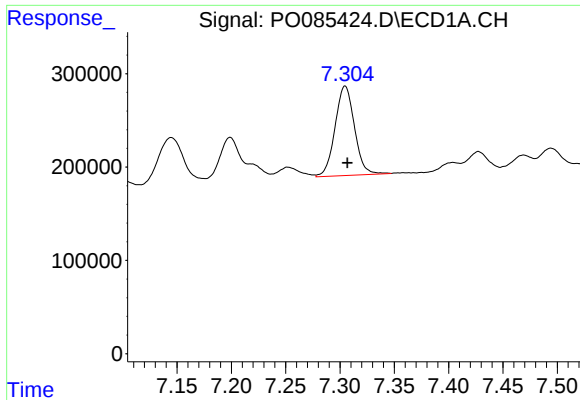


#31 AR-1260-1

R.T.: 7.305 min
Delta R.T.: -0.002 min
Response: 1193749
Conc: 173.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

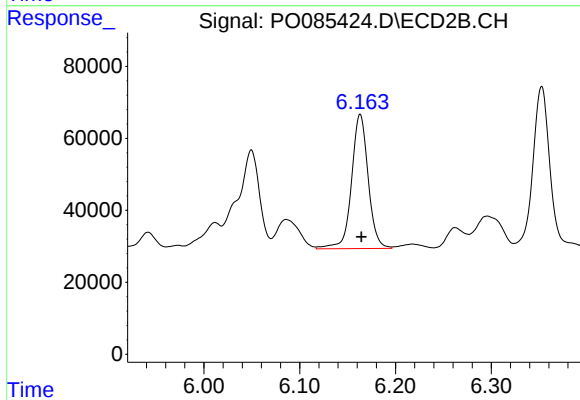


#31 AR-1260-1

R.T.: 6.163 min
Delta R.T.: -0.001 min
Response: 449000
Conc: 189.39 ng/ml

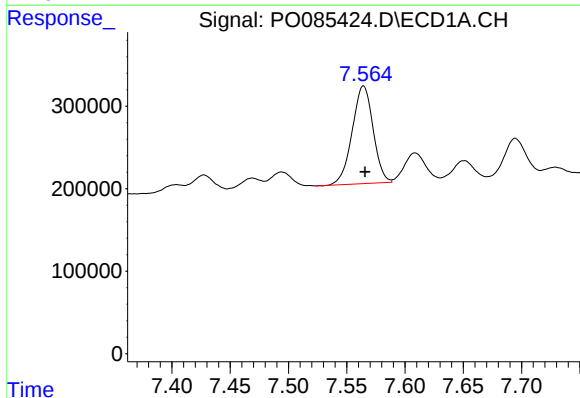


#32 AR-1260-2

R.T.: 7.564 min
Delta R.T.: -0.001 min
Response: 1482269
Conc: 189.48 ng/ml

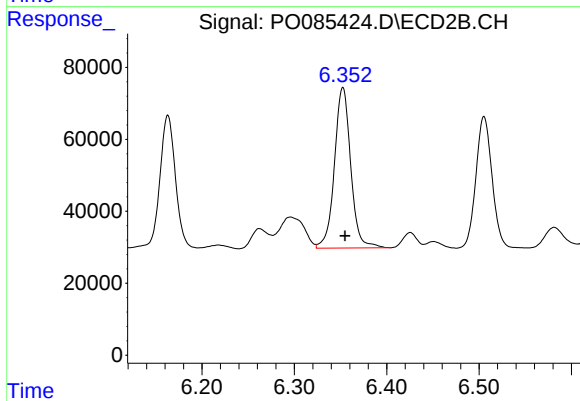

#32 AR-1260-2

R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 546242
Conc: 195.67 ng/ml

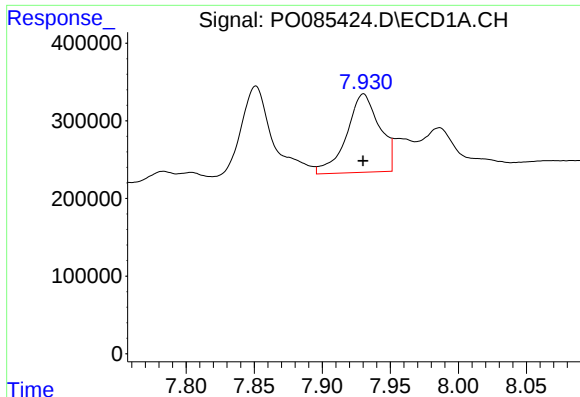


#33 AR-1260-3

R.T.: 7.930 min
Delta R.T.: 0.000 min
Response: 1722938
Conc: 293.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

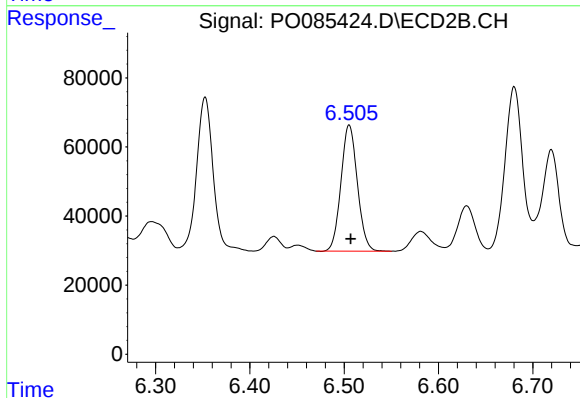


#33 AR-1260-3

R.T.: 6.505 min
Delta R.T.: -0.002 min
Response: 441077
Conc: 167.76 ng/ml

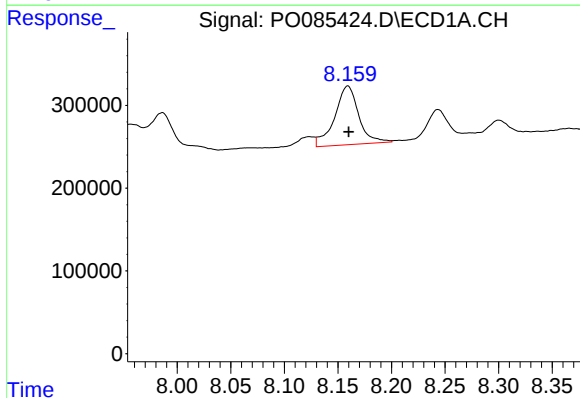


#34 AR-1260-4

R.T.: 8.159 min
Delta R.T.: 0.000 min
Response: 1107201
Conc: 160.30 ng/ml

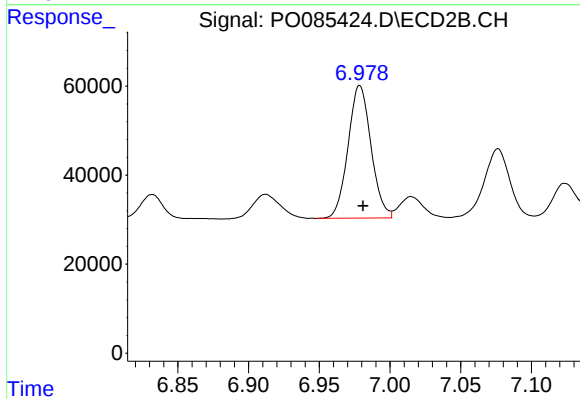

#34 AR-1260-4

R.T.: 6.979 min
Delta R.T.: -0.002 min
Response: 337130
Conc: 150.52 ng/ml

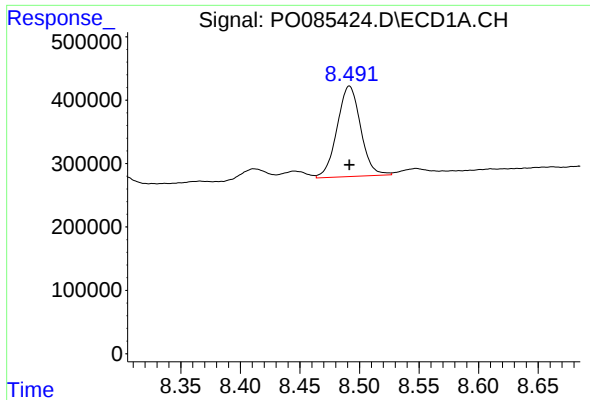


#35 AR-1260-5

R.T.: 8.492 min
Delta R.T.: 0.000 min
Response: 1961639
Conc: 139.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

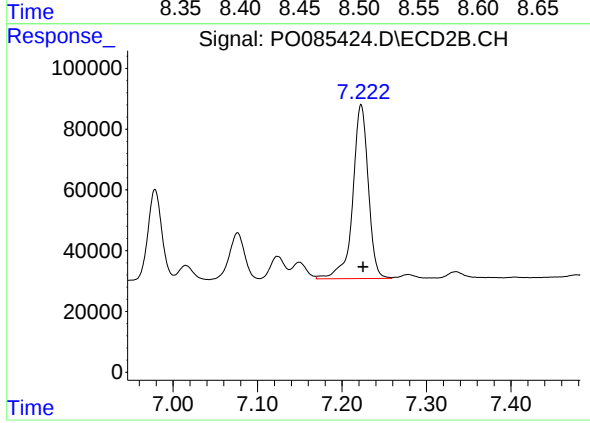

#35 AR-1260-5

R.T.: 7.223 min
Delta R.T.: -0.002 min
Response: 731227
Conc: 145.15 ng/ml