

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031622\
 Data File : P0085425.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2022 00:02
 Operator : YP\AJ
 Sample : N1956-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TPK-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2022
 Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:11:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.590	3779009	986823	18.481	23.034
2) SA Decachlor...	10.392	8.605	2436858	677246	20.272	17.640
Target Compounds						
31) L7 AR-1260-1	7.305	6.163	528585	203258	76.607	85.733
32) L7 AR-1260-2	7.563	6.352	691527	212361	88.401	76.072m
33) L7 AR-1260-3	7.930	6.505	425651	171330	72.468	65.164
34) L7 AR-1260-4	8.160	6.978	458356	134970	66.361m	60.260
35) L7 AR-1260-5	8.490	7.222	851355	299730	60.598	59.496

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031622\
Data File : P0085425.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2022 00:02
Operator : YP\AJ
Sample : N1956-02
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TPK-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:11:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

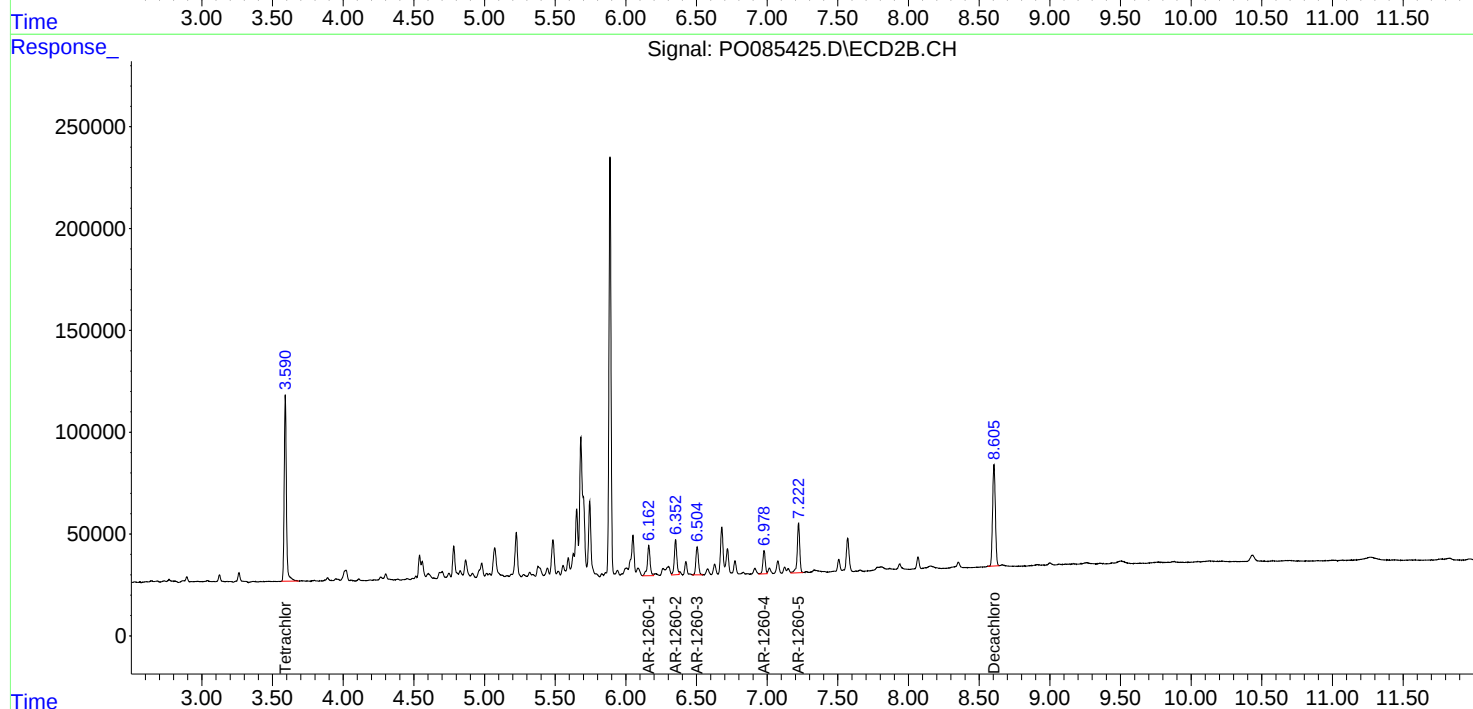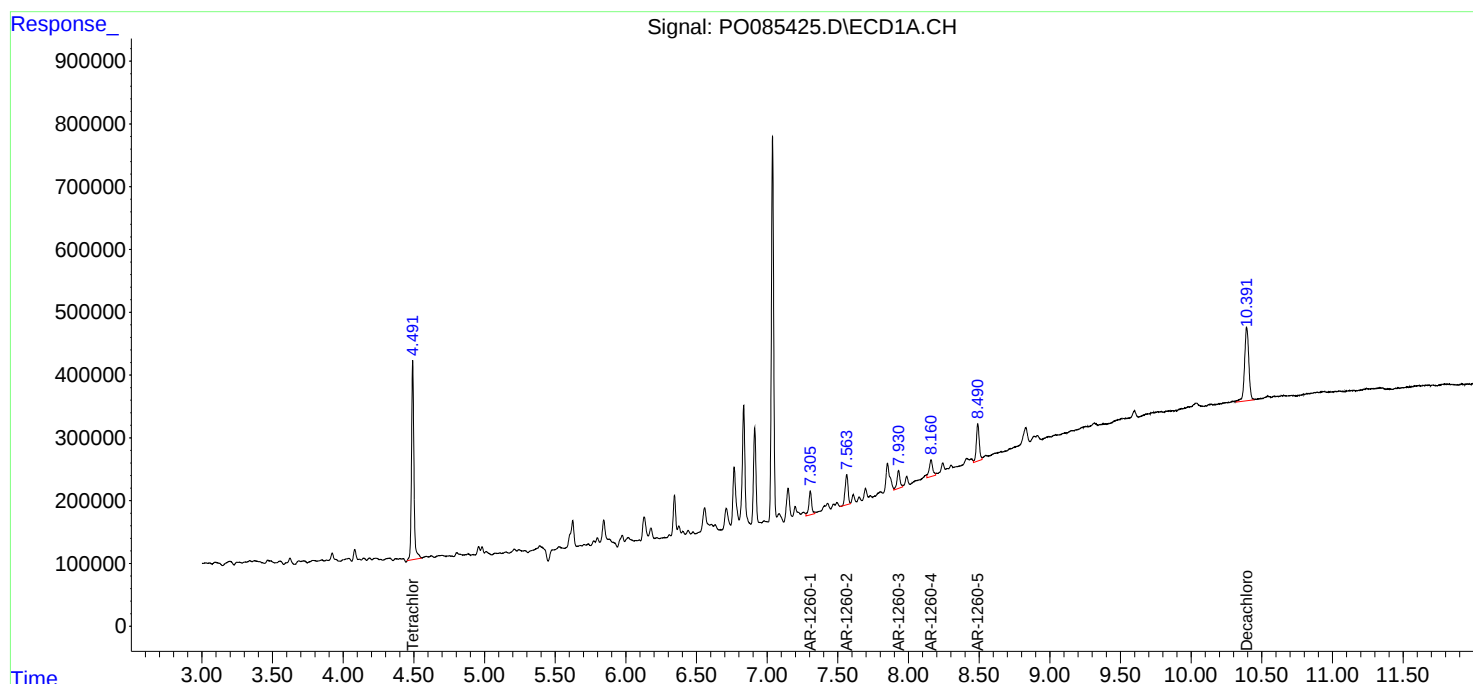

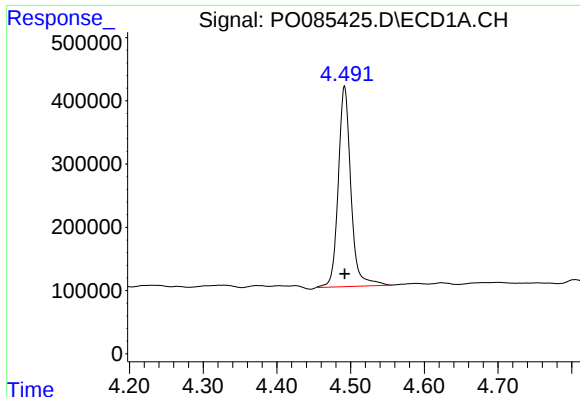


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: 0.000 min
Response: 3779009
Conc: 18.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

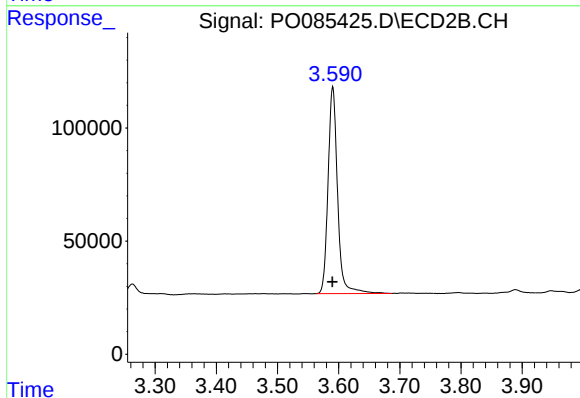


#1 Tetrachloro-m-xylene

R.T.: 3.590 min
Delta R.T.: 0.000 min
Response: 986823
Conc: 23.03 ng/ml

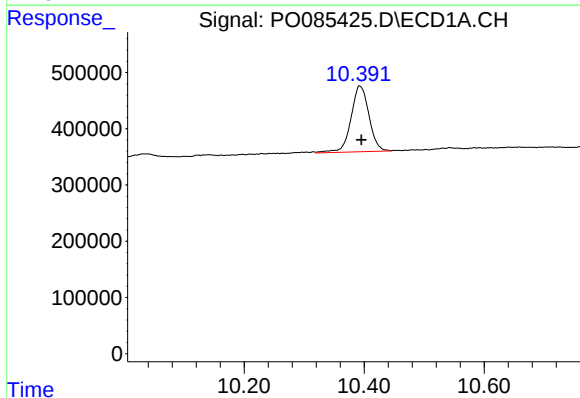


#2 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.003 min
Response: 2436858
Conc: 20.27 ng/ml

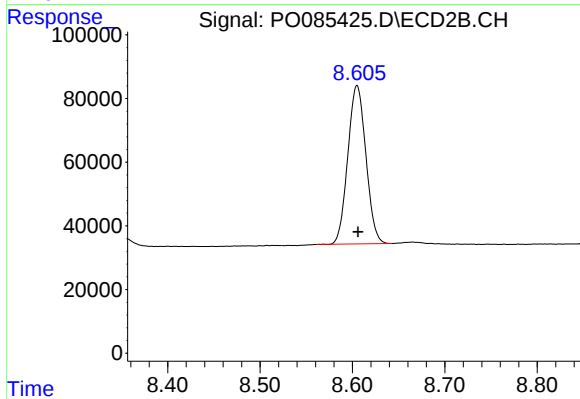

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: -0.001 min
Response: 677246
Conc: 17.64 ng/ml

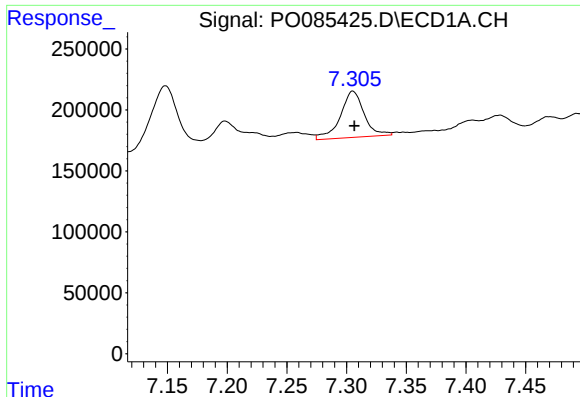


#31 AR-1260-1

R.T.: 7.305 min
Delta R.T.: -0.001 min
Response: 528585
Conc: 76.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

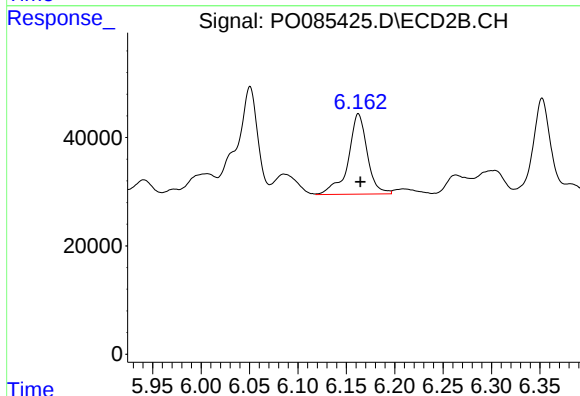


#31 AR-1260-1

R.T.: 6.163 min
Delta R.T.: -0.002 min
Response: 203258
Conc: 85.73 ng/ml

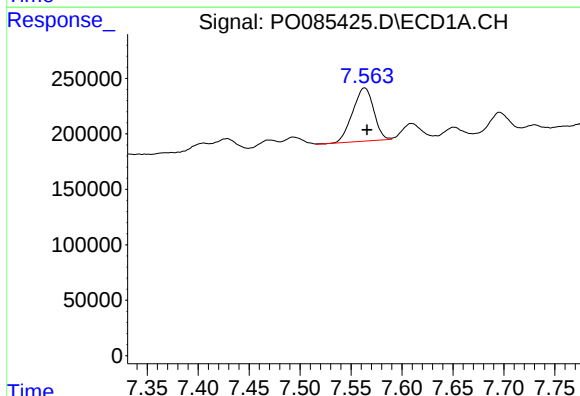


#32 AR-1260-2

R.T.: 7.563 min
Delta R.T.: -0.002 min
Response: 691527
Conc: 88.40 ng/ml

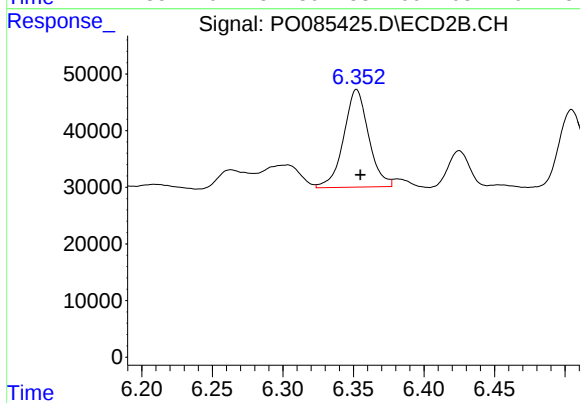

#32 AR-1260-2

R.T.: 6.352 min
Delta R.T.: -0.003 min
Response: 212361
Conc: 76.07 ng/ml m

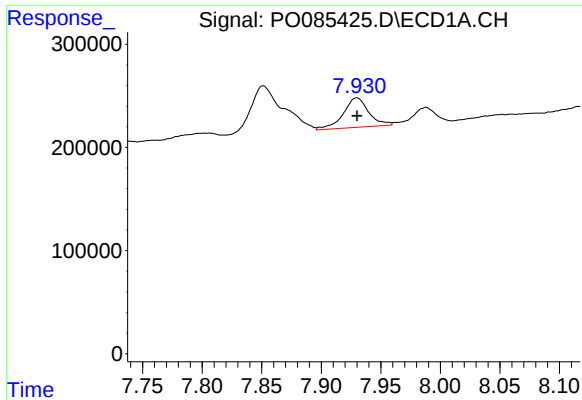


#33 AR-1260-3

R.T.: 7.930 min
Delta R.T.: 0.000 min
Response: 425651
Conc: 72.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

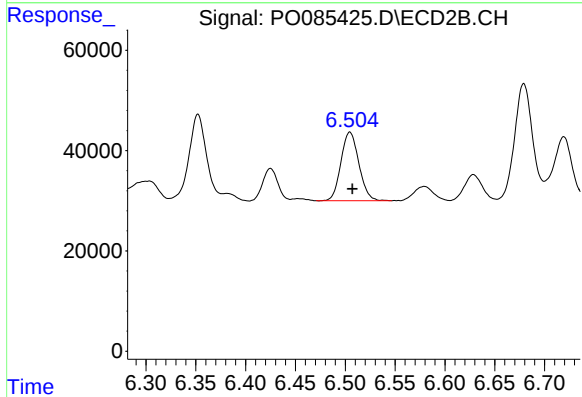


#33 AR-1260-3

R.T.: 6.505 min
Delta R.T.: -0.002 min
Response: 171330
Conc: 65.16 ng/ml

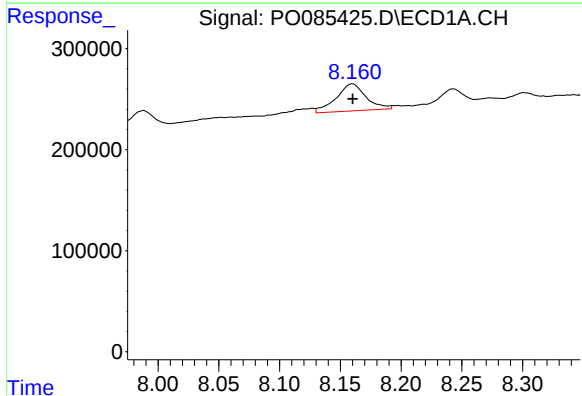


#34 AR-1260-4

R.T.: 8.160 min
Delta R.T.: 0.000 min
Response: 458356
Conc: 66.36 ng/ml m

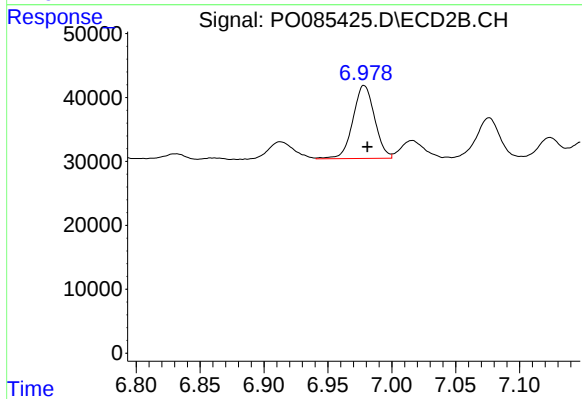

#34 AR-1260-4

R.T.: 6.978 min
Delta R.T.: -0.002 min
Response: 134970
Conc: 60.26 ng/ml

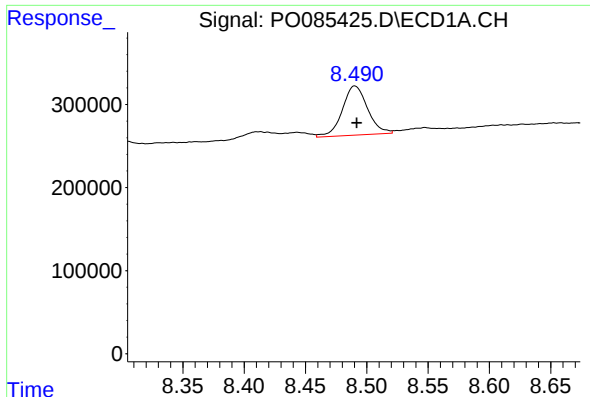


#35 AR-1260-5

R.T.: 8.490 min
Delta R.T.: -0.001 min
Response: 851355
Conc: 60.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

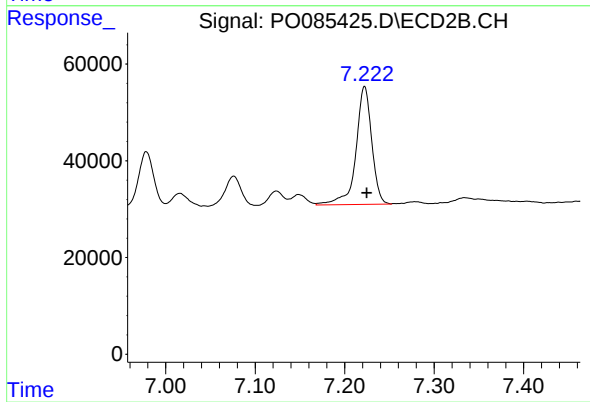

#35 AR-1260-5

R.T.: 7.222 min
Delta R.T.: -0.003 min
Response: 299730
Conc: 59.50 ng/ml