

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031622\
 Data File : P0085426.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2022 00:18
 Operator : YP\AJ
 Sample : N1956-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TPK-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2022
 Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:11:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.591	3656116	1003505	17.880	23.423 #
2) SA Decachlor...	10.394	8.604	2365972	683474	19.683	17.802
Target Compounds						
26) L6 AR-1254-1	6.550	5.481	354274	149683	53.457	56.952
27) L6 AR-1254-2	6.768	5.629	696188	126904	69.565	54.386
28) L6 AR-1254-3	7.141	6.031	493341	152109	47.937	41.415m
29) L6 AR-1254-4	7.426	6.261	198894	74921	28.349m	33.823
30) L6 AR-1254-5	7.852	6.680	474186	187159	61.972	57.538

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031622\
Data File : PO085426.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2022 00:18
Operator : YP\AJ
Sample : N1956-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TPK-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:11:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

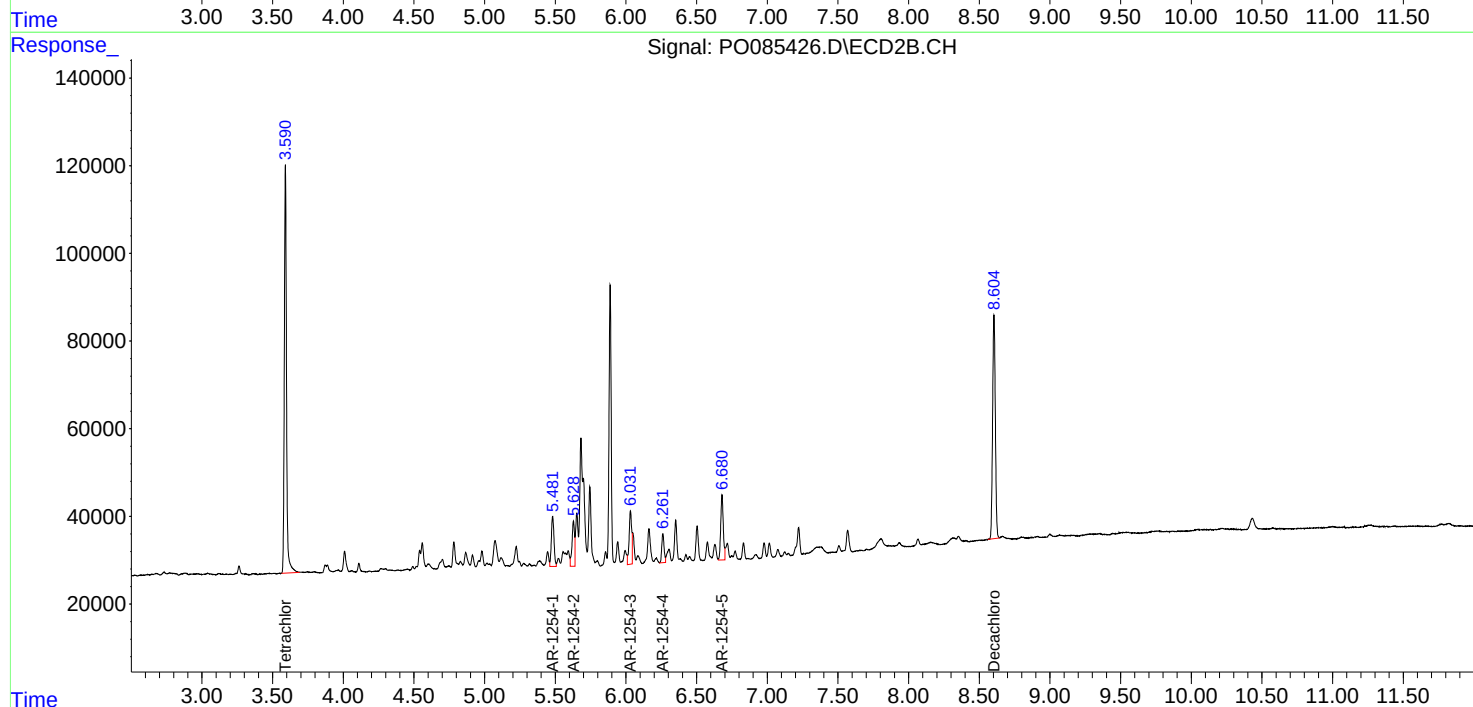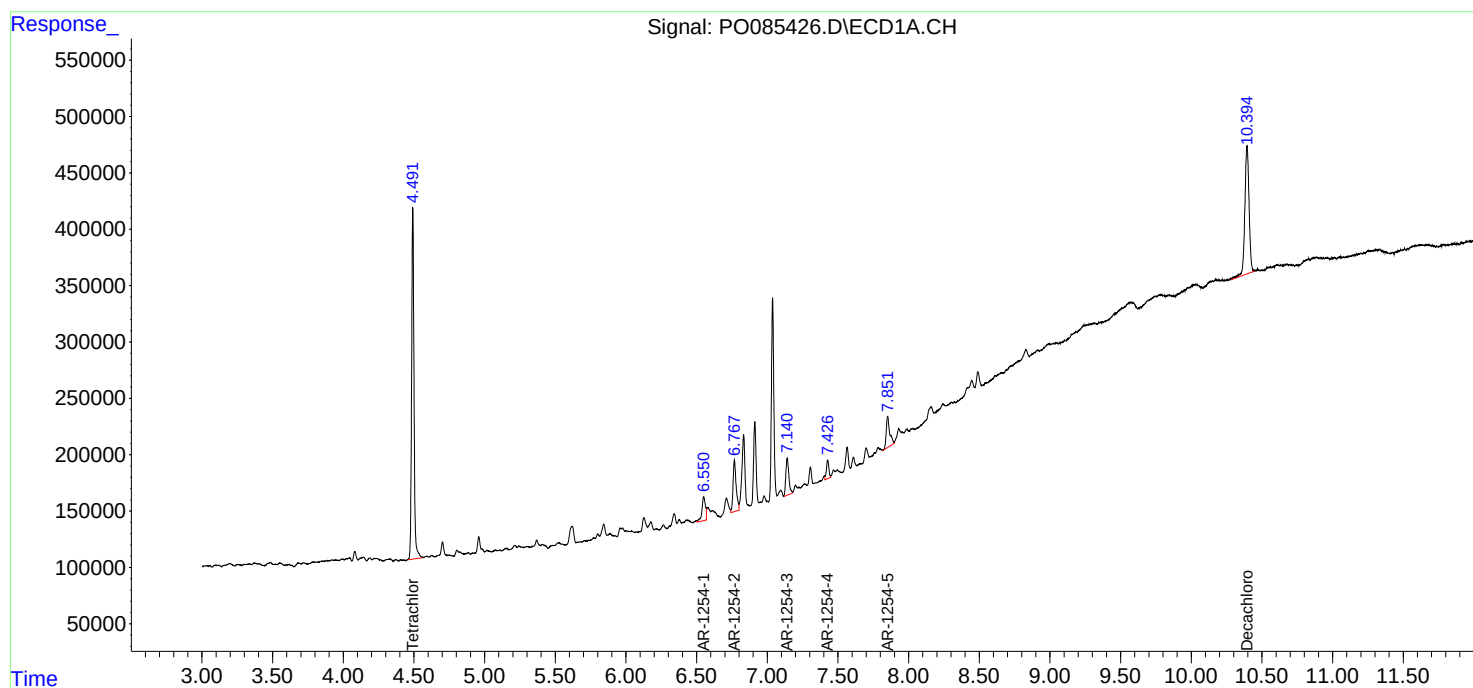

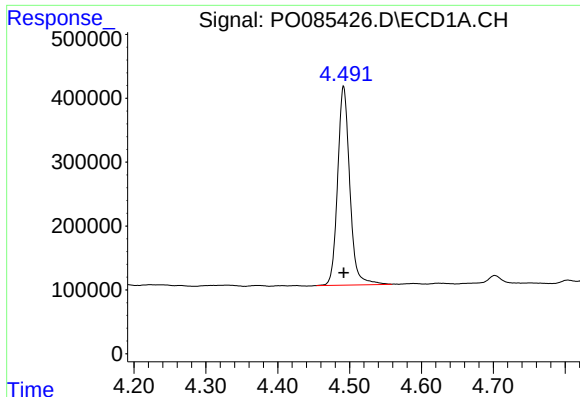


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: 0.000 min
Response: 3656116
Conc: 17.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

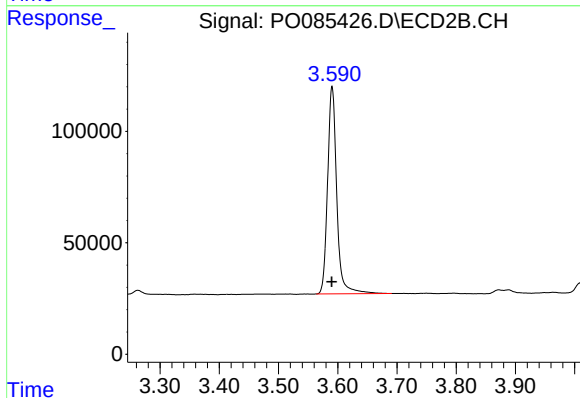


#1 Tetrachloro-m-xylene

R.T.: 3.591 min
Delta R.T.: 0.000 min
Response: 1003505
Conc: 23.42 ng/ml

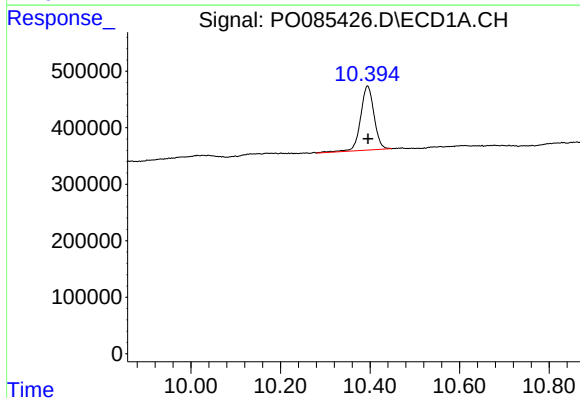


#2 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: 0.000 min
Response: 2365972
Conc: 19.68 ng/ml

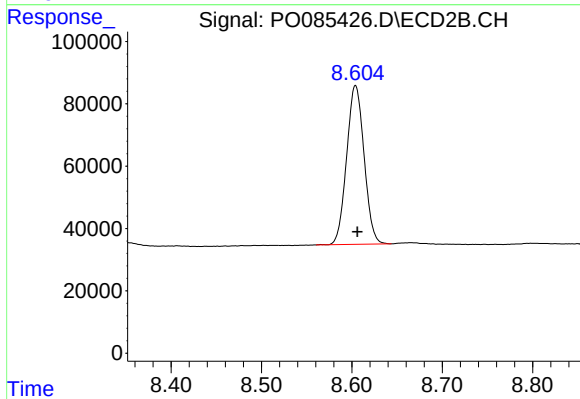

#2 Decachlorobiphenyl

R.T.: 8.604 min
Delta R.T.: -0.002 min
Response: 683474
Conc: 17.80 ng/ml

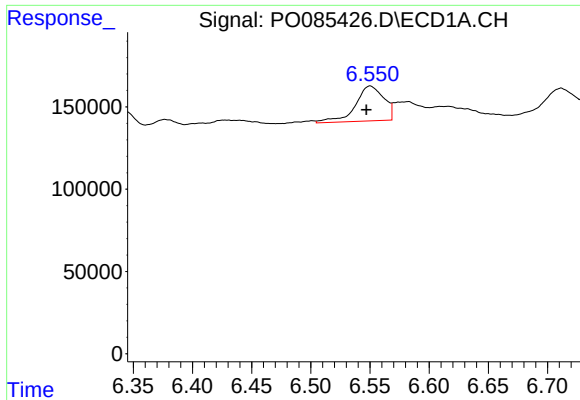


#26 AR-1254-1

R.T.: 6.550 min
Delta R.T.: 0.003 min
Response: 354274
Conc: 53.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

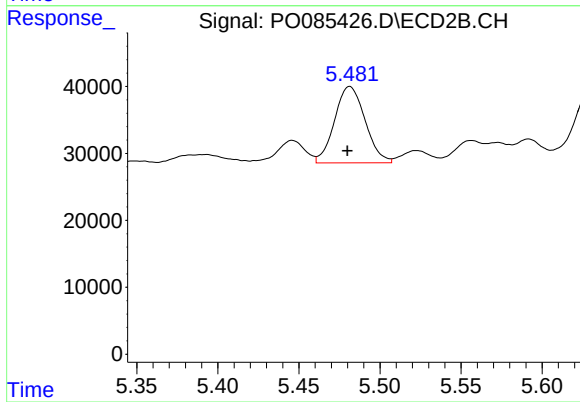


#26 AR-1254-1

R.T.: 5.481 min
Delta R.T.: 0.001 min
Response: 149683
Conc: 56.95 ng/ml

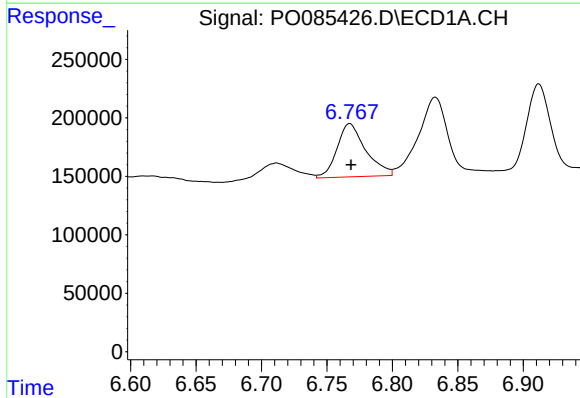


#27 AR-1254-2

R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 696188
Conc: 69.57 ng/ml

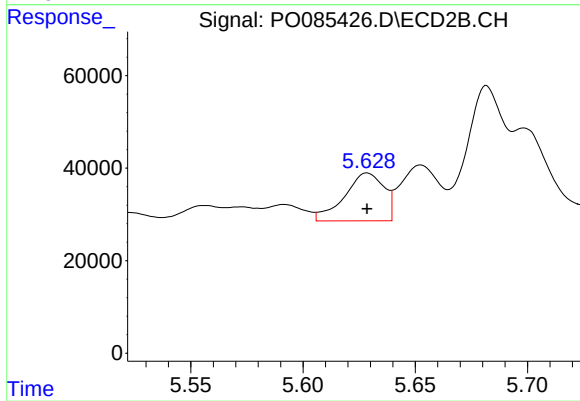

#27 AR-1254-2

R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 126904
Conc: 54.39 ng/ml

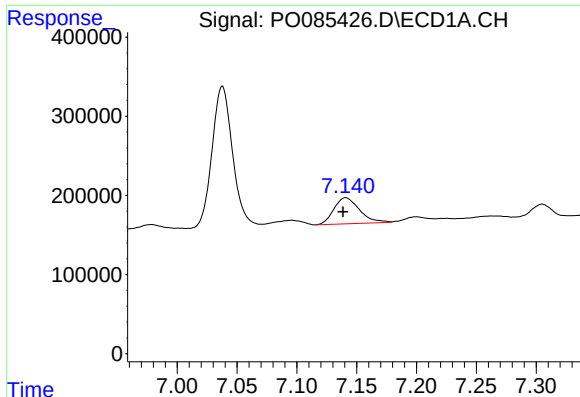


#28 AR-1254-3

R.T.: 7.141 min
Delta R.T.: 0.002 min
Response: 493341
Conc: 47.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

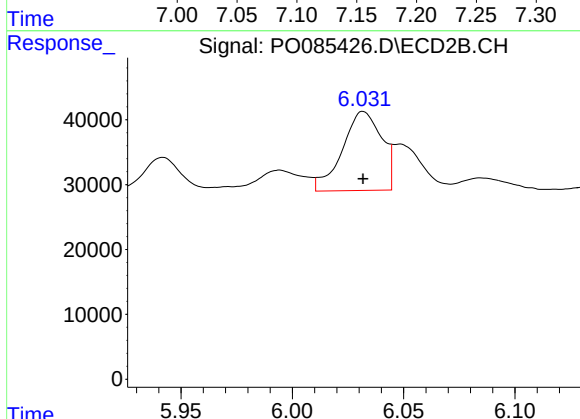


#28 AR-1254-3

R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 152109
Conc: 41.41 ng/ml m

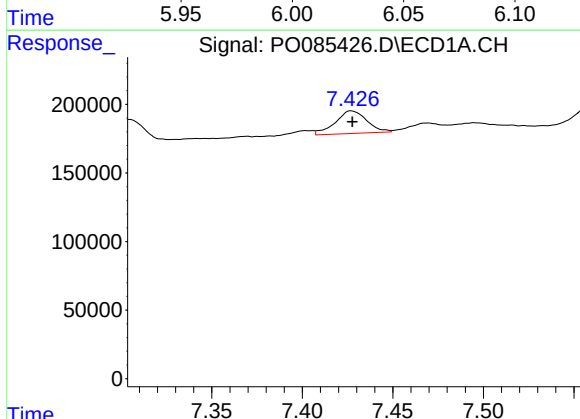


#29 AR-1254-4

R.T.: 7.426 min
Delta R.T.: -0.001 min
Response: 198894
Conc: 28.35 ng/ml m

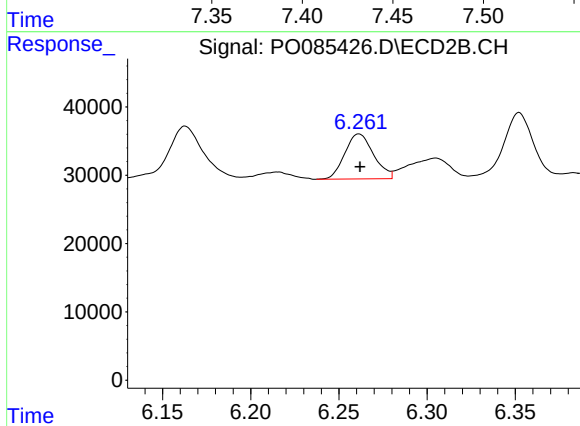

#29 AR-1254-4

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 74921
Conc: 33.82 ng/ml

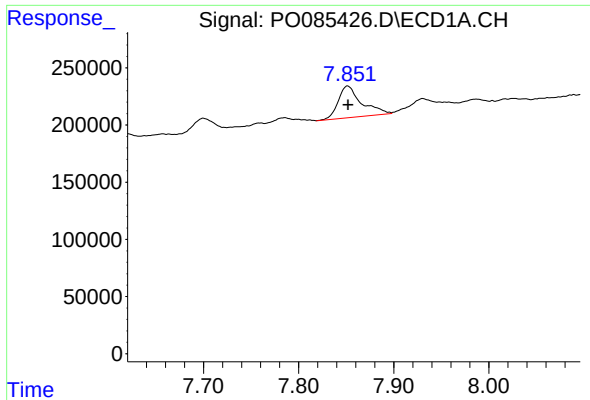


#30 AR-1254-5

R.T.: 7.852 min
Delta R.T.: 0.000 min
Response: 474186
Conc: 61.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TPK-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

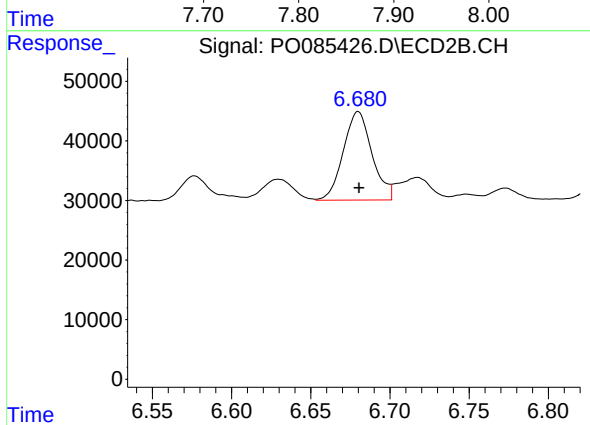

#30 AR-1254-5

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 187159
Conc: 57.54 ng/ml