

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031622\
 Data File : P0085449.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2022 9:52
 Operator : YP\AJ
 Sample : N1978-02RE
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-RW7A-IDWGW-20220315RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 17:42:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 16 04:43:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.589	3143394	822748	15.373	19.204
2) SA Decachlor...	10.393	8.603	788051	270712	6.556	7.051

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031622\
Data File : P0085449.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2022 9:52
Operator : YP\AJ
Sample : N1978-02RE
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-RW7A-IDWGW-20220315RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 17:42:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 16 04:43:31 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

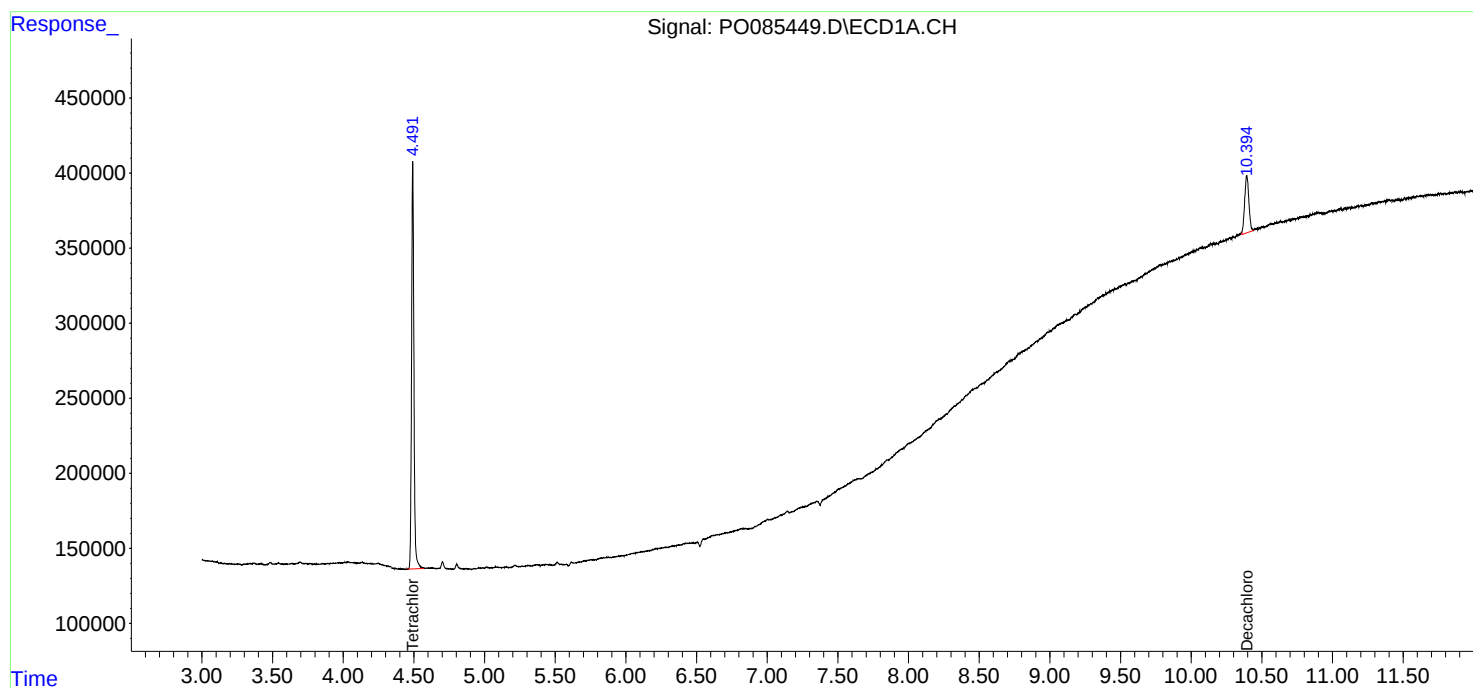

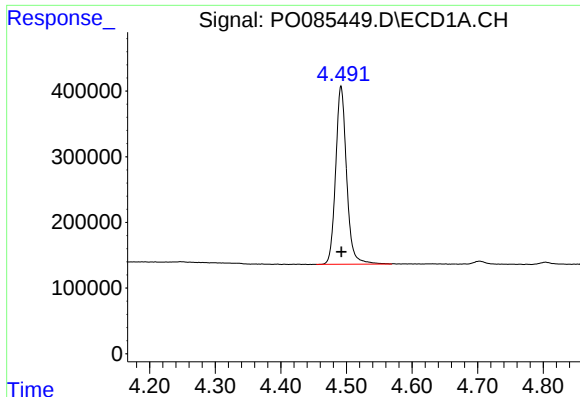

#1 Tetrachloro-m-xylene


R.T.: 4.492 min
Delta R.T.: 0.000 min
Response: 3143394
Conc: 15.37 ng/ml

Instrument :

ECD_O


ClientSampleId :

TT-RW7A-IDWGW-20220315RE

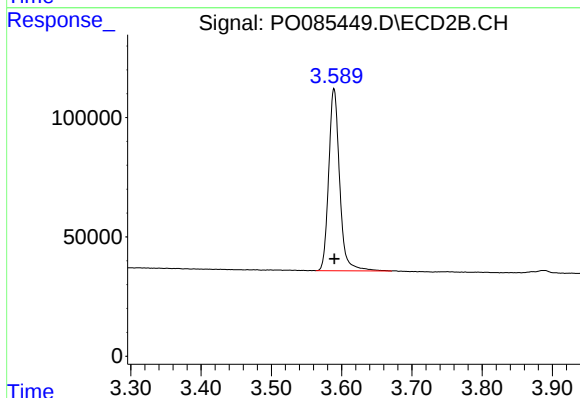


#1 Tetrachloro-m-xylene

R.T.: 3.589 min
Delta R.T.: 0.000 min
Response: 822748
Conc: 19.20 ng/ml

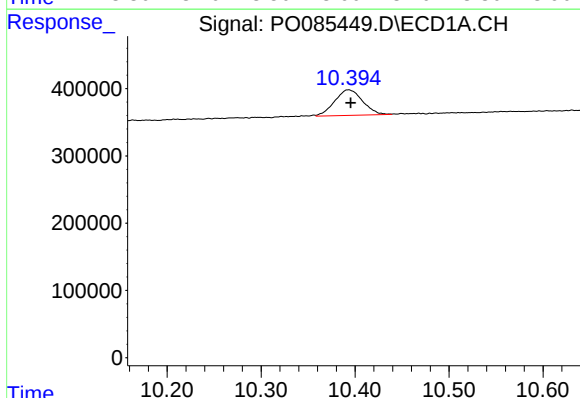

#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: -0.002 min
Response: 788051
Conc: 6.56 ng/ml

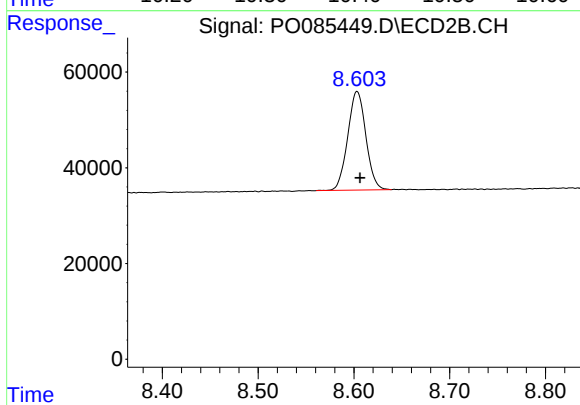

#2 Decachlorobiphenyl

R.T.: 8.603 min
Delta R.T.: -0.003 min
Response: 270712
Conc: 7.05 ng/ml