

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031623\
 Data File : P0093242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 23:48
 Operator : YP/AJ
 Sample : 01923-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SAMPLE-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2023
 Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:20:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.632	60354647	25838941	19.273m	22.910
2) SA Decachlor...	10.262	8.664	31135598	14636474	14.386	14.948

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031623\
Data File : PO093242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 23:48
Operator : YP/AJ
Sample : 01923-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SAMPLE-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:20:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

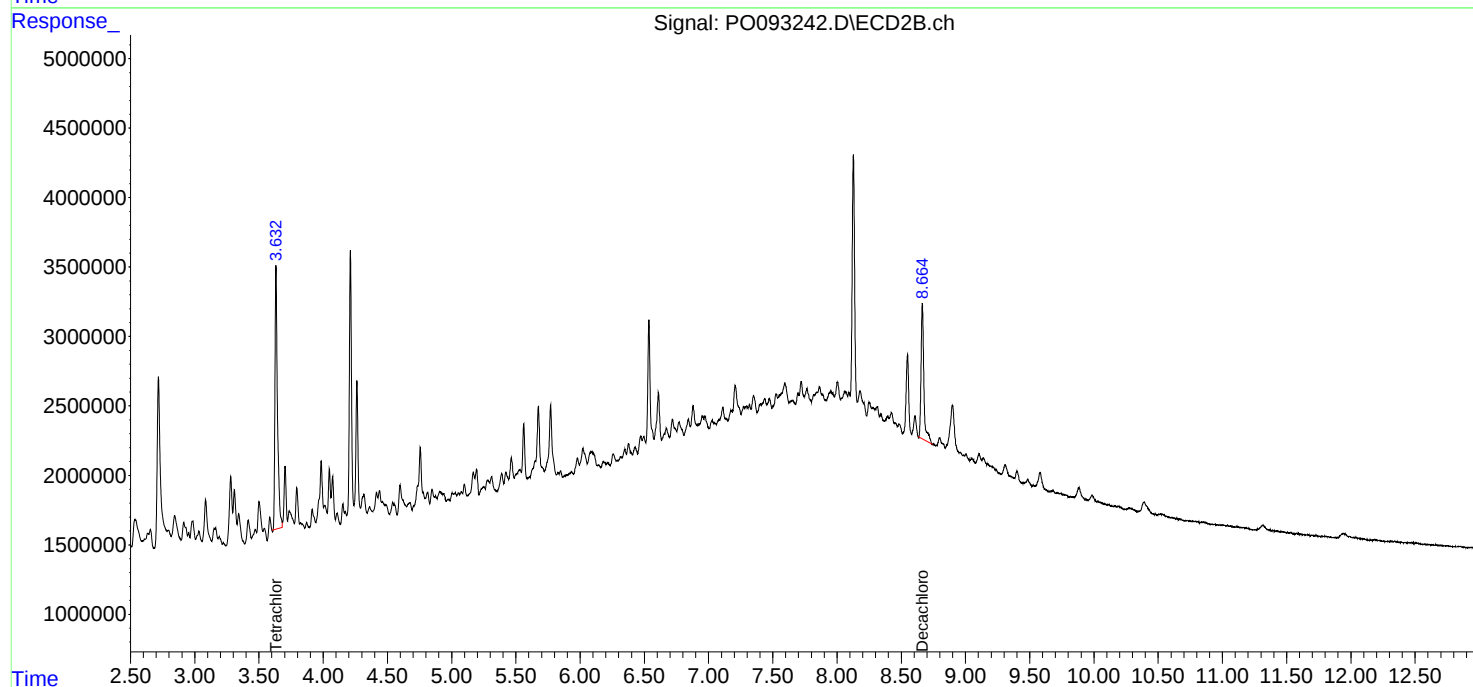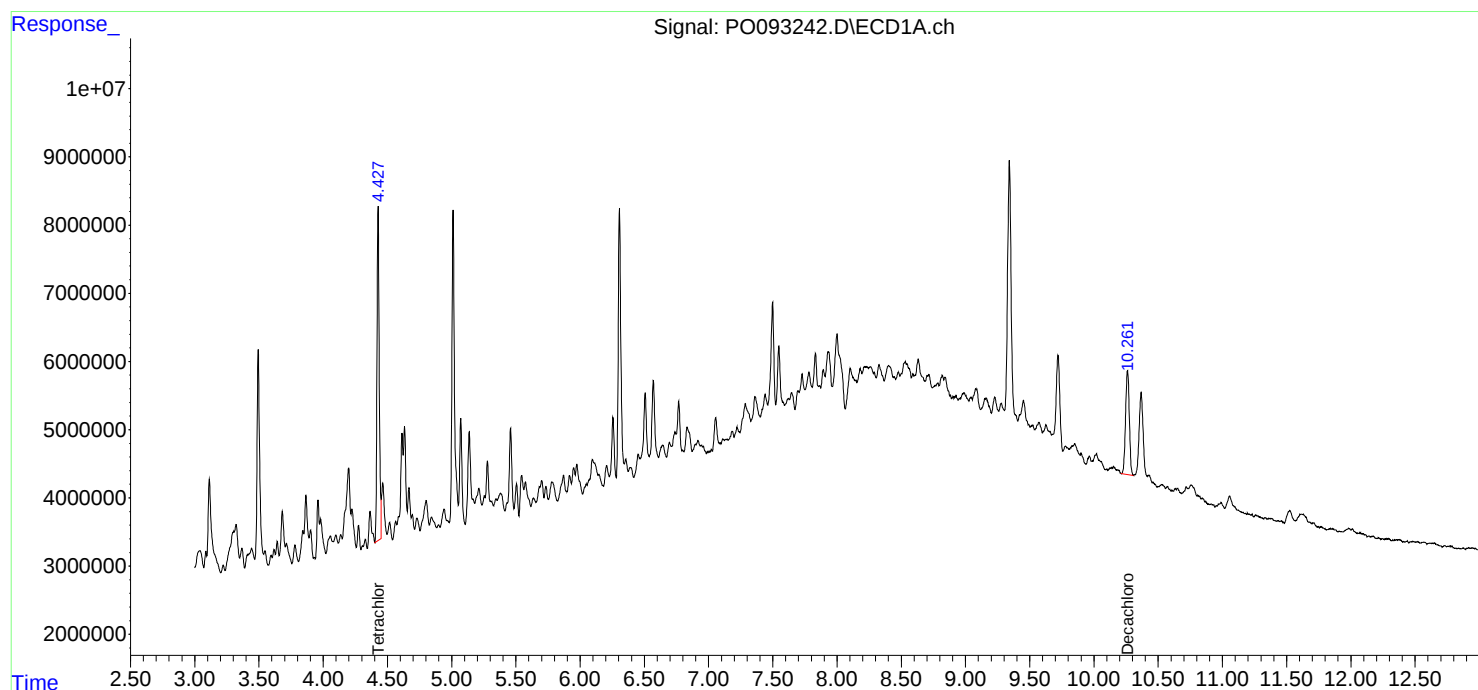

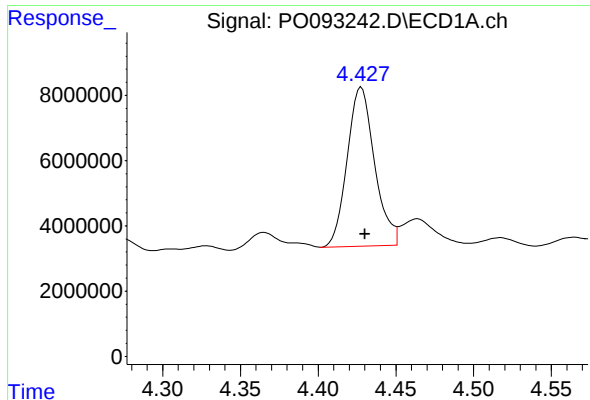


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: -0.003 min
Response: 60354647
Conc: 19.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
SAMPLE-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

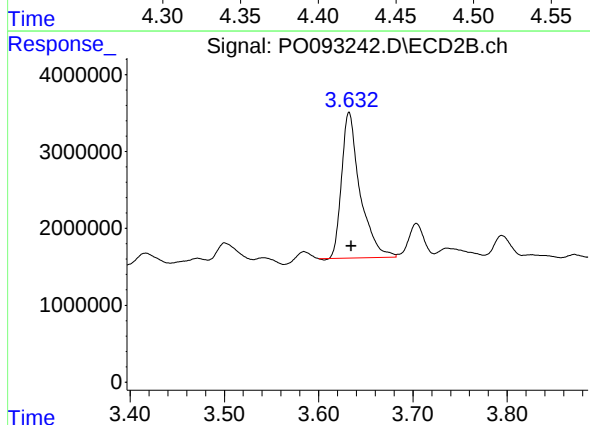


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.002 min
Response: 25838941
Conc: 22.91 ng/ml

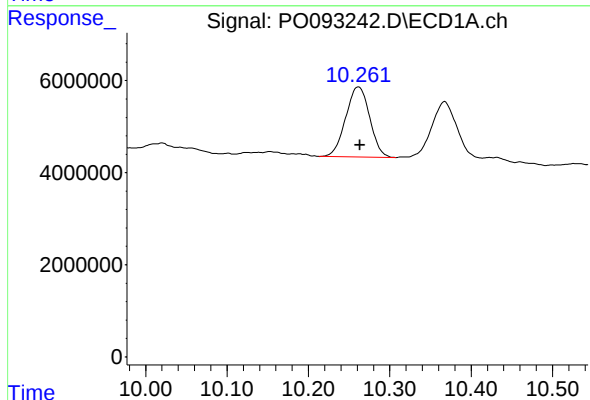

#2 Decachlorobiphenyl

R.T.: 10.262 min
Delta R.T.: -0.002 min
Response: 31135598
Conc: 14.39 ng/ml

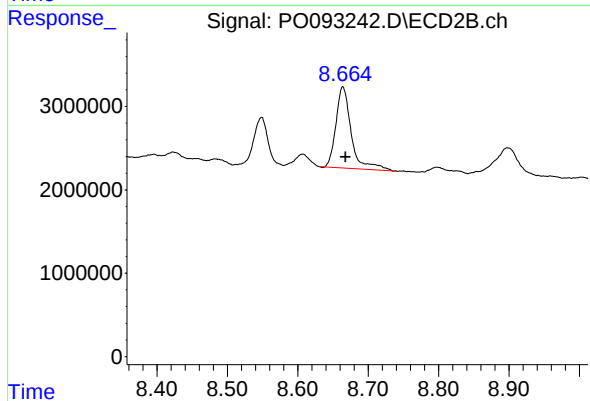

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: -0.004 min
Response: 14636474
Conc: 14.95 ng/ml