

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031623\
 Data File : P0093244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2023 00:23
 Operator : YP/AJ
 Sample : 01939-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 D2958

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:20:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 14 05:32:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.428	3.632	54036102	19983270	17.256	17.718
2) SA Decachlor...	10.261	8.664	30763648	13605846	14.214	13.896

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031623\
Data File : P0093244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2023 00:23
Operator : YP/AJ
Sample : 01939-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
D2958

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:20:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 14 05:32:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

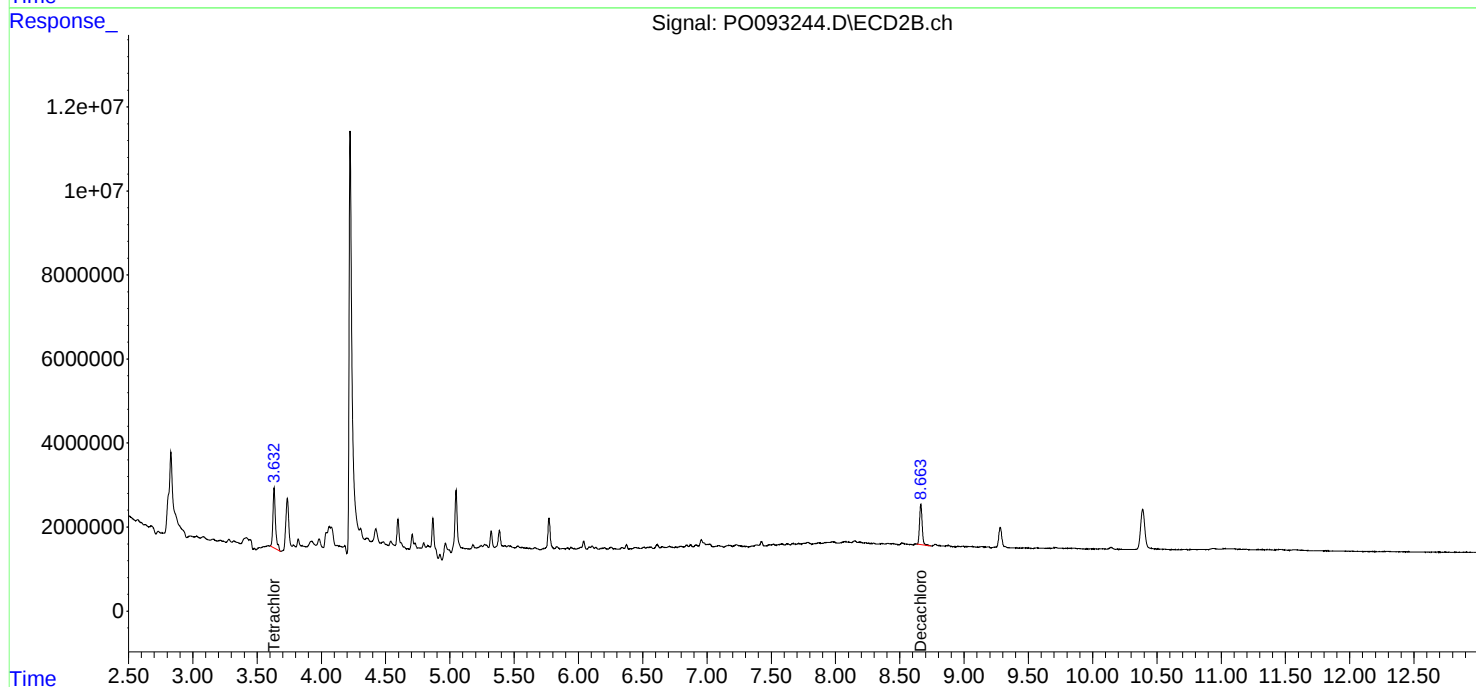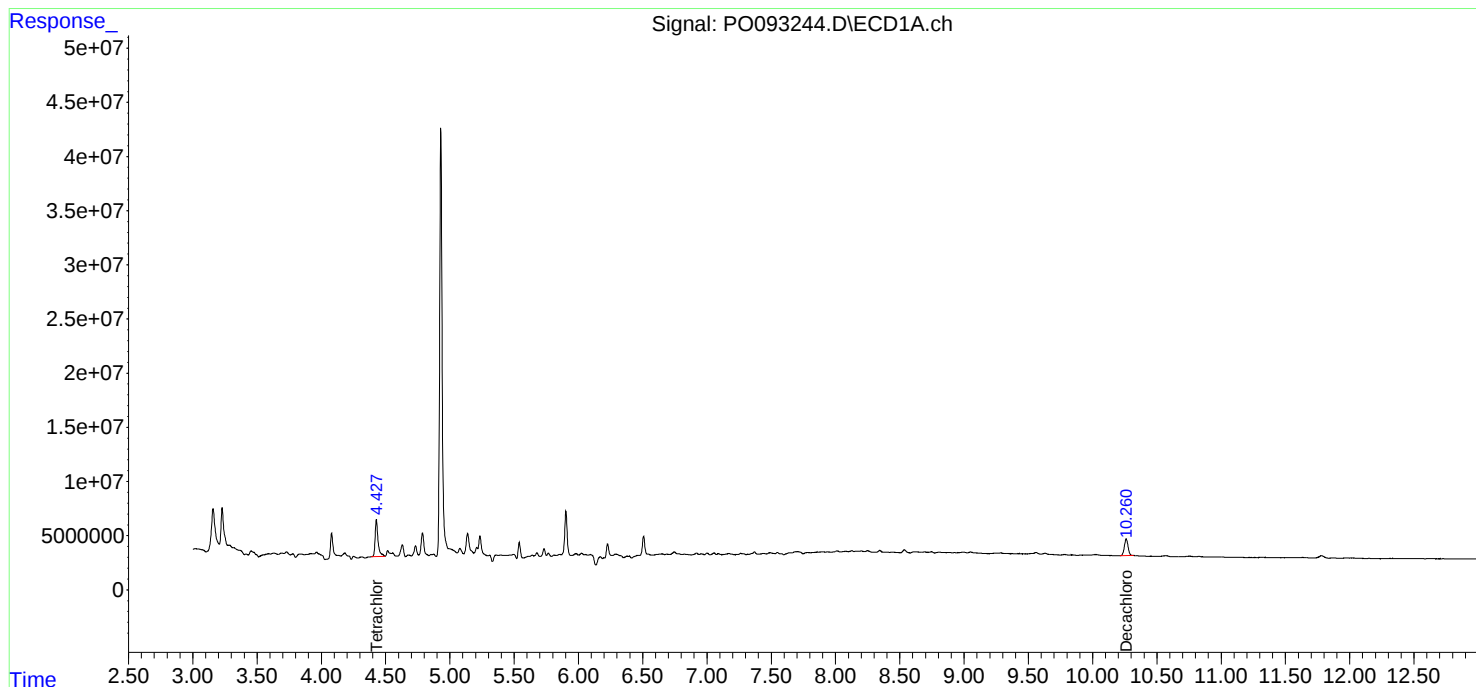


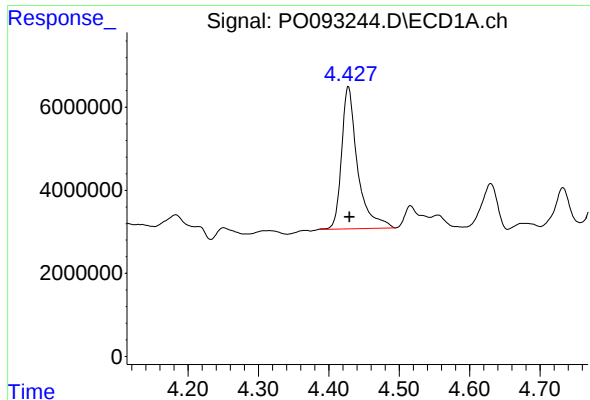

#1 Tetrachloro-m-xylene


R.T.: 4.428 min
Delta R.T.: -0.002 min
Response: 54036102
Conc: 17.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
D2958

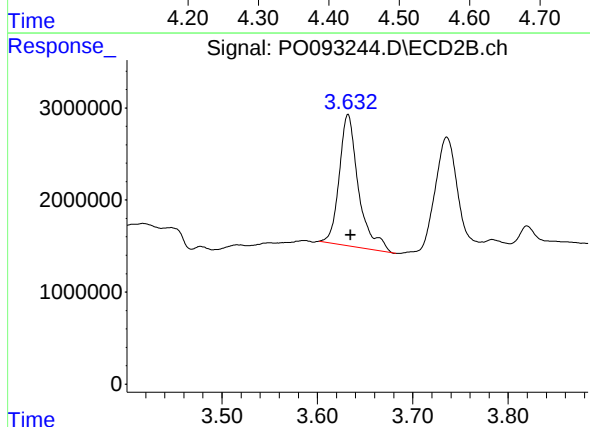


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.003 min
Response: 19983270
Conc: 17.72 ng/ml

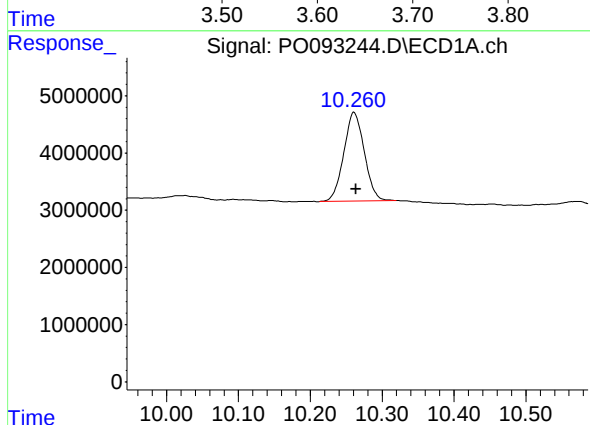

#2 Decachlorobiphenyl

R.T.: 10.261 min
Delta R.T.: -0.002 min
Response: 30763648
Conc: 14.21 ng/ml

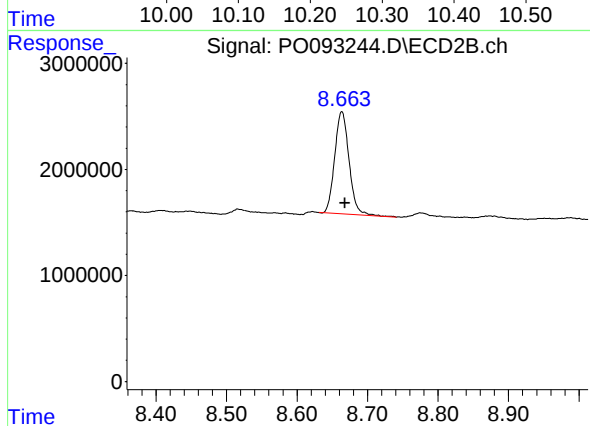

#2 Decachlorobiphenyl

R.T.: 8.664 min
Delta R.T.: -0.004 min
Response: 13605846
Conc: 13.90 ng/ml