

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
 Data File : P0076230.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 11:51
 Operator : DD\AJ
 Sample : M1458-08
 Misc : AR1242 LOQ 50 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOQ-WATER-02-QT1-2021

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:01:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 14:55:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.930	3.936	807758	600766	14.219	14.399
2)	SA Decachlor...	10.929	9.204	610147	581249	15.863	15.138
Target Compounds							
16)	L4 AR-1242-1	6.253	5.185	71433	54671	56.564	61.622
17)	L4 AR-1242-2	6.277	5.204	109677	95861	55.339	55.384
18)	L4 AR-1242-3	6.342	5.395	67639	41569	53.378	51.608
19)	L4 AR-1242-4	6.451	5.489	50667	44093	52.326	50.796m
20)	L4 AR-1242-5	7.234	6.052	56925	50891	56.659	50.498

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031721\
Data File : PO076230.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 11:51
Operator : DD\AJ
Sample : M1458-08
Misc : AR1242 LOQ 50 PPB
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2021


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 14:55:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

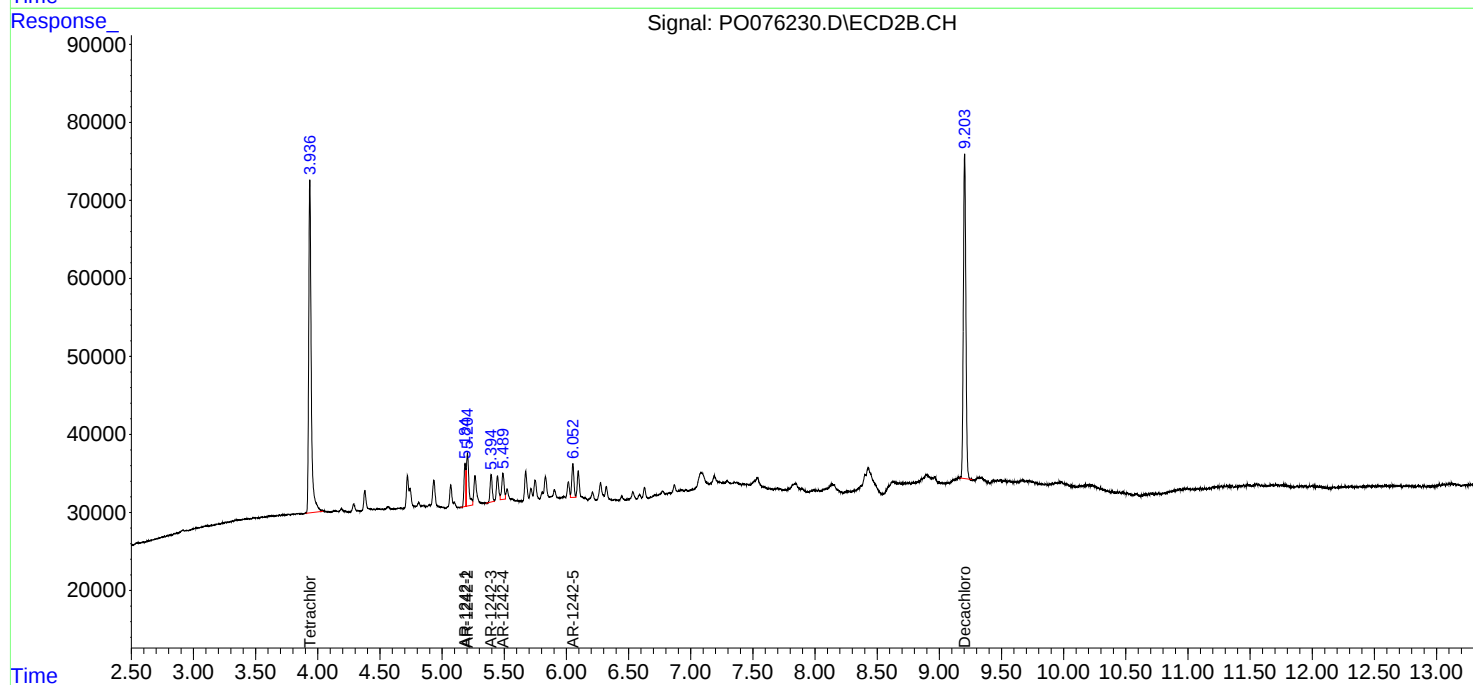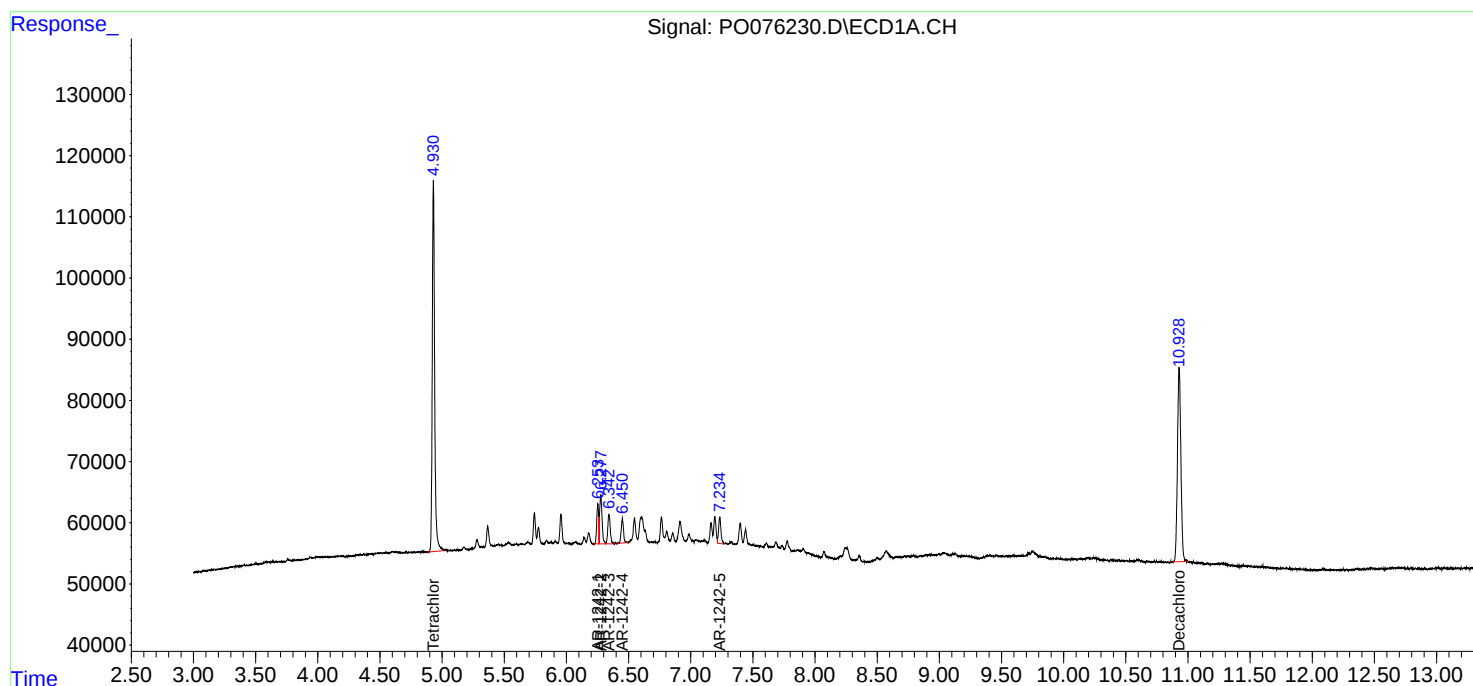

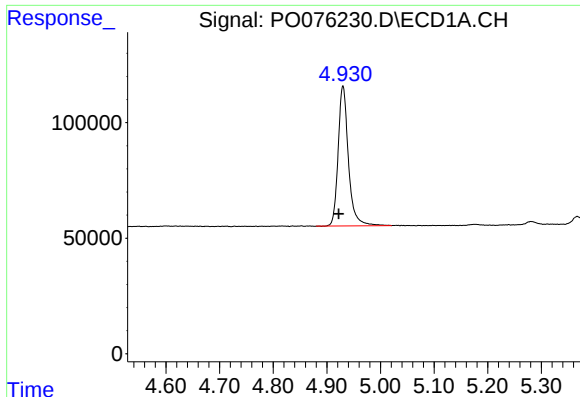


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: 0.008 min
Response: 807758
Conc: 14.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2021


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:03 PM

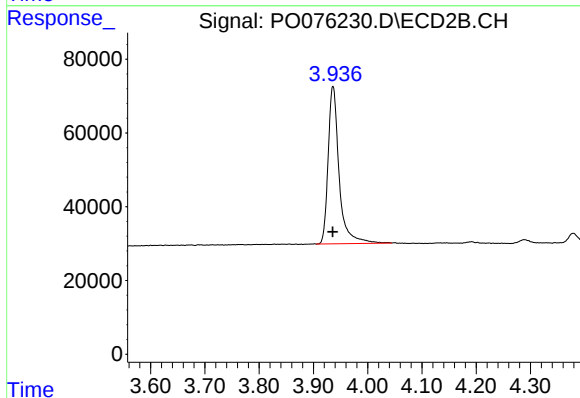


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 600766
Conc: 14.40 ng/ml

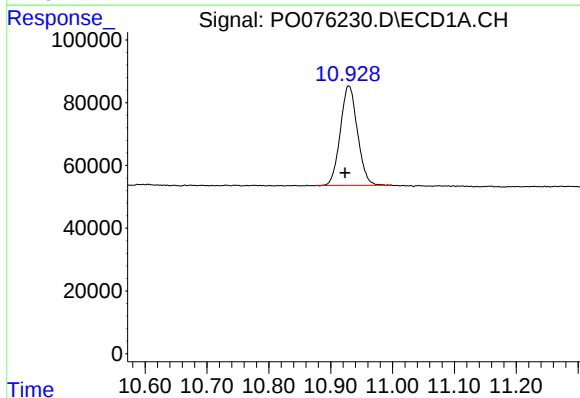


#2 Decachlorobiphenyl

R.T.: 10.929 min
Delta R.T.: 0.006 min
Response: 610147
Conc: 15.86 ng/ml

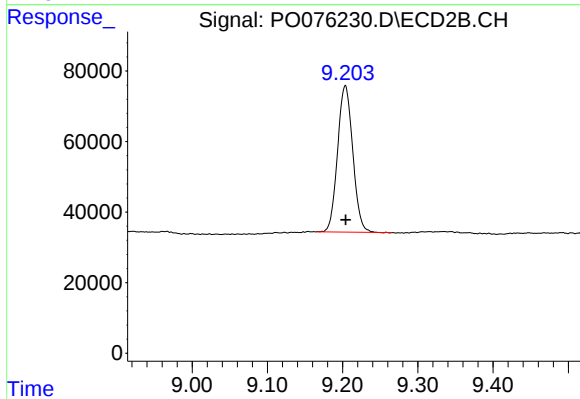

#2 Decachlorobiphenyl

R.T.: 9.204 min
Delta R.T.: 0.000 min
Response: 581249
Conc: 15.14 ng/ml

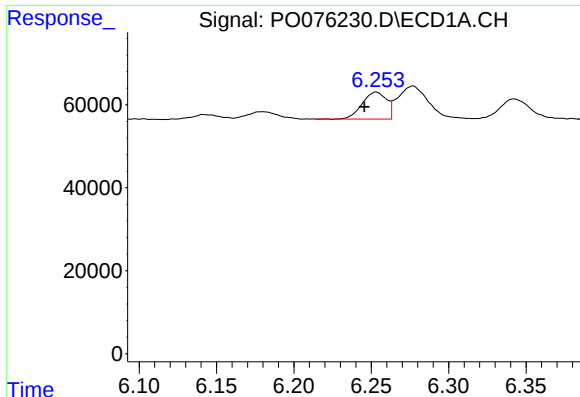


#16 AR-1242-1

R.T.: 6.253 min
Delta R.T.: 0.008 min
Response: 71433
Conc: 56.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2021


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:03 PM

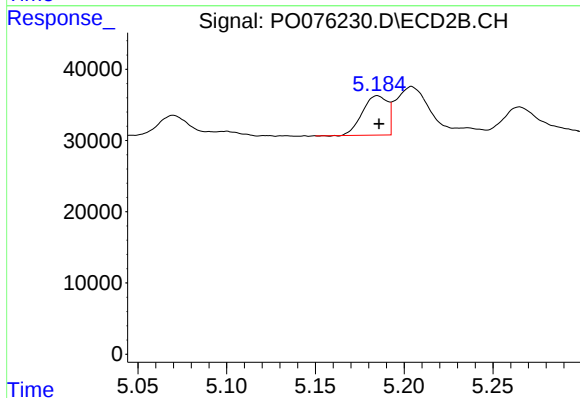


#16 AR-1242-1

R.T.: 5.185 min
Delta R.T.: 0.000 min
Response: 54671
Conc: 61.62 ng/ml

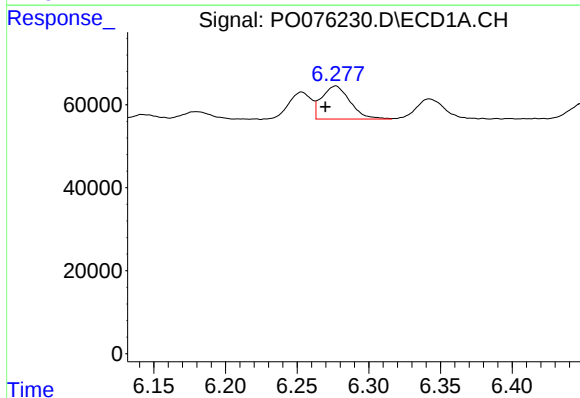


#17 AR-1242-2

R.T.: 6.277 min
Delta R.T.: 0.007 min
Response: 109677
Conc: 55.34 ng/ml

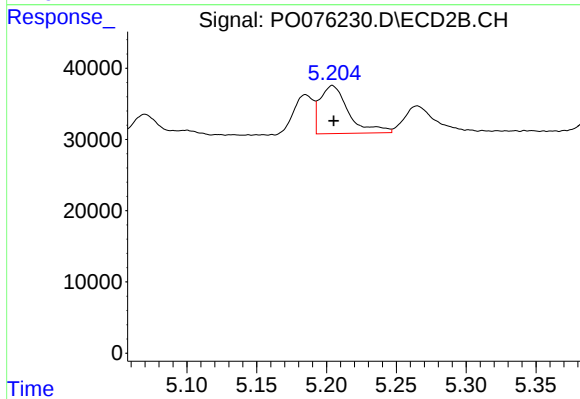

#17 AR-1242-2

R.T.: 5.204 min
Delta R.T.: 0.000 min
Response: 95861
Conc: 55.38 ng/ml

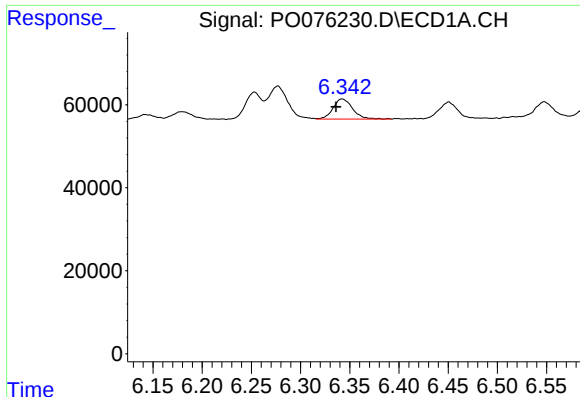


#18 AR-1242-3

R.T.: 6.342 min
Delta R.T.: 0.006 min
Response: 67639
Conc: 53.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2021


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:03 PM

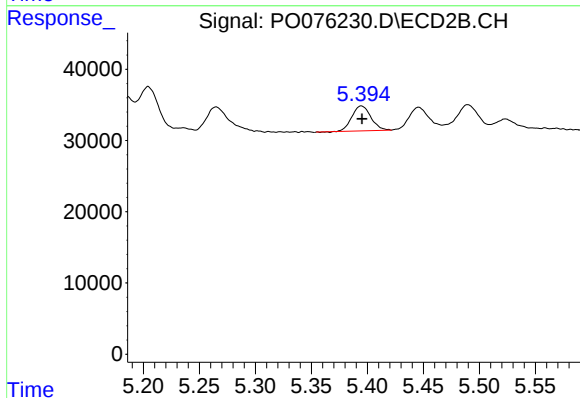


#18 AR-1242-3

R.T.: 5.395 min
Delta R.T.: 0.000 min
Response: 41569
Conc: 51.61 ng/ml

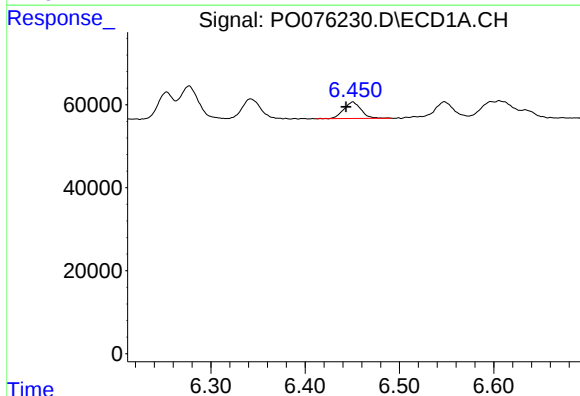


#19 AR-1242-4

R.T.: 6.451 min
Delta R.T.: 0.007 min
Response: 50667
Conc: 52.33 ng/ml

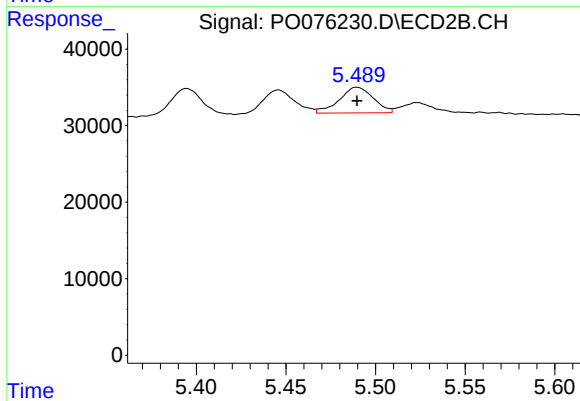

#19 AR-1242-4

R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 44093
Conc: 50.80 ng/ml m

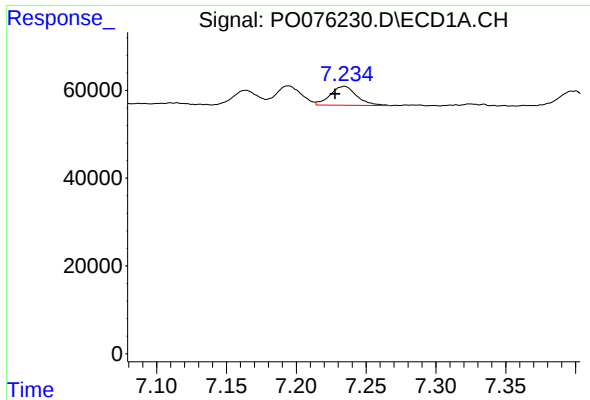


#20 AR-1242-5

R.T.: 7.234 min
Delta R.T.: 0.007 min
Response: 56925
Conc: 56.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT1-2021

Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:03 PM

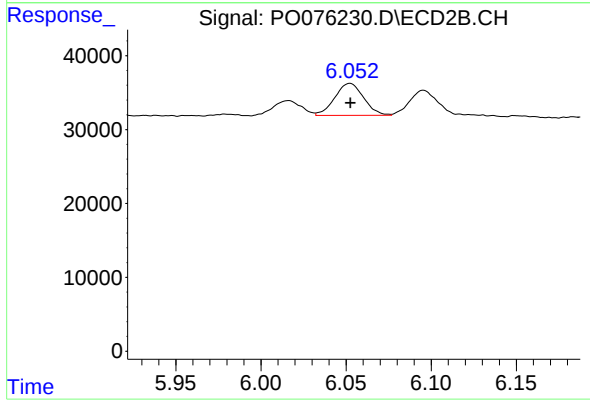

#20 AR-1242-5

R.T.: 6.052 min
Delta R.T.: 0.000 min
Response: 50891
Conc: 50.50 ng/ml