

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
 Data File : P0076234.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 13:58
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:01:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 14:57:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.935	3137445	2159815	55.228	51.768
2) SA Decachlor...	10.923	9.201	2215792	2045204	57.607	53.264
Target Compounds						
21) L5 AR-1248-1	6.245	5.183	557147	396929	590.964	577.952m
22) L5 AR-1248-2	6.540	5.444	819768	651810	544.193	503.773
23) L5 AR-1248-3	6.758	5.488	965660	659338	556.764	515.832
24) L5 AR-1248-4	7.187	5.671	945633	755934	537.494m	514.079
25) L5 AR-1248-5	7.227	6.094	916423	775068	518.152m	501.154

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
Data File : P0076234.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 13:58
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 99 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 14:57:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

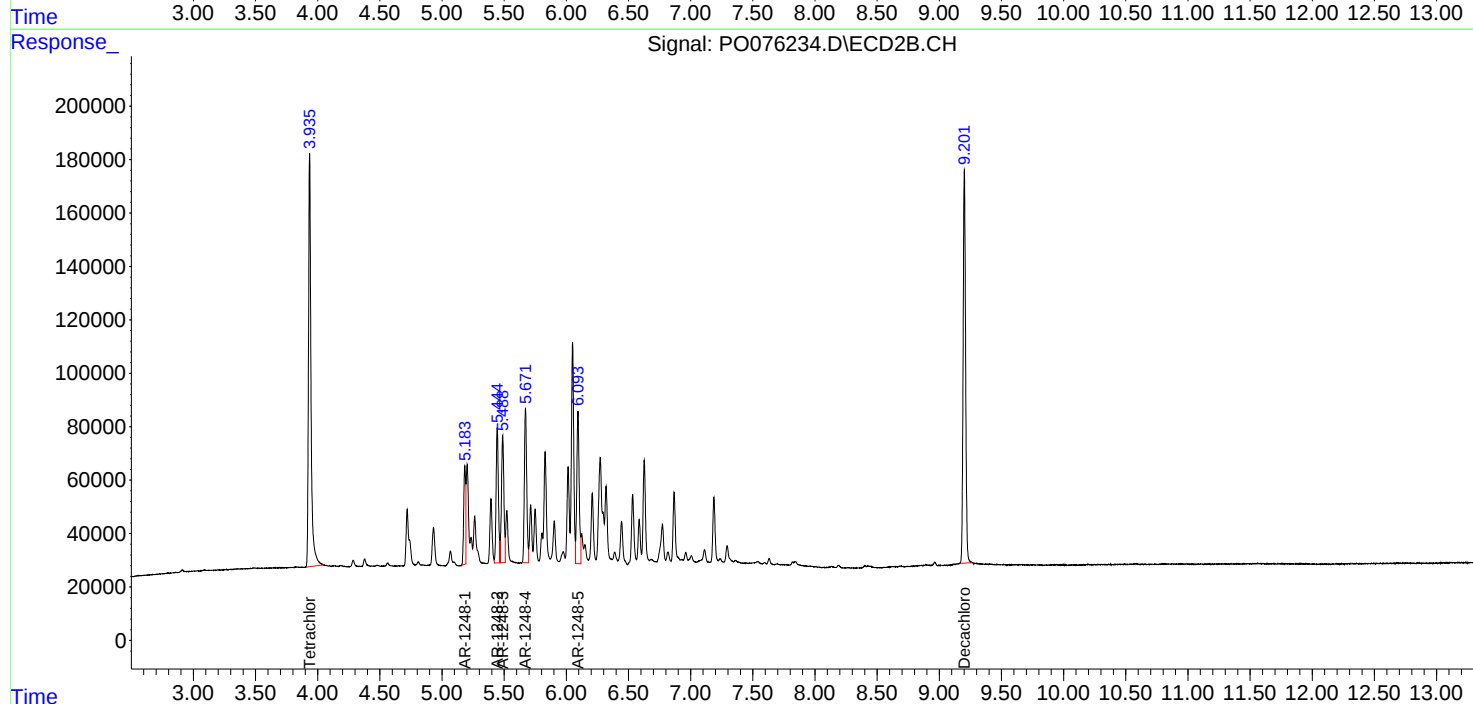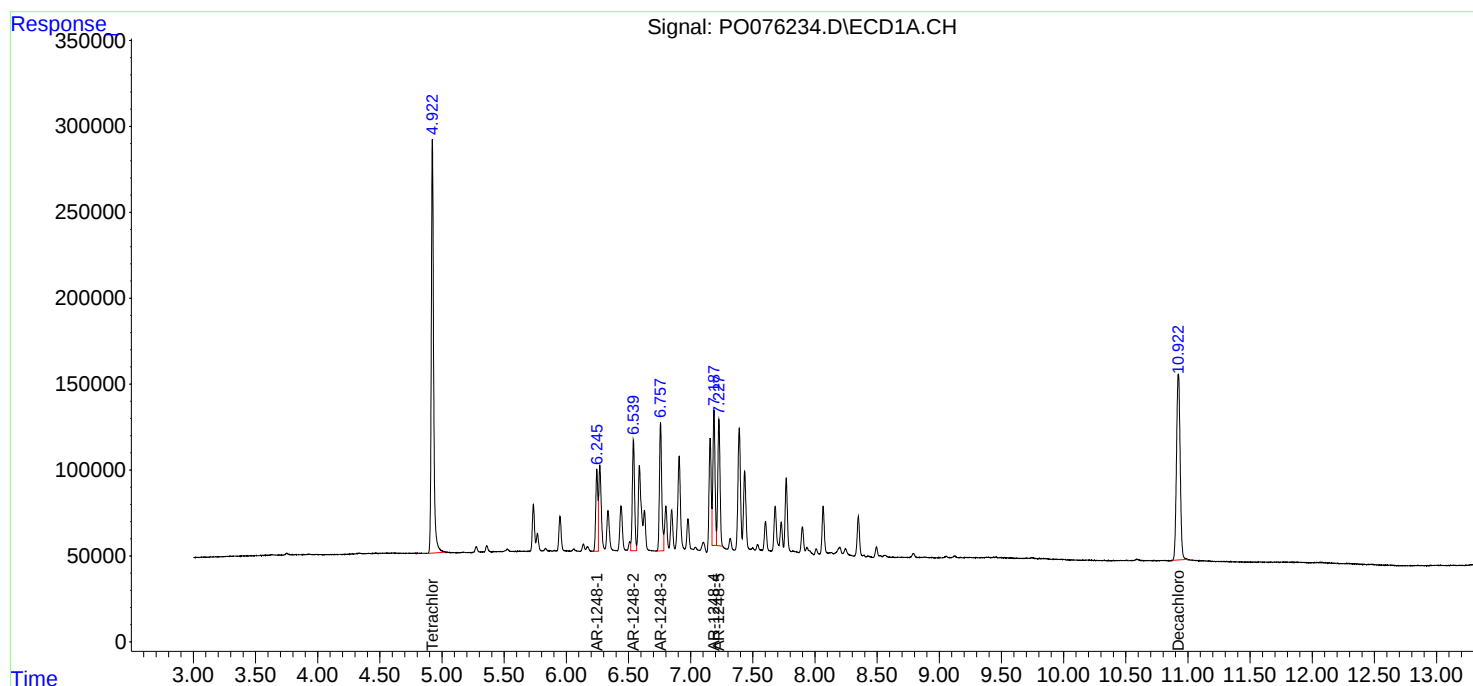

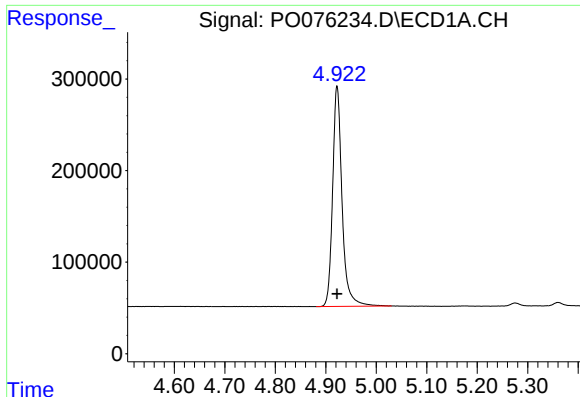


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 3137445
Conc: 55.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:04 PM

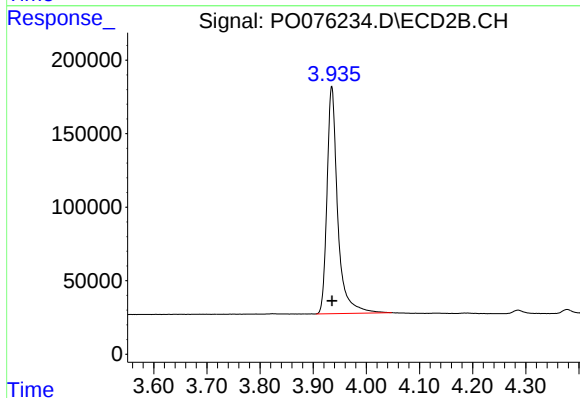


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 2159815
Conc: 51.77 ng/ml

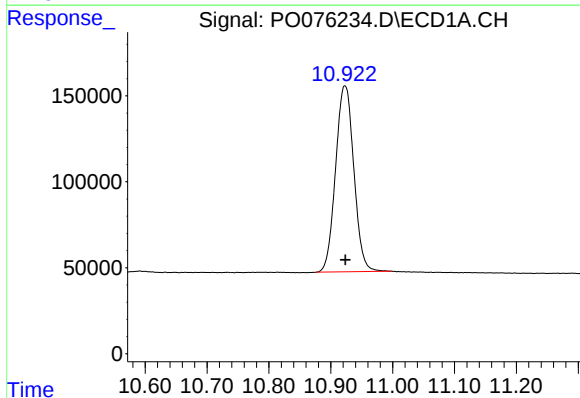


#2 Decachlorobiphenyl

R.T.: 10.923 min
Delta R.T.: 0.000 min
Response: 2215792
Conc: 57.61 ng/ml

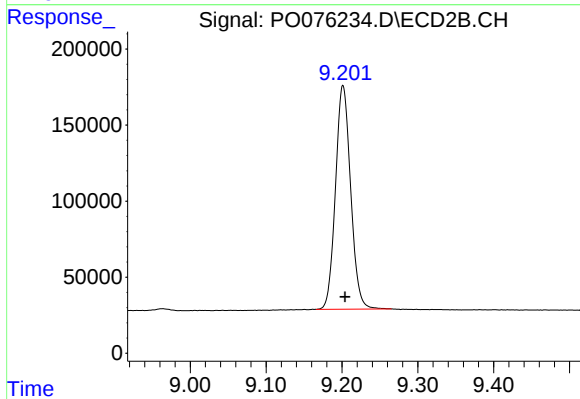

#2 Decachlorobiphenyl

R.T.: 9.201 min
Delta R.T.: -0.003 min
Response: 2045204
Conc: 53.26 ng/ml

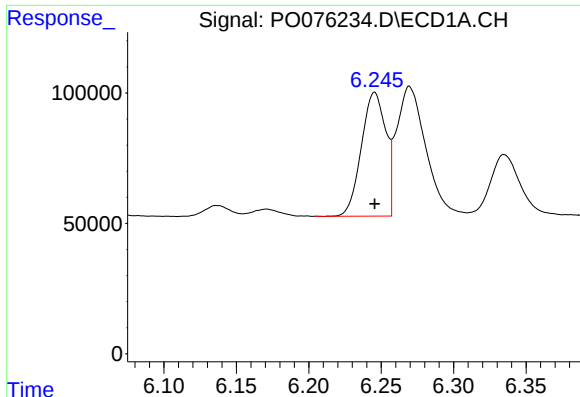


#21 AR-1248-1

R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 557147
Conc: 590.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:04 PM

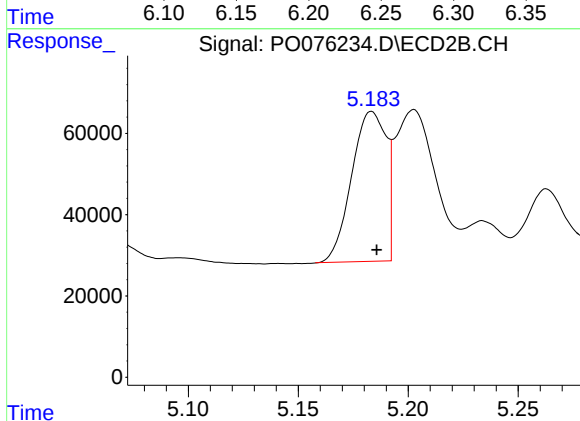


#21 AR-1248-1

R.T.: 5.183 min
Delta R.T.: -0.003 min
Response: 396929
Conc: 577.95 ng/ml m

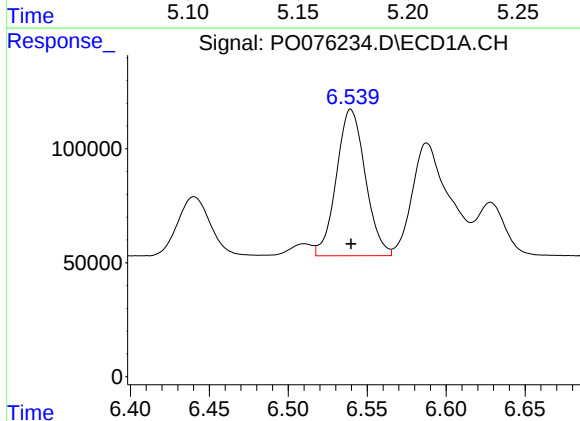


#22 AR-1248-2

R.T.: 6.540 min
Delta R.T.: 0.000 min
Response: 819768
Conc: 544.19 ng/ml

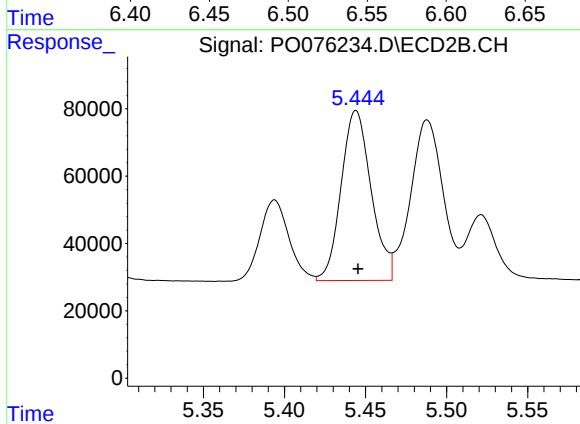

#22 AR-1248-2

R.T.: 5.444 min
Delta R.T.: -0.001 min
Response: 651810
Conc: 503.77 ng/ml

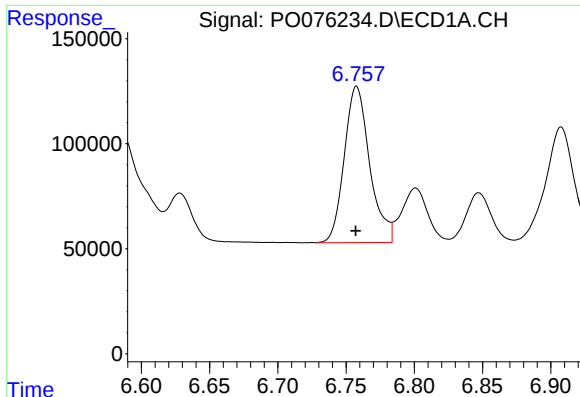


#23 AR-1248-3

R.T.: 6.758 min
Delta R.T.: 0.000 min
Response: 965660
Conc: 556.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:04 PM

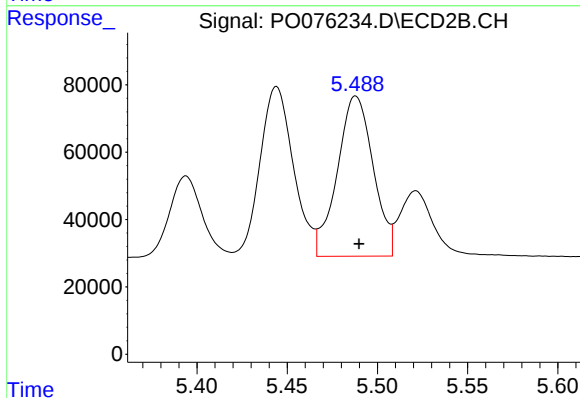


#23 AR-1248-3

R.T.: 5.488 min
Delta R.T.: -0.002 min
Response: 659338
Conc: 515.83 ng/ml

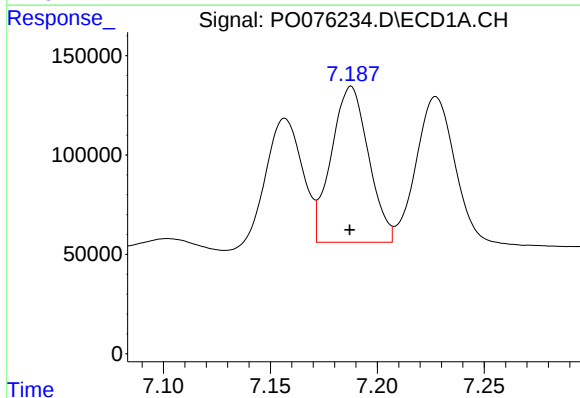


#24 AR-1248-4

R.T.: 7.187 min
Delta R.T.: 0.000 min
Response: 945633
Conc: 537.49 ng/ml m

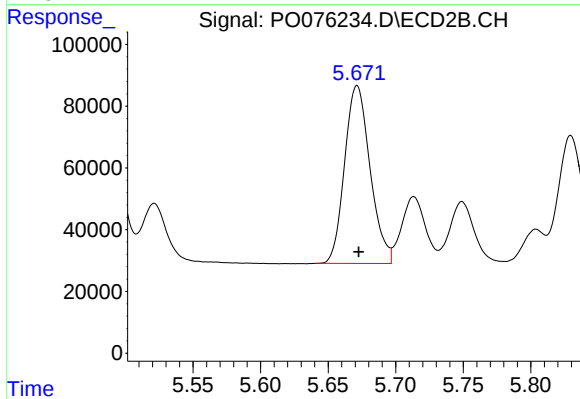

#24 AR-1248-4

R.T.: 5.671 min
Delta R.T.: -0.001 min
Response: 755934
Conc: 514.08 ng/ml

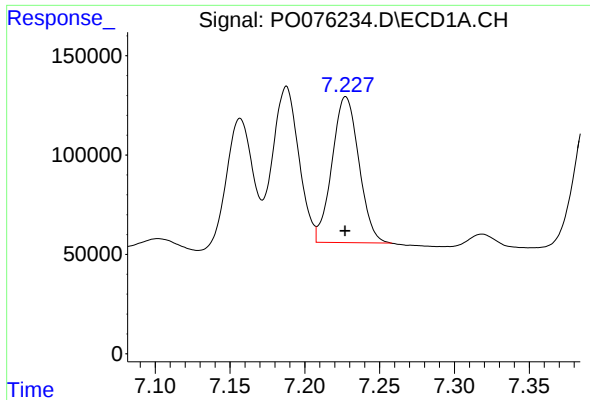


#25 AR-1248-5

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 916423
Conc: 518.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:04 PM

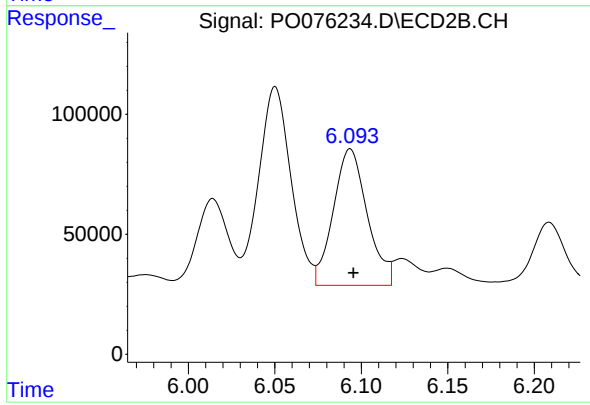

#25 AR-1248-5

R.T.: 6.094 min
Delta R.T.: -0.002 min
Response: 775068
Conc: 501.15 ng/ml