

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0031721\
 Data File : P0076241.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 15:57
 Operator : DD\AJ
 Sample : M1688-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 R-LA-4-1-WC

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:01:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 17:48:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	3.934	1227819	879456	21.613	21.079
2) SA Decachlor...	10.920	9.200	665156	662154	17.293	17.245
Target Compounds						
26) L6 AR-1254-1	7.155	6.049	43124	82769	21.042	36.215 #
27) L6 AR-1254-2	7.385	6.207	88240	37199	28.395	18.782 #
28) L6 AR-1254-3	7.769	6.625	102369	62677	32.177	20.809m#
29) L6 AR-1254-4	8.064	6.865	78729	65521	37.577	37.129
30) L6 AR-1254-5	8.497	7.291	188136	65809	81.917	25.136 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031721\
Data File : PO076241.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 15:57
Operator : DD\AJ
Sample : M1688-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
R-LA-4-1-WC


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 17:48:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

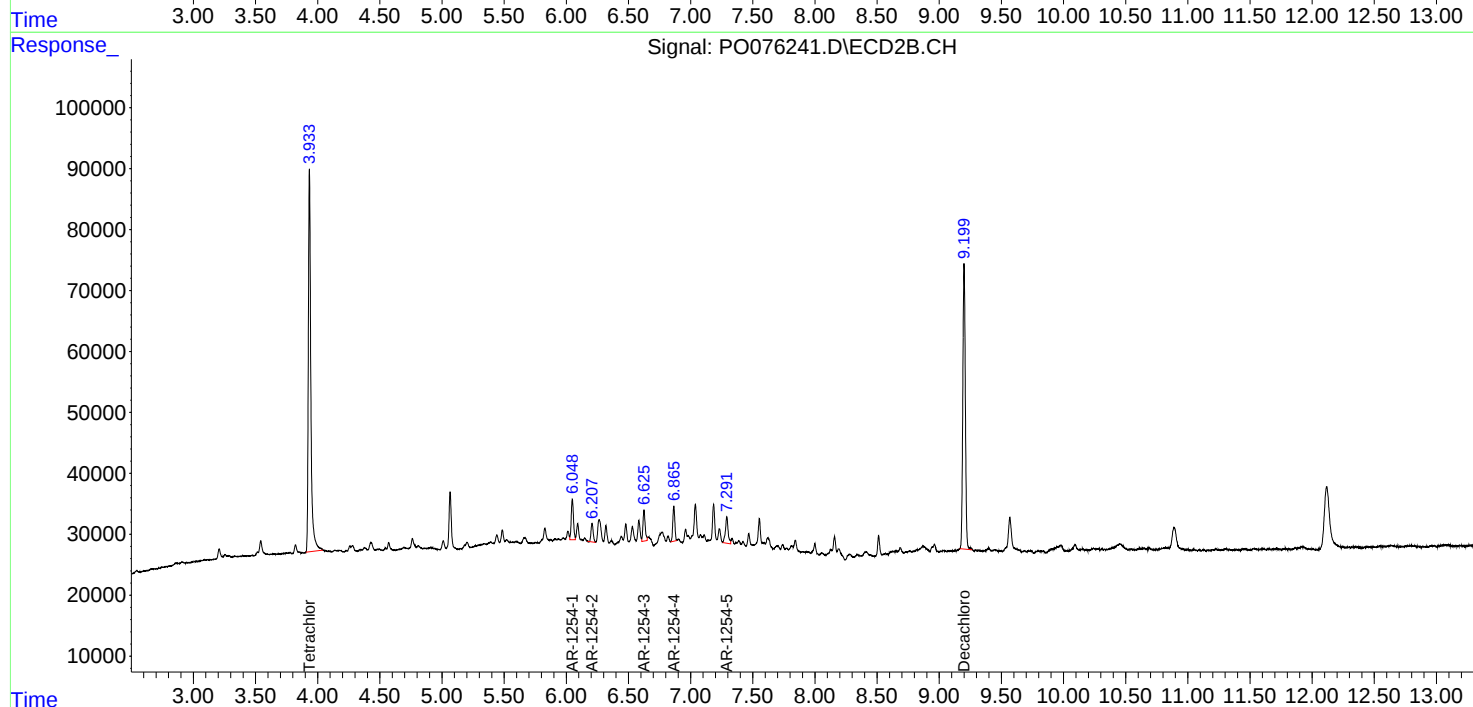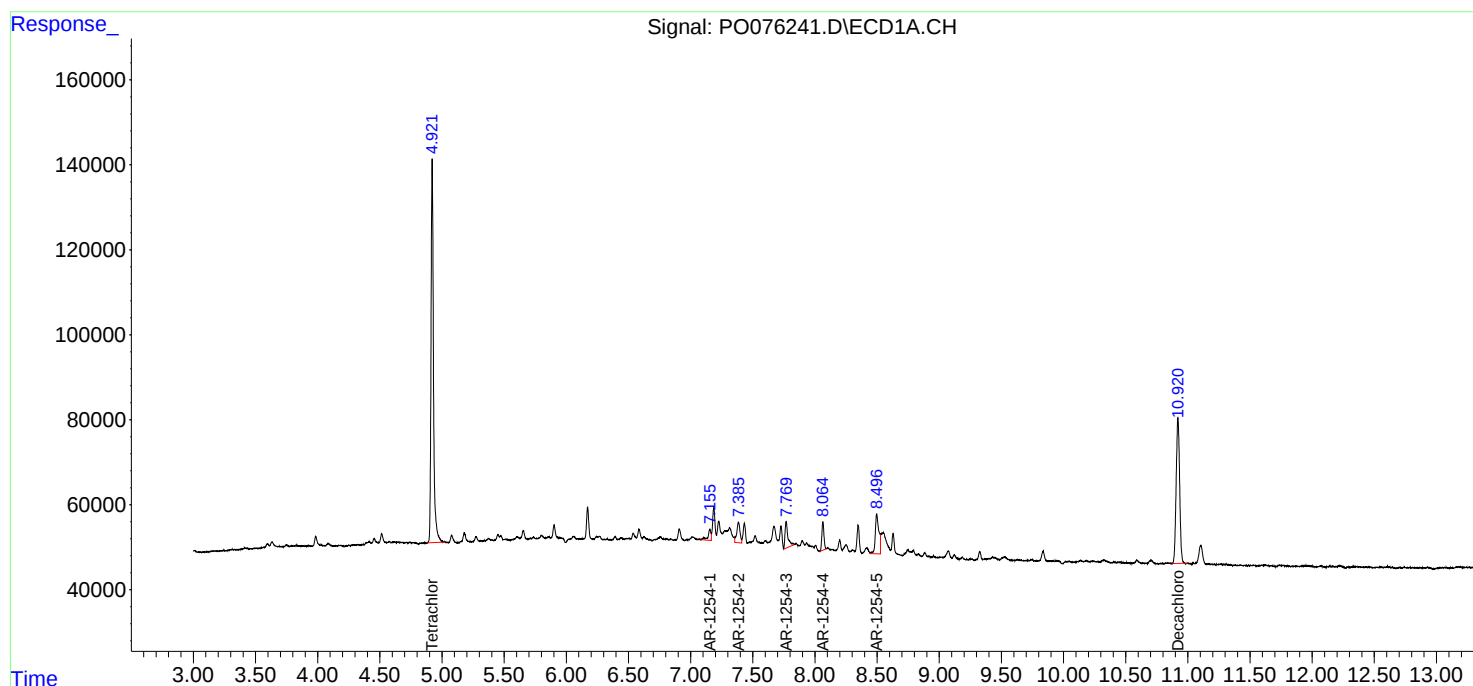

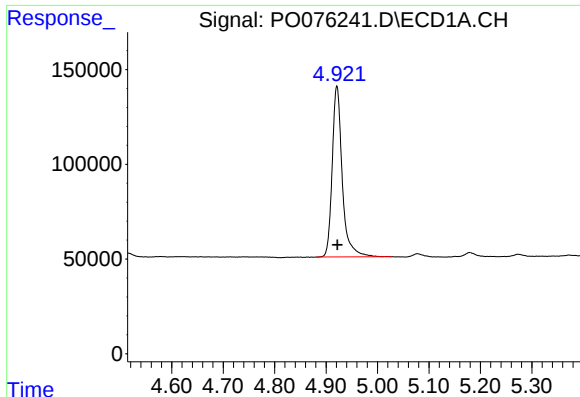


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 1227819
Conc: 21.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
R-LA-4-1-WC


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:08 PM

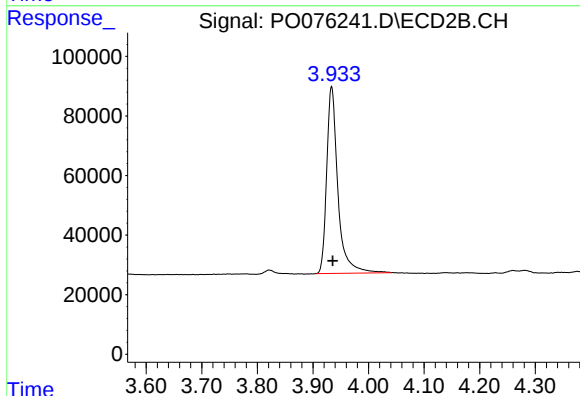


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 879456
Conc: 21.08 ng/ml

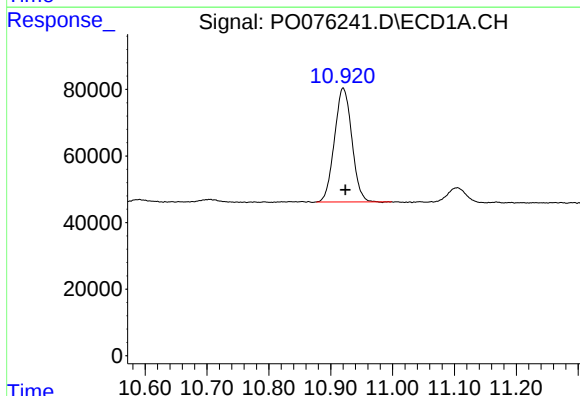


#2 Decachlorobiphenyl

R.T.: 10.920 min
Delta R.T.: -0.004 min
Response: 665156
Conc: 17.29 ng/ml

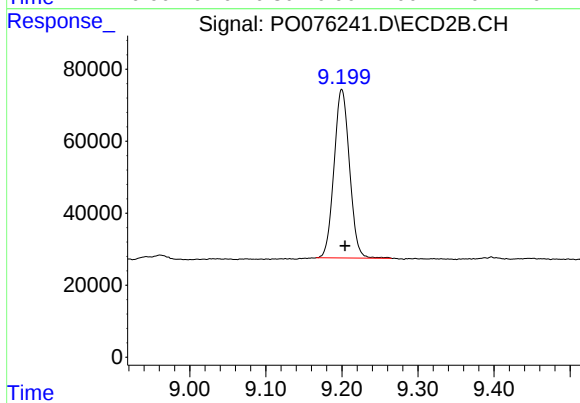

#2 Decachlorobiphenyl

R.T.: 9.200 min
Delta R.T.: -0.004 min
Response: 662154
Conc: 17.24 ng/ml

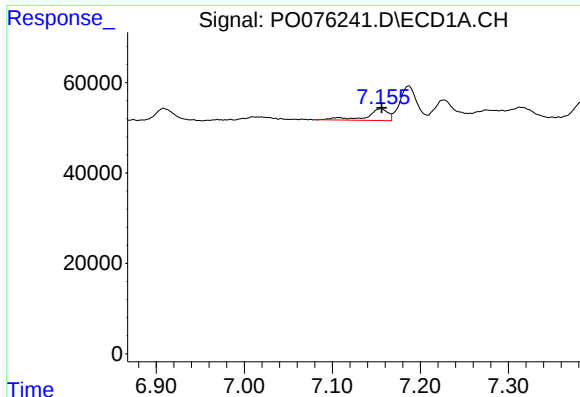


#26 AR-1254-1

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 43124
Conc: 21.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
R-LA-4-1-WC


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:08 PM

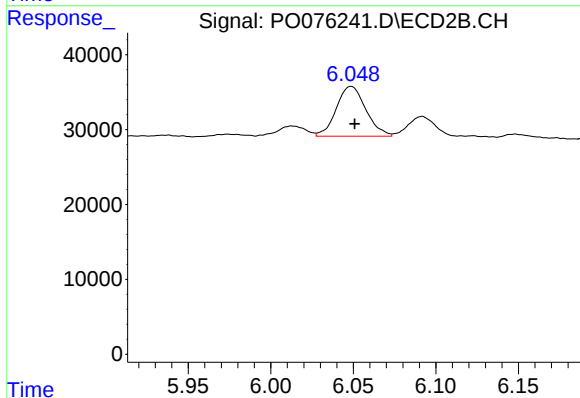


#26 AR-1254-1

R.T.: 6.049 min
Delta R.T.: -0.002 min
Response: 82769
Conc: 36.21 ng/ml

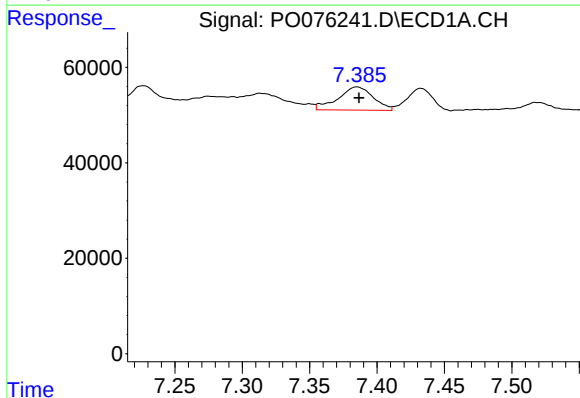


#27 AR-1254-2

R.T.: 7.385 min
Delta R.T.: -0.001 min
Response: 88240
Conc: 28.40 ng/ml

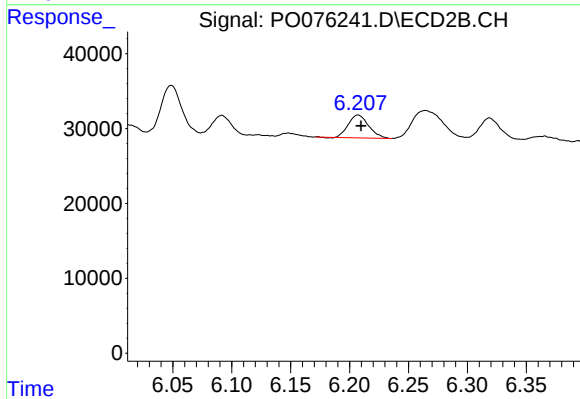

#27 AR-1254-2

R.T.: 6.207 min
Delta R.T.: -0.002 min
Response: 37199
Conc: 18.78 ng/ml

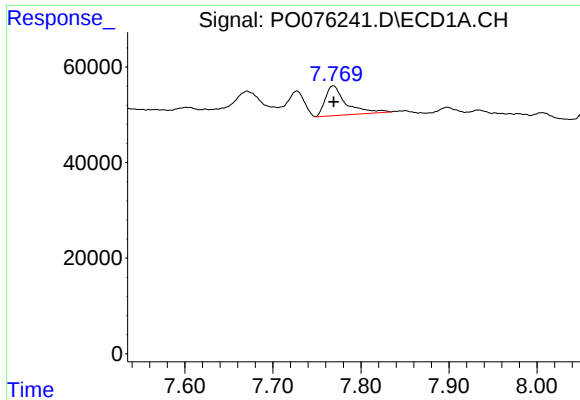


#28 AR-1254-3

R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 102369
Conc: 32.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
R-LA-4-1-WC


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:08 PM

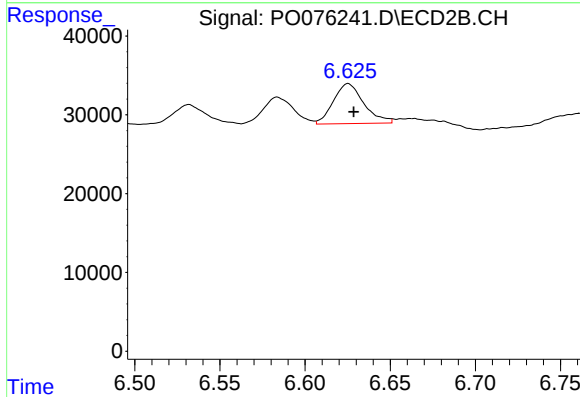


#28 AR-1254-3

R.T.: 6.625 min
Delta R.T.: -0.004 min
Response: 62677
Conc: 20.81 ng/ml m

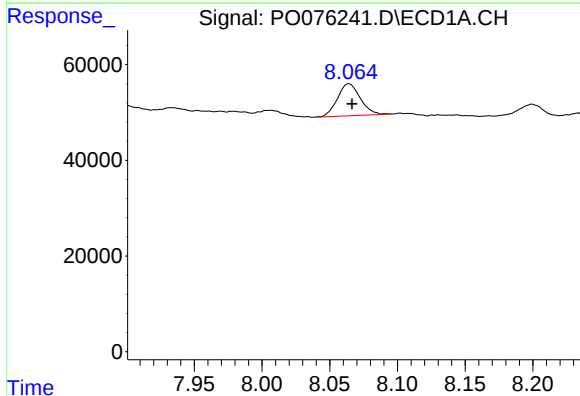


#29 AR-1254-4

R.T.: 8.064 min
Delta R.T.: -0.002 min
Response: 78729
Conc: 37.58 ng/ml

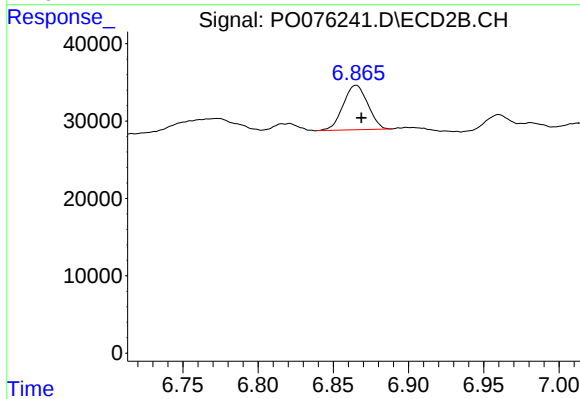

#29 AR-1254-4

R.T.: 6.865 min
Delta R.T.: -0.004 min
Response: 65521
Conc: 37.13 ng/ml

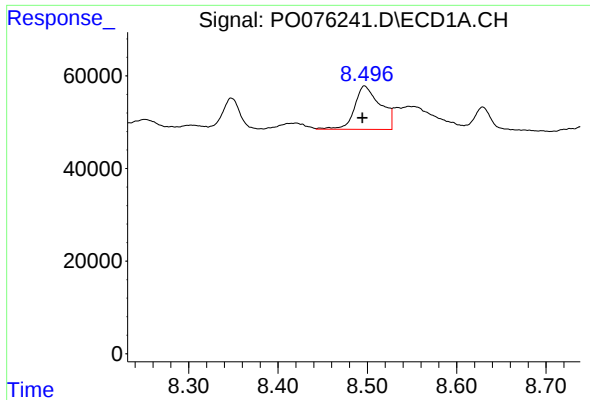


#30 AR-1254-5

R.T.: 8.497 min
Delta R.T.: 0.002 min
Response: 188136
Conc: 81.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
R-LA-4-1-WC

Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:08 PM

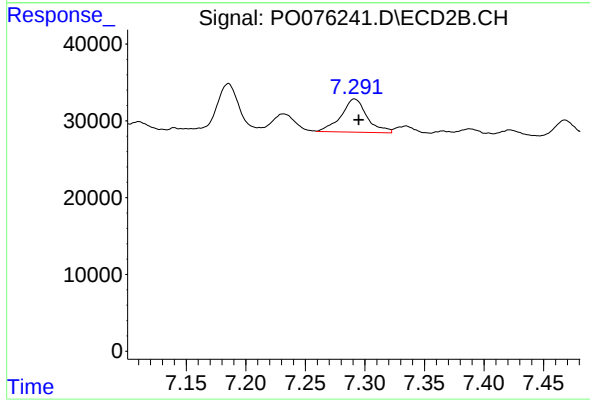

#30 AR-1254-5

R.T.: 7.291 min
Delta R.T.: -0.004 min
Response: 65809
Conc: 25.14 ng/ml