

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
 Data File : P0076252.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 19:23
 Operator : DD\AJ
 Sample : M1693-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-5A

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:01:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:35:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.936	1296984	907731	22.830	21.757
2) SA Decachlor...	10.924	9.202	921824	785713	23.966	20.463
Target Compounds						
26) L6 AR-1254-1	7.157	6.050	535032	503460	261.068m	220.283
27) L6 AR-1254-2	7.387	6.210	903747	630818	290.823m	318.507
28) L6 AR-1254-3	7.771	6.627	1227579	1175782	385.858	390.361
29) L6 AR-1254-4	8.065	6.866	736013	540105	351.295m	306.063
30) L6 AR-1254-5	8.495	7.294	1134648	1441153	494.040m	550.464

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
Data File : P0076252.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 19:23
Operator : DD\AJ
Sample : M1693-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-5A


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:35:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

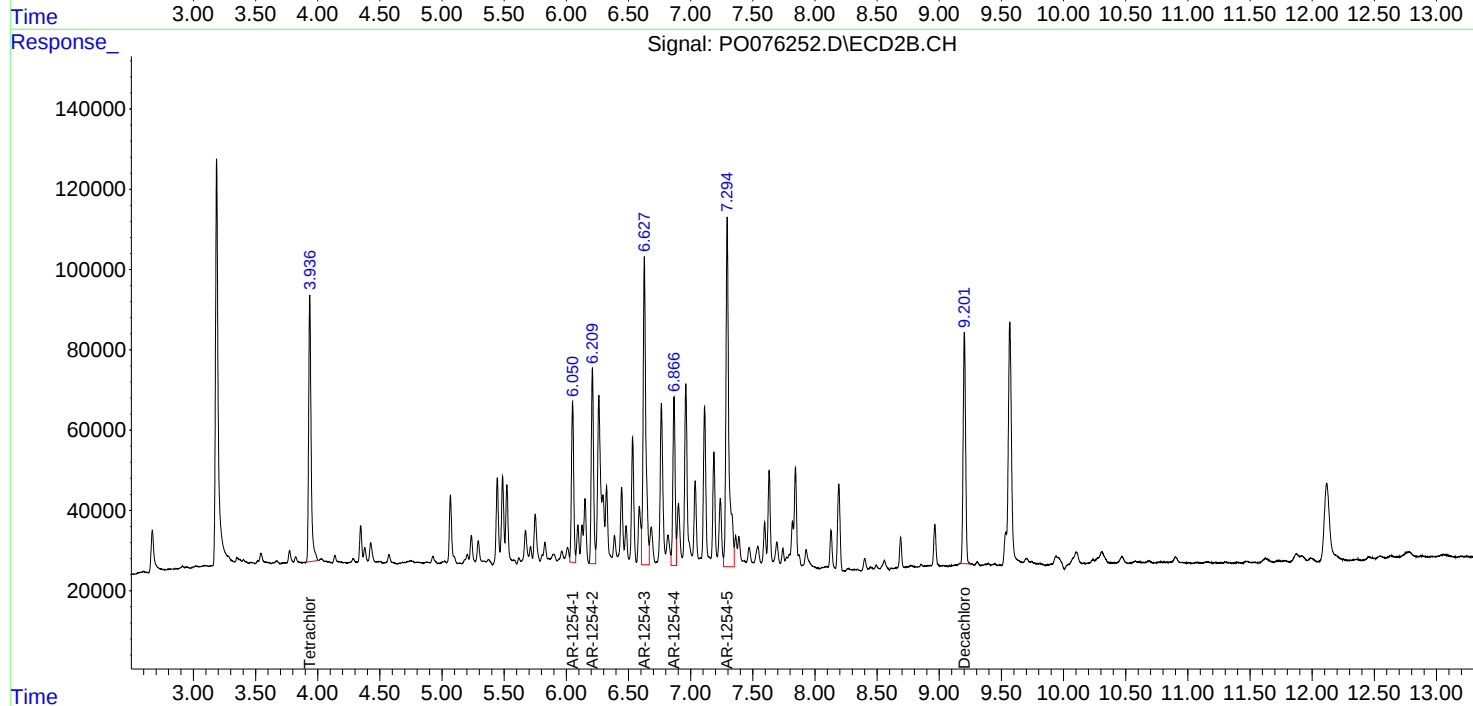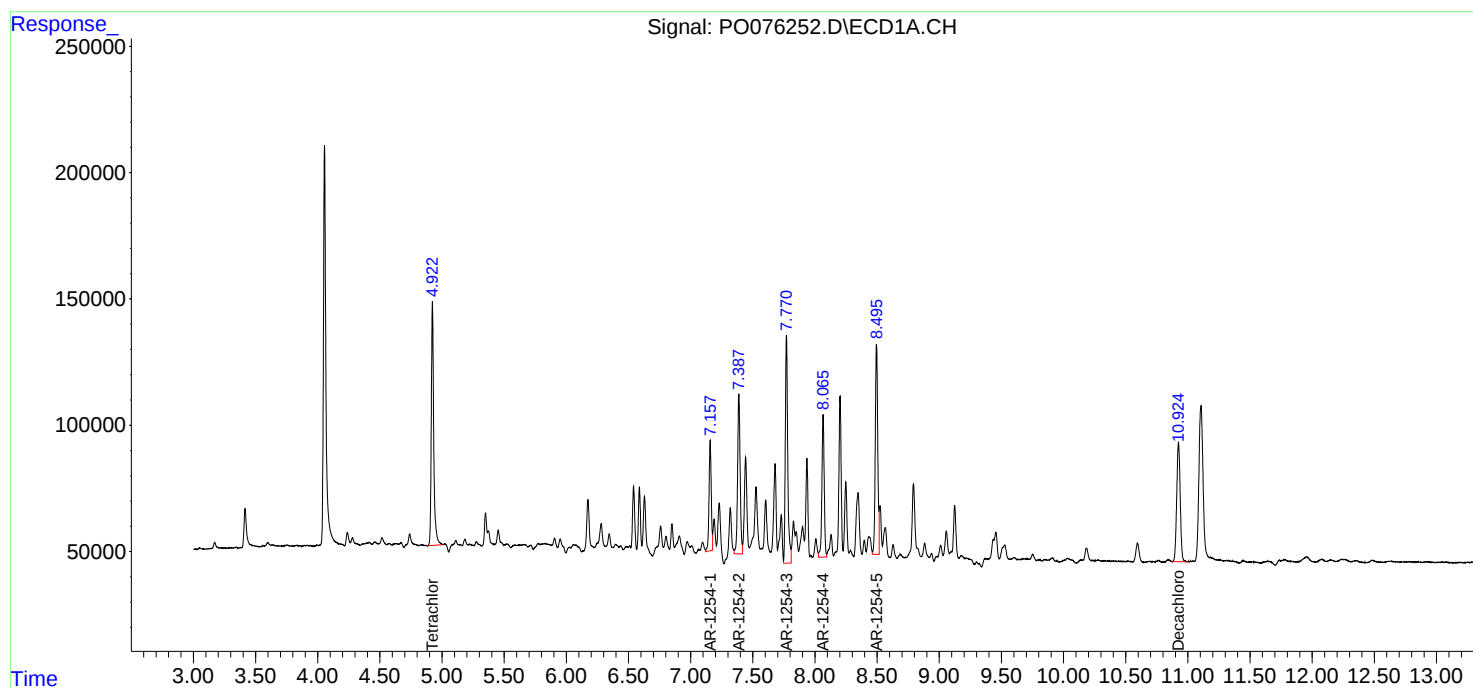

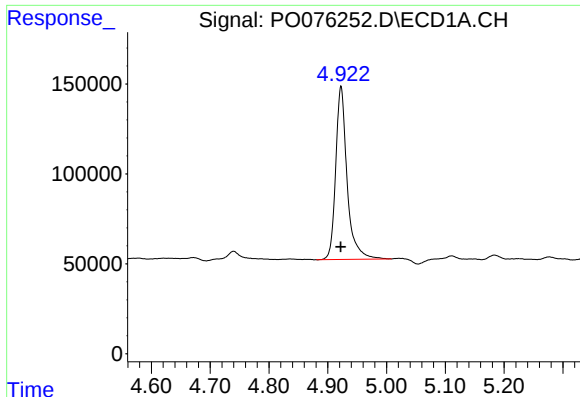


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 1296984
Conc: 22.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5A


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:19 PM

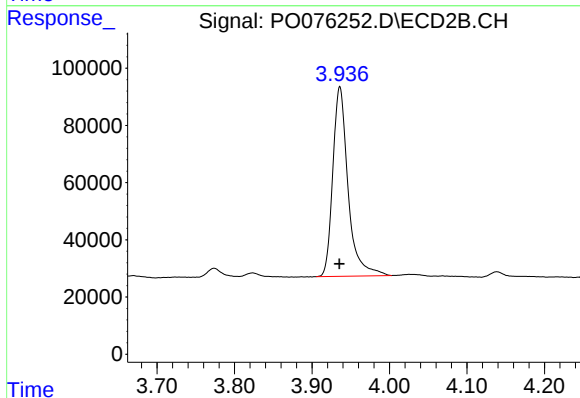


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 907731
Conc: 21.76 ng/ml

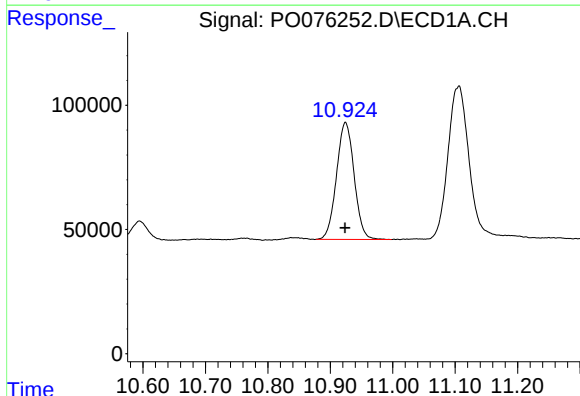


#2 Decachlorobiphenyl

R.T.: 10.924 min
Delta R.T.: 0.000 min
Response: 921824
Conc: 23.97 ng/ml

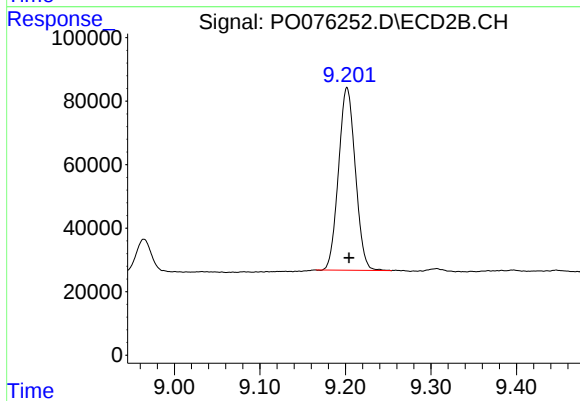

#2 Decachlorobiphenyl

R.T.: 9.202 min
Delta R.T.: -0.002 min
Response: 785713
Conc: 20.46 ng/ml

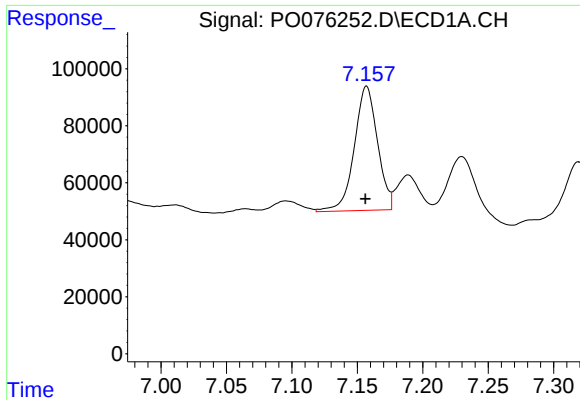


#26 AR-1254-1

R.T.: 7.157 min
Delta R.T.: 0.000 min
Response: 535032
Conc: 261.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-5A


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:19 PM

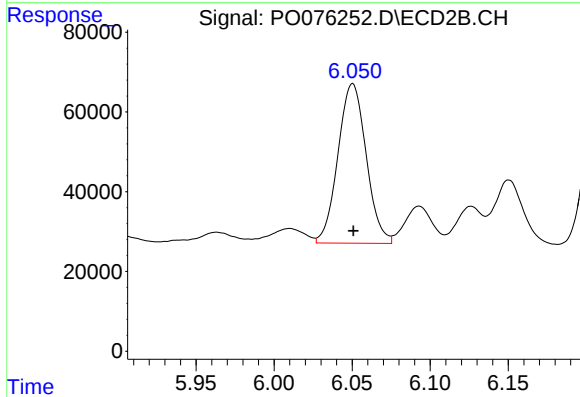


#26 AR-1254-1

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 503460
Conc: 220.28 ng/ml

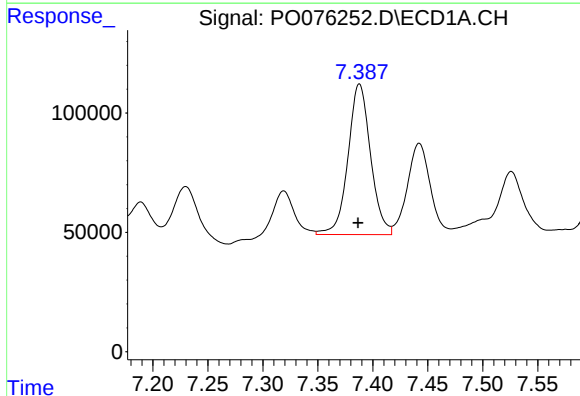


#27 AR-1254-2

R.T.: 7.387 min
Delta R.T.: 0.000 min
Response: 903747
Conc: 290.82 ng/ml m

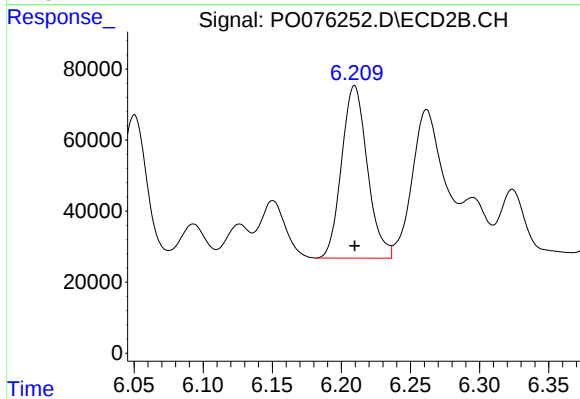

#27 AR-1254-2

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 630818
Conc: 318.51 ng/ml

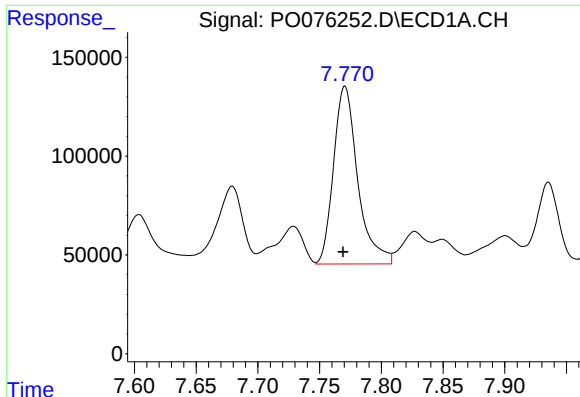


#28 AR-1254-3

R.T.: 7.771 min
Delta R.T.: 0.001 min
Response: 1227579
Conc: 385.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5A


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:19 PM

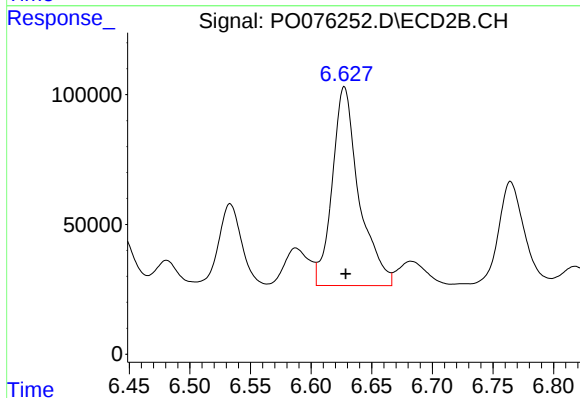


#28 AR-1254-3

R.T.: 6.627 min
Delta R.T.: -0.001 min
Response: 1175782
Conc: 390.36 ng/ml

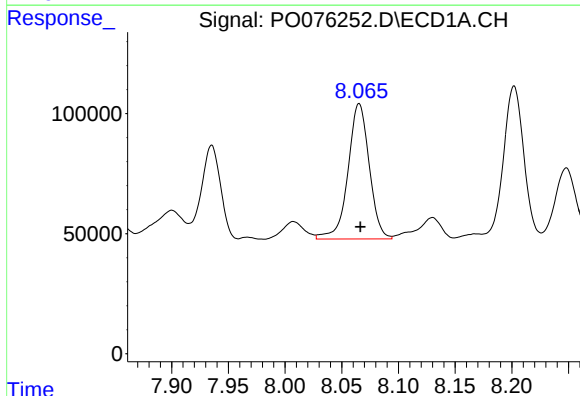


#29 AR-1254-4

R.T.: 8.065 min
Delta R.T.: -0.002 min
Response: 736013
Conc: 351.29 ng/ml m

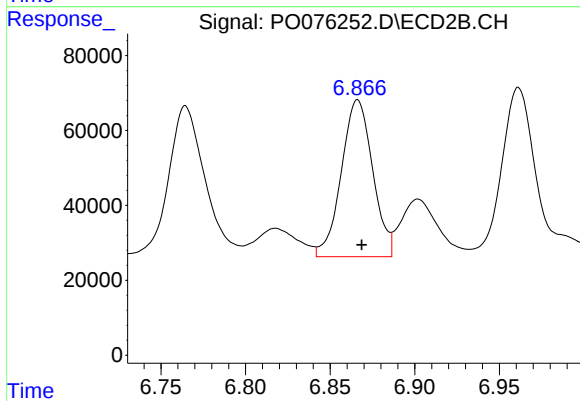

#29 AR-1254-4

R.T.: 6.866 min
Delta R.T.: -0.002 min
Response: 540105
Conc: 306.06 ng/ml

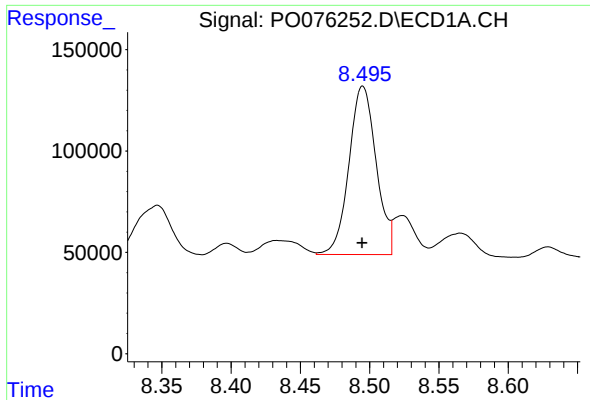


#30 AR-1254-5

R.T.: 8.495 min
Delta R.T.: 0.000 min
Response: 1134648
Conc: 494.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-5A

Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:19 PM

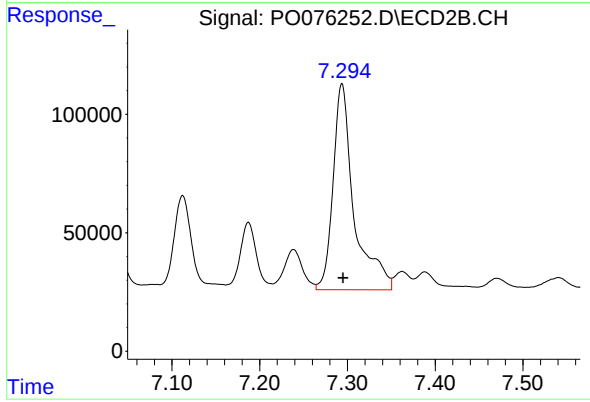

#30 AR-1254-5

R.T.: 7.294 min
Delta R.T.: -0.001 min
Response: 1441153
Conc: 550.46 ng/ml