

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
 Data File : P0076258.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 21:06
 Operator : DD\AJ
 Sample : M1687-29
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1031-1032

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:01:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:38:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.935	1356906	968777	23.885	23.220
2) SA Decachlor...	10.918	9.198	968838	895167	25.188	23.313
Target Compounds						
26) L6 AR-1254-1	7.154	6.045	22335	28882	10.898	12.637m
27) L6 AR-1254-2	7.384	6.206	52815	40513	16.996	20.456
28) L6 AR-1254-3	7.767	6.624	60255	52858	18.940	17.549
29) L6 AR-1254-4	8.063	6.864	54872	35087	26.190	19.883
30) L6 AR-1254-5	8.492	7.291	39114	44667	17.031m	17.061

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
Data File : P0076258.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 21:06
Operator : DD\AJ
Sample : M1687-29
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AUD-1031-1032


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:38:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

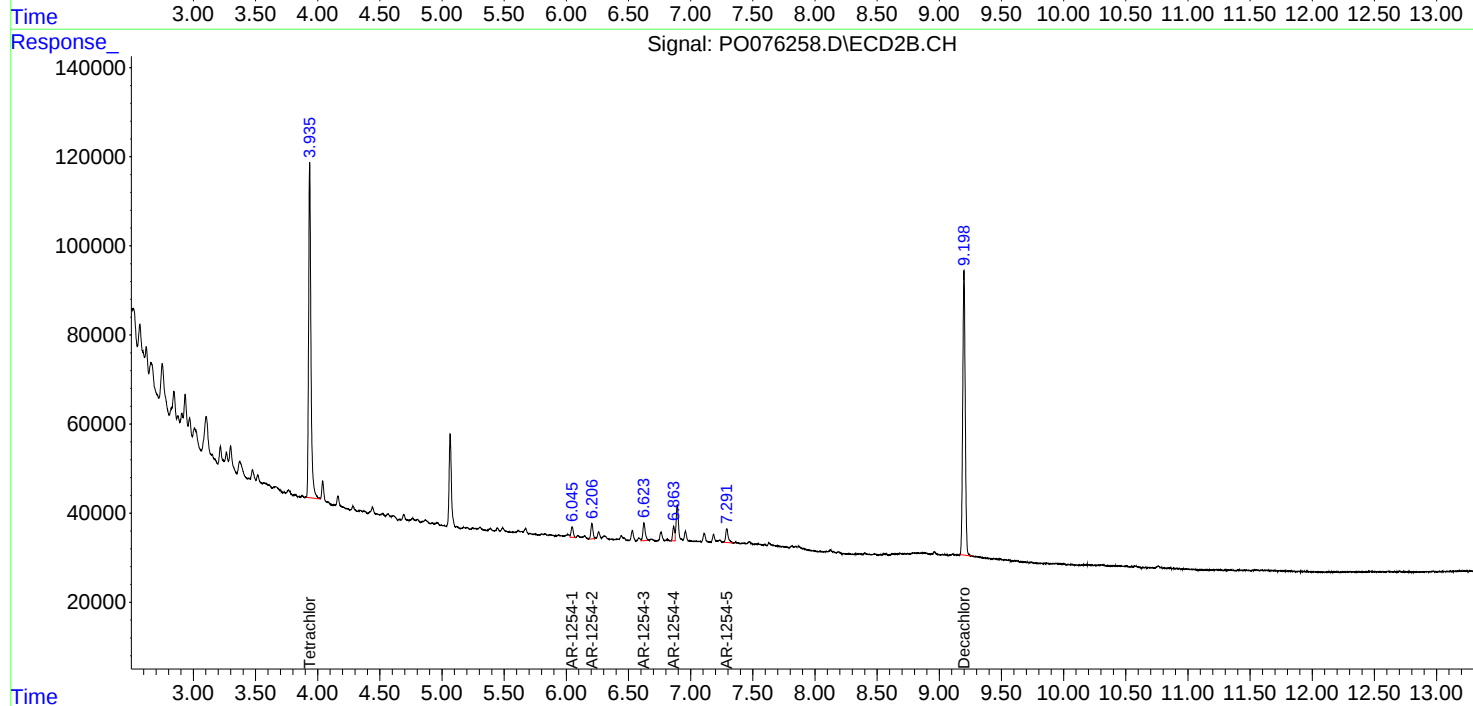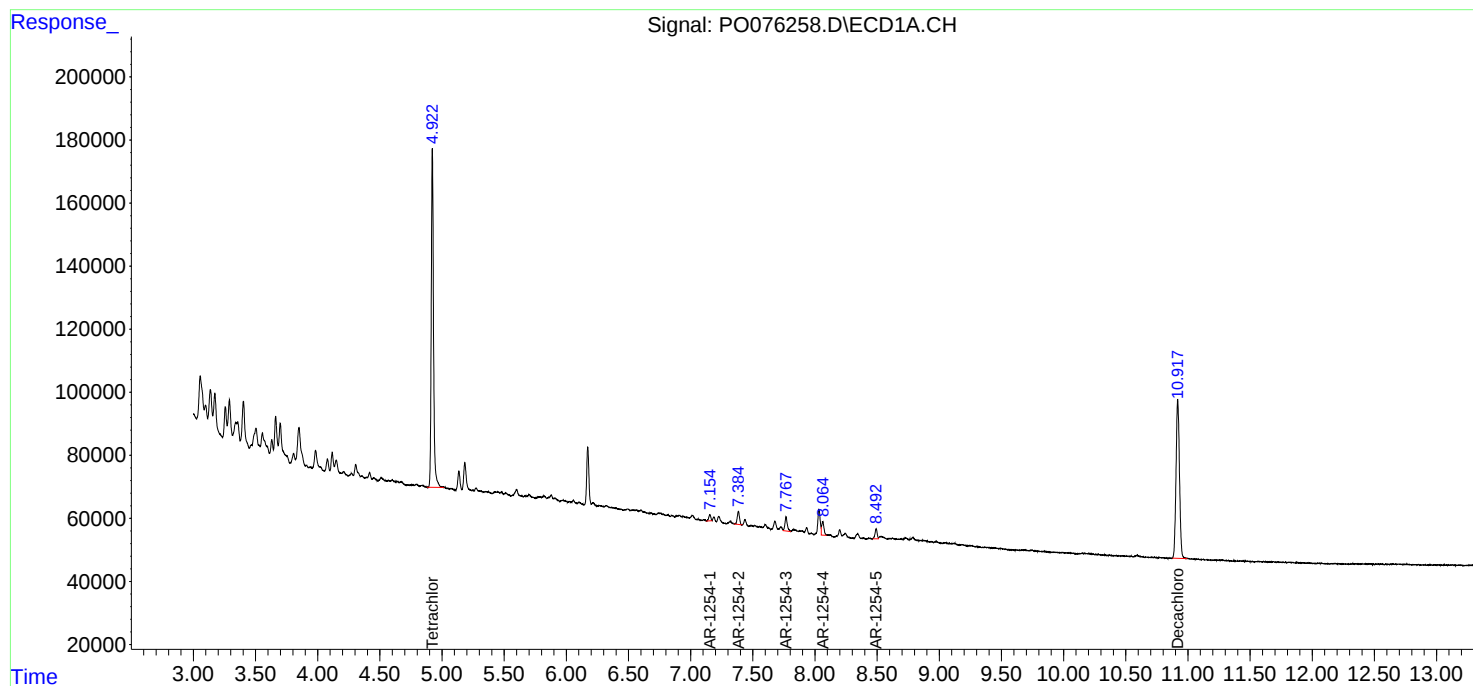

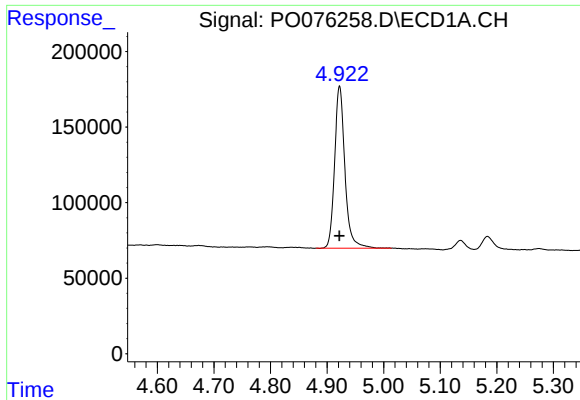


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 1356906
Conc: 23.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1031-1032


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:21 PM

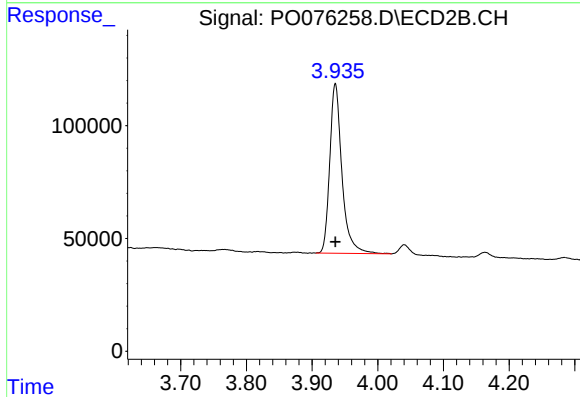


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 968777
Conc: 23.22 ng/ml

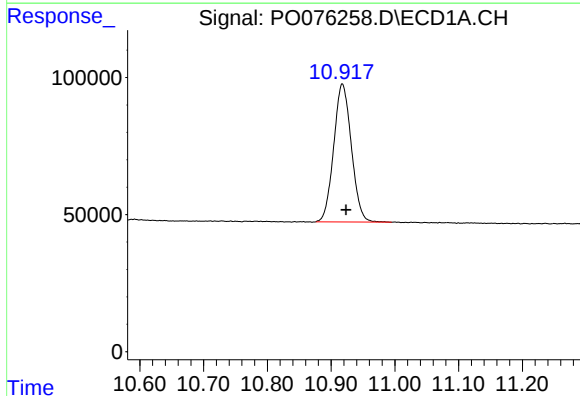


#2 Decachlorobiphenyl

R.T.: 10.918 min
Delta R.T.: -0.006 min
Response: 968838
Conc: 25.19 ng/ml

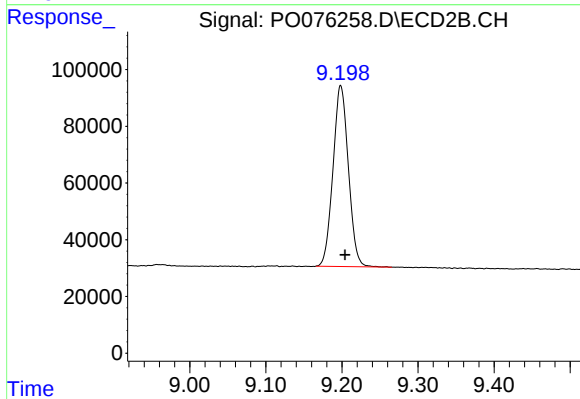

#2 Decachlorobiphenyl

R.T.: 9.198 min
Delta R.T.: -0.006 min
Response: 895167
Conc: 23.31 ng/ml

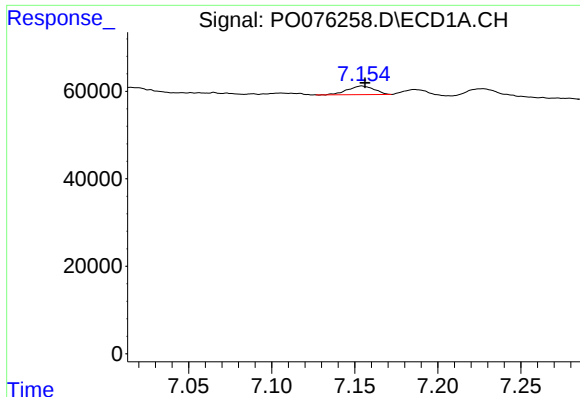


#26 AR-1254-1

R.T.: 7.154 min
Delta R.T.: -0.002 min
Response: 22335
Conc: 10.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1031-1032


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:21 PM

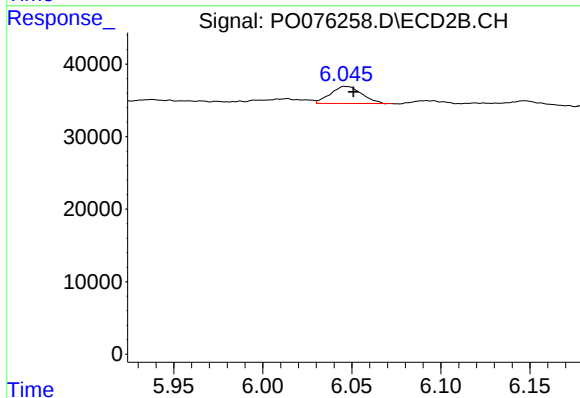


#26 AR-1254-1

R.T.: 6.045 min
Delta R.T.: -0.006 min
Response: 28882
Conc: 12.64 ng/ml m

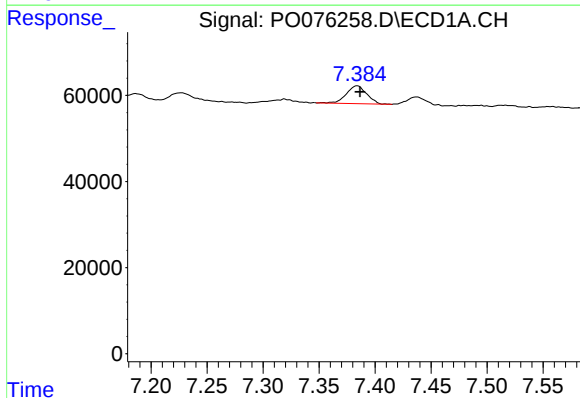


#27 AR-1254-2

R.T.: 7.384 min
Delta R.T.: -0.003 min
Response: 52815
Conc: 17.00 ng/ml

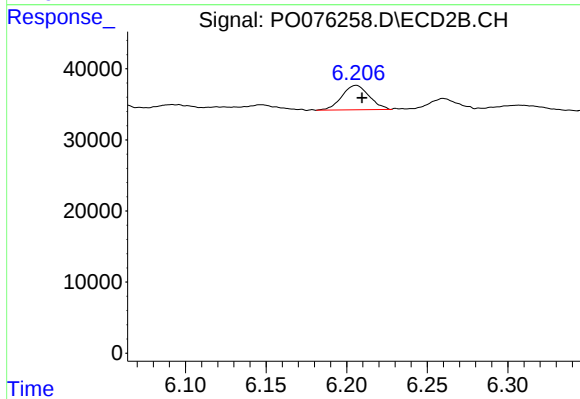

#27 AR-1254-2

R.T.: 6.206 min
Delta R.T.: -0.004 min
Response: 40513
Conc: 20.46 ng/ml

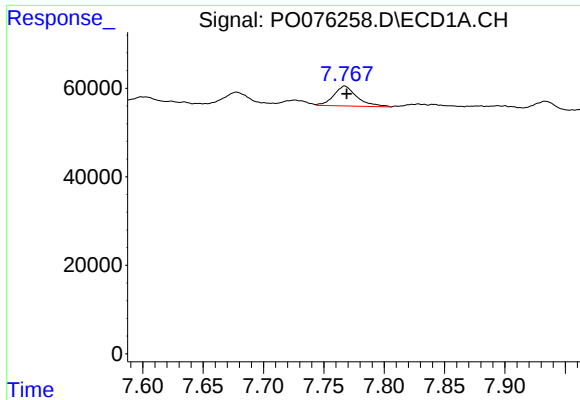


#28 AR-1254-3

R.T.: 7.767 min
Delta R.T.: -0.002 min
Response: 60255
Conc: 18.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1031-1032


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:21 PM

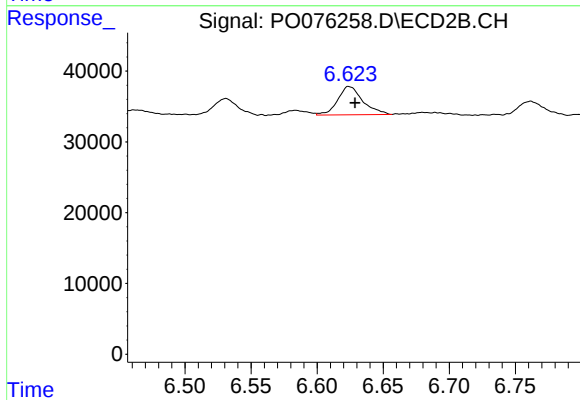


#28 AR-1254-3

R.T.: 6.624 min
Delta R.T.: -0.004 min
Response: 52858
Conc: 17.55 ng/ml

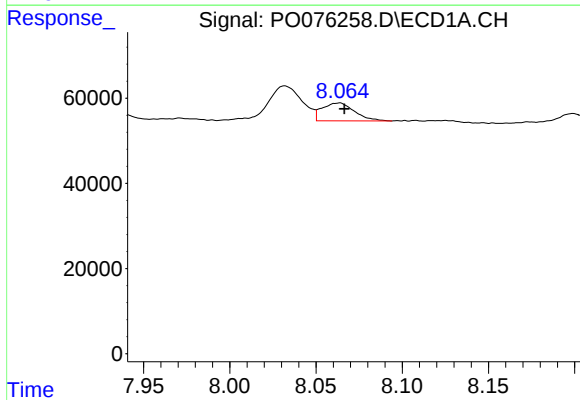


#29 AR-1254-4

R.T.: 8.063 min
Delta R.T.: -0.003 min
Response: 54872
Conc: 26.19 ng/ml

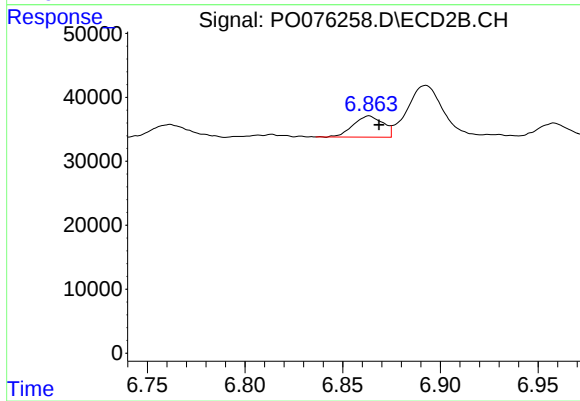

#29 AR-1254-4

R.T.: 6.864 min
Delta R.T.: -0.005 min
Response: 35087
Conc: 19.88 ng/ml

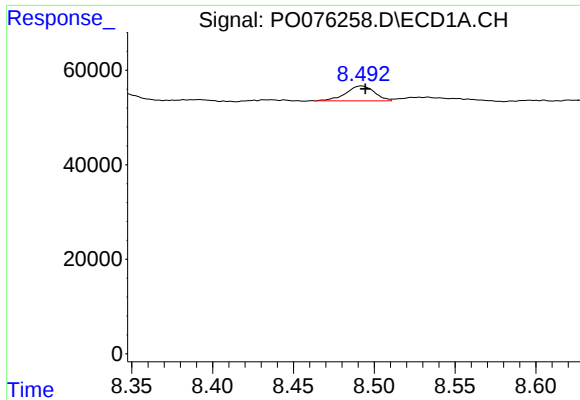


#30 AR-1254-5

R.T.: 8.492 min
Delta R.T.: -0.003 min
Response: 39114
Conc: 17.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AUD-1031-1032

Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:21 PM

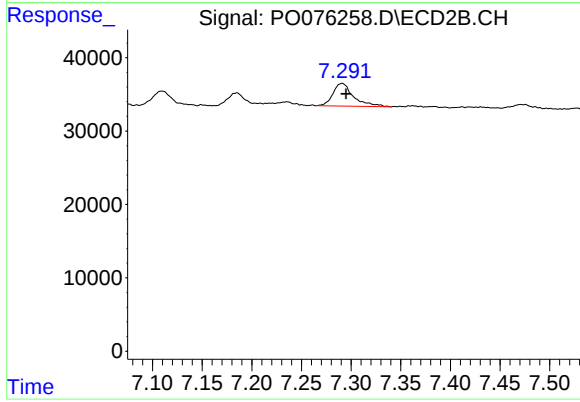

#30 AR-1254-5

R.T.: 7.291 min
Delta R.T.: -0.004 min
Response: 44667
Conc: 17.06 ng/ml