

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
 Data File : P0076260.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Mar 2021 21:40
 Operator : DD\AJ
 Sample : M1687-38
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1049-1051

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:01:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:39:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	3.935	1354347	1034567	23.840	24.797
2) SA Decachlor...	10.919	9.198	589864	552411	15.336	14.387
Target Compounds						
26) L6 AR-1254-1	7.155	6.048	259503	345915	126.624m	151.351
27) L6 AR-1254-2	7.384	6.208	615351	493545	198.018	249.196 #
28) L6 AR-1254-3	7.767	6.625	611009	644234	192.055	213.887
29) L6 AR-1254-4	8.064	6.865	549155	483096	262.109	273.757
30) L6 AR-1254-5	8.493	7.292	461602	499210	200.987	190.678

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031721\
Data File : PO076260.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Mar 2021 21:40
Operator : DD\AJ
Sample : M1687-38
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-1049-1051


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:39:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

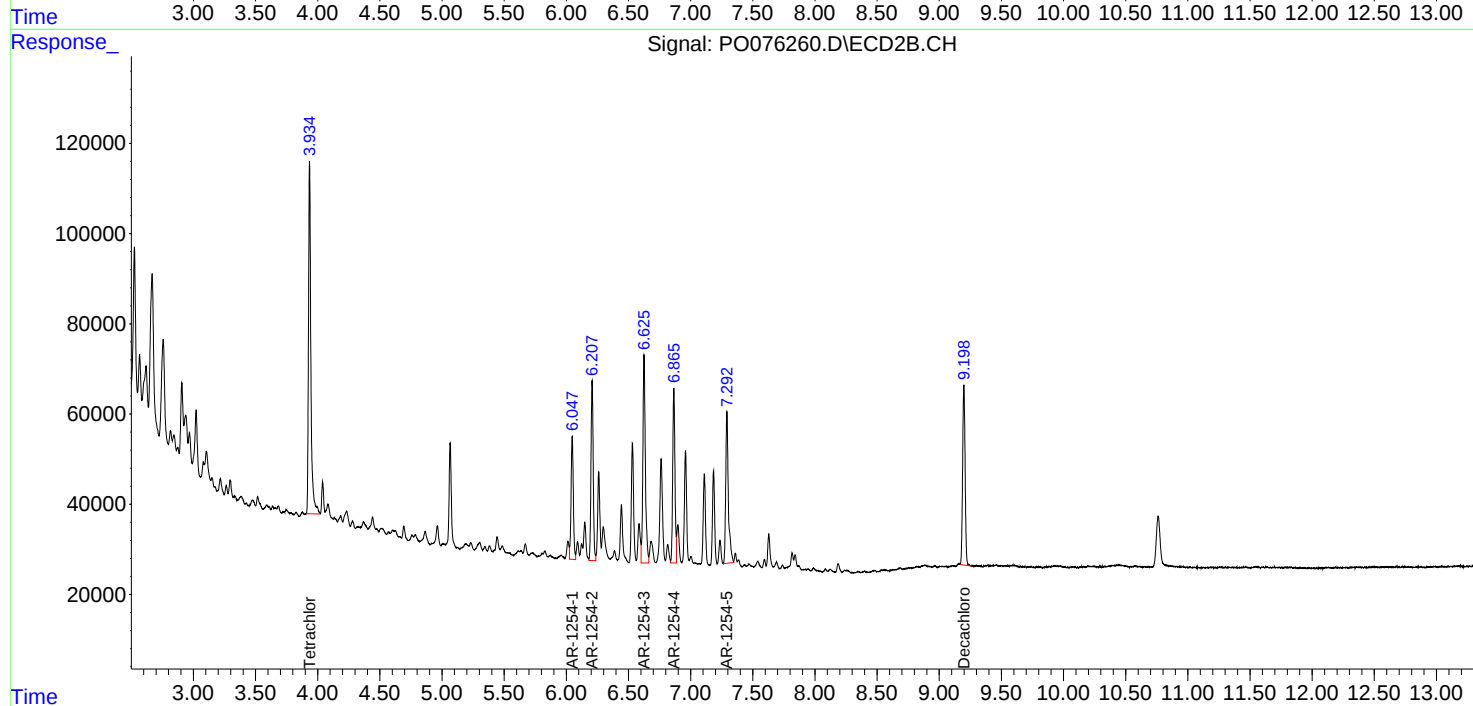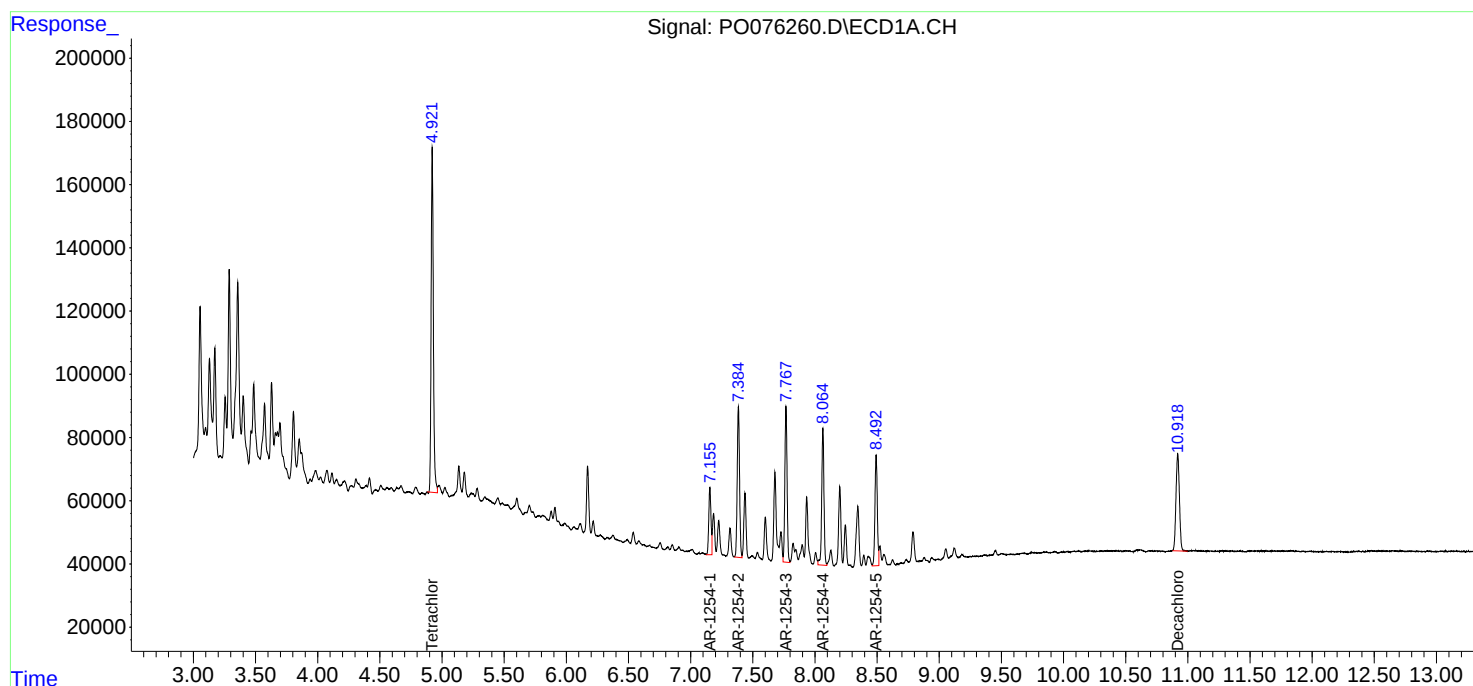

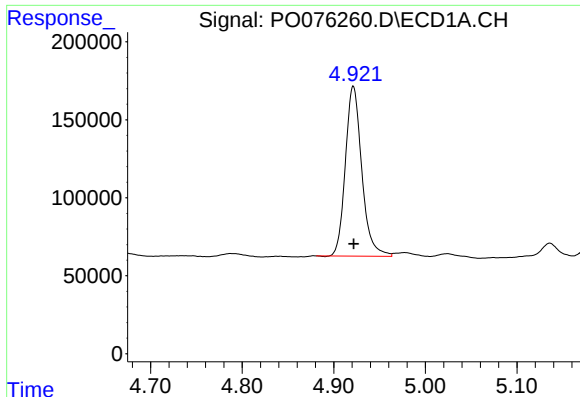


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: 0.000 min
Response: 1354347
Conc: 23.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1049-1051


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:25 PM

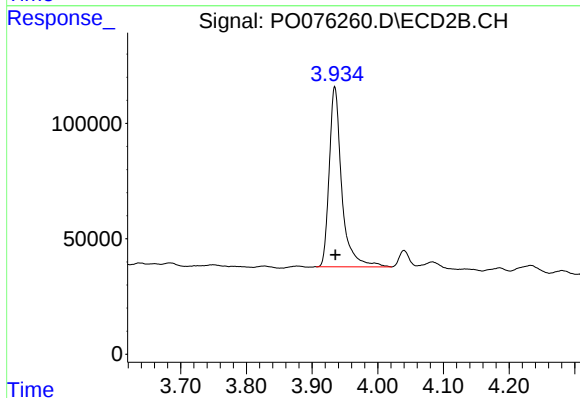


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 1034567
Conc: 24.80 ng/ml

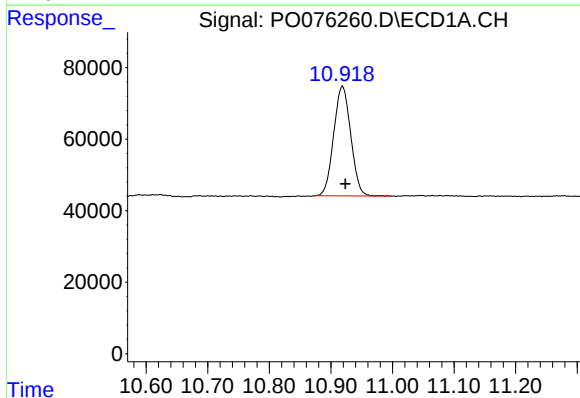


#2 Decachlorobiphenyl

R.T.: 10.919 min
Delta R.T.: -0.005 min
Response: 589864
Conc: 15.34 ng/ml

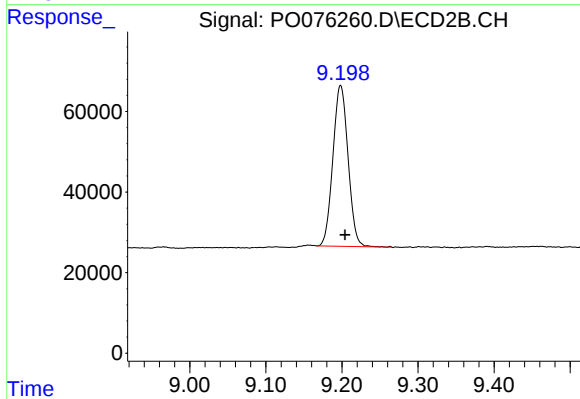

#2 Decachlorobiphenyl

R.T.: 9.198 min
Delta R.T.: -0.006 min
Response: 552411
Conc: 14.39 ng/ml

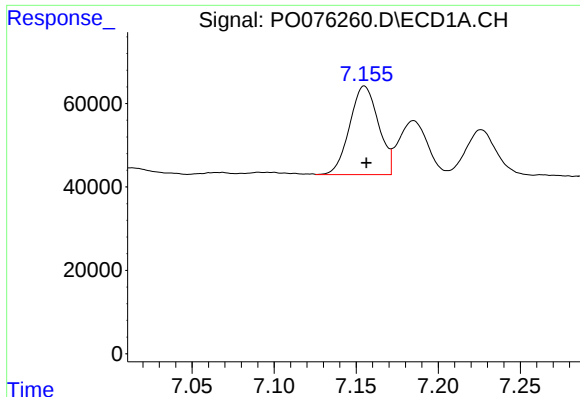


#26 AR-1254-1

R.T.: 7.155 min
Delta R.T.: -0.002 min
Response: 259503
Conc: 126.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AUD-1049-1051


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:25 PM

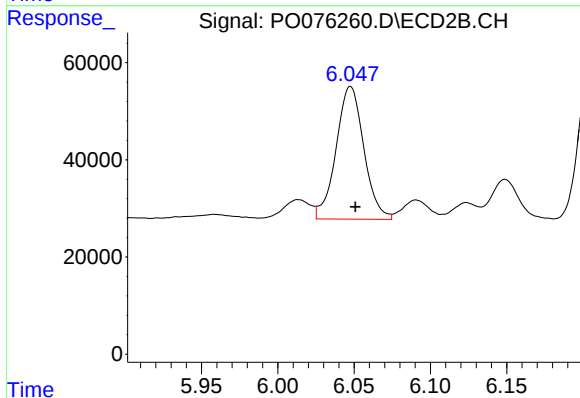


#26 AR-1254-1

R.T.: 6.048 min
Delta R.T.: -0.003 min
Response: 345915
Conc: 151.35 ng/ml

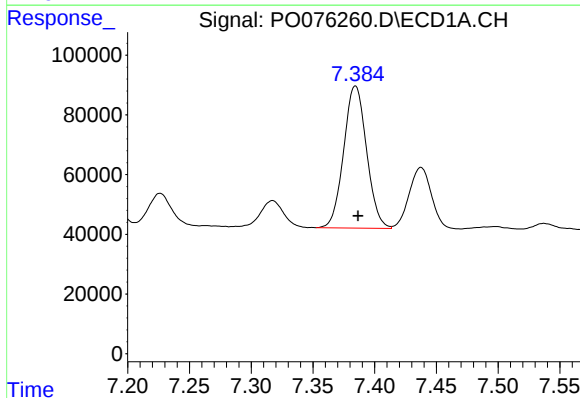


#27 AR-1254-2

R.T.: 7.384 min
Delta R.T.: -0.002 min
Response: 615351
Conc: 198.02 ng/ml

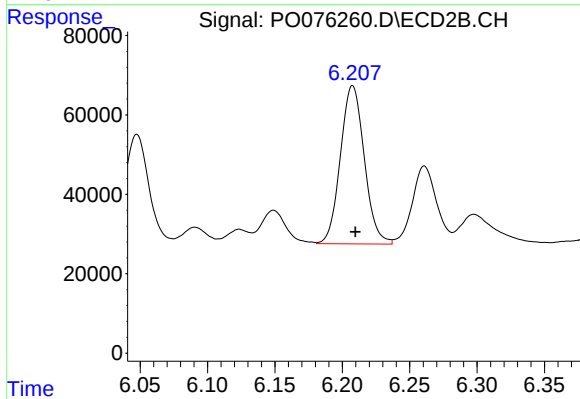

#27 AR-1254-2

R.T.: 6.208 min
Delta R.T.: -0.002 min
Response: 493545
Conc: 249.20 ng/ml

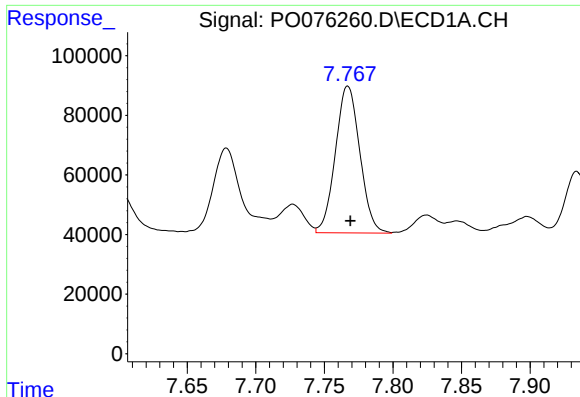


#28 AR-1254-3

R.T.: 7.767 min
Delta R.T.: -0.002 min
Response: 611009
Conc: 192.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1049-1051


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:25 PM

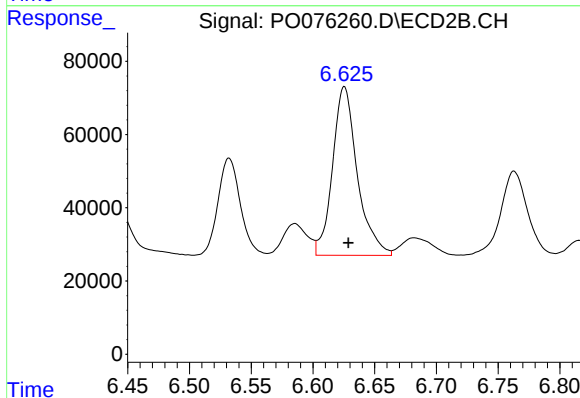


#28 AR-1254-3

R.T.: 6.625 min
Delta R.T.: -0.003 min
Response: 644234
Conc: 213.89 ng/ml

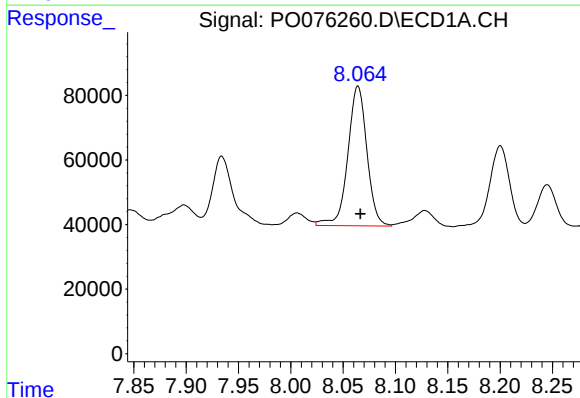


#29 AR-1254-4

R.T.: 8.064 min
Delta R.T.: -0.002 min
Response: 549155
Conc: 262.11 ng/ml

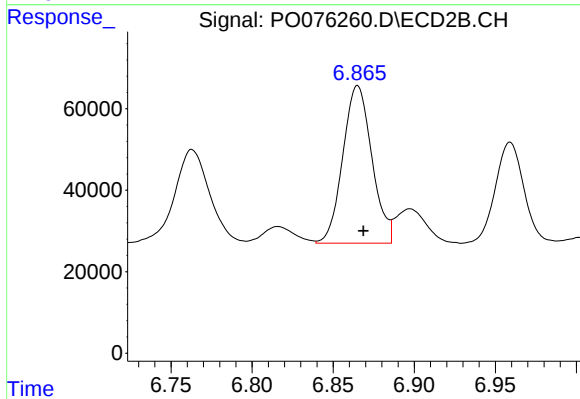

#29 AR-1254-4

R.T.: 6.865 min
Delta R.T.: -0.004 min
Response: 483096
Conc: 273.76 ng/ml

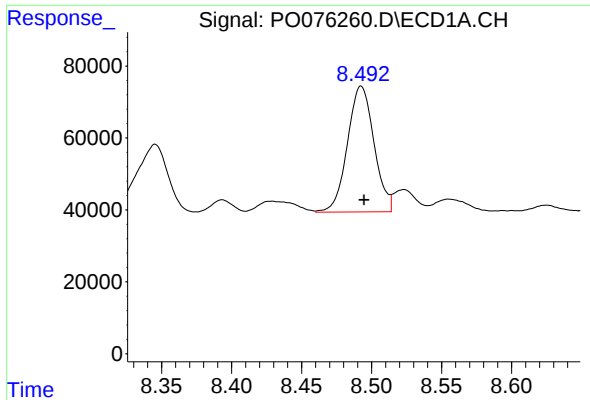


#30 AR-1254-5

R.T.: 8.493 min
Delta R.T.: -0.002 min
Response: 461602
Conc: 200.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1049-1051

Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:25 PM

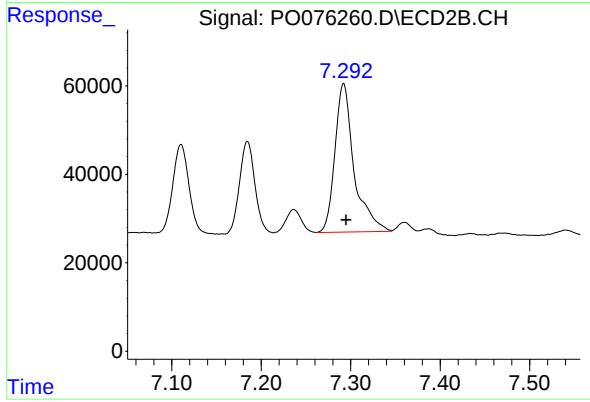

#30 AR-1254-5

R.T.: 7.292 min
Delta R.T.: -0.003 min
Response: 499210
Conc: 190.68 ng/ml