

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031721\
 Data File : P0076275.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2021 2:31
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 3/18/2021 4:01:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 06:53:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.935	3373428	2357173	59.382	56.498
2) SA Decachlor...	10.925	9.200	2372336	2176103	61.677	56.673
Target Compounds						
26) L6 AR-1254-1	7.156	6.048	1105268	1278327	539.312m	559.318
27) L6 AR-1254-2	7.386	6.208	1784759	1153139	574.329m	582.232
28) L6 AR-1254-3	7.769	6.626	1870600	1752666	587.975m	581.888
29) L6 AR-1254-4	8.065	6.866	1256433	999565	599.688m	566.426
30) L6 AR-1254-5	8.494	7.293	1370860	1539050	596.889	587.856

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031721\
Data File : PO076275.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2021 2:31
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 06:53:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

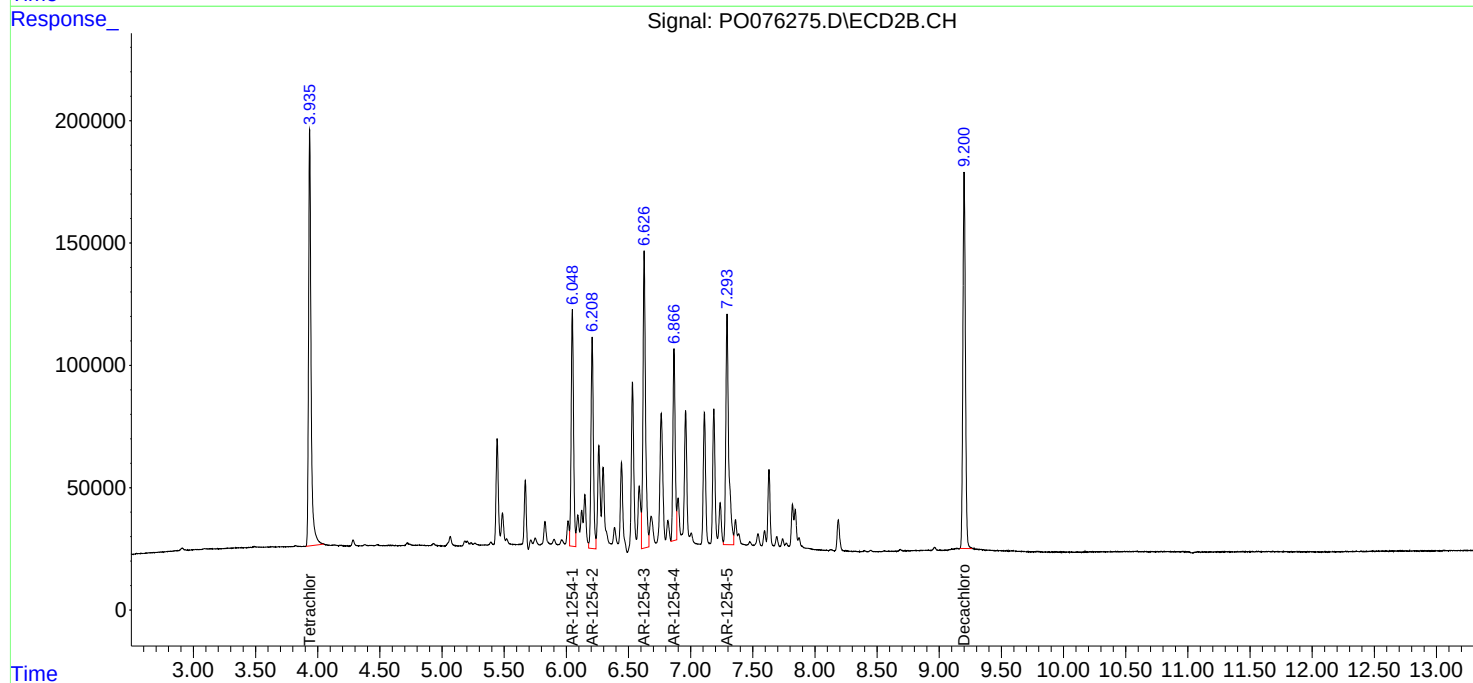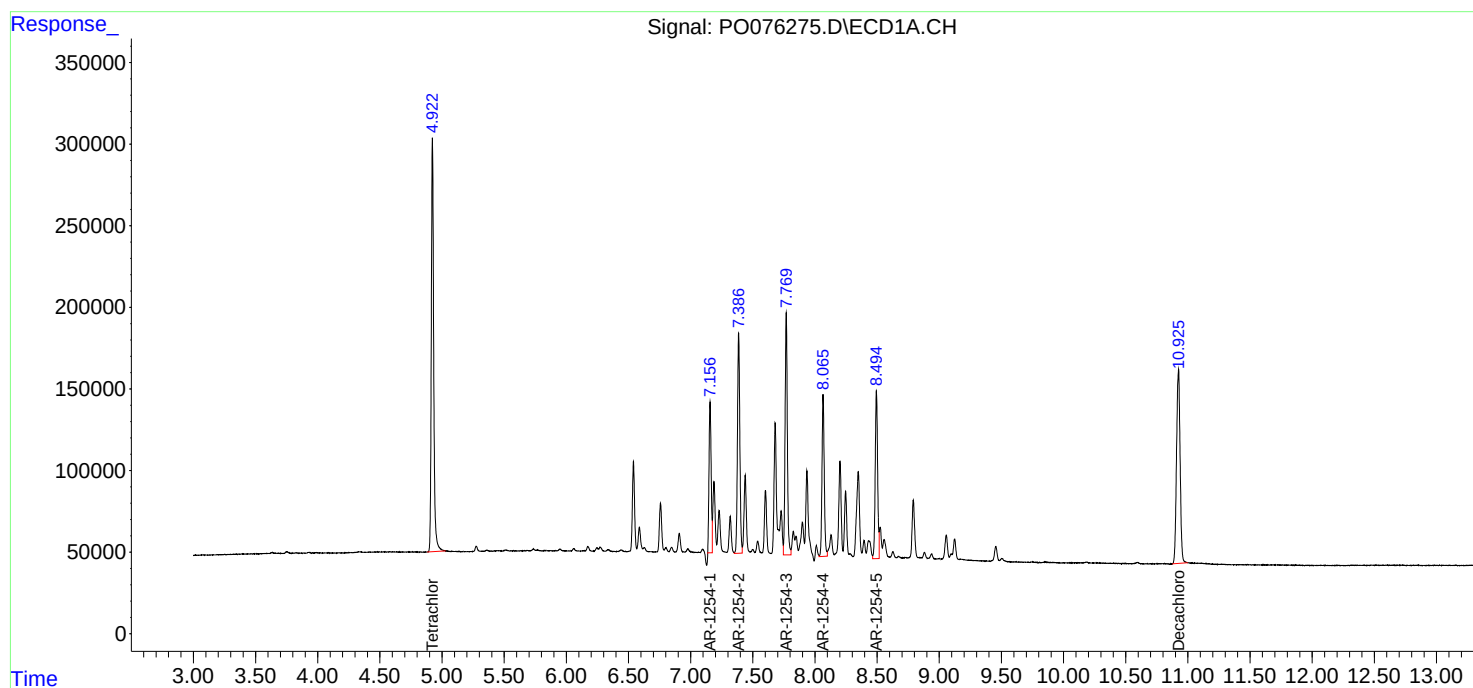

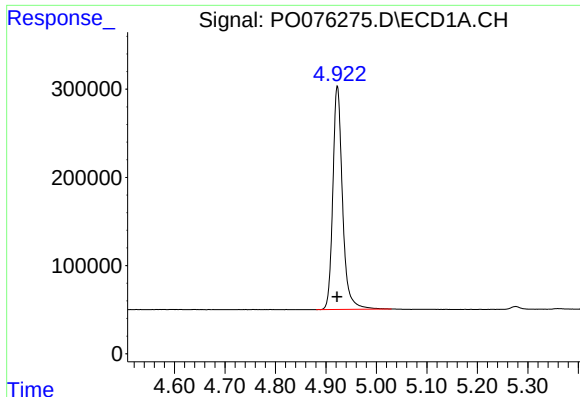


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 3373428
Conc: 59.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:32 PM

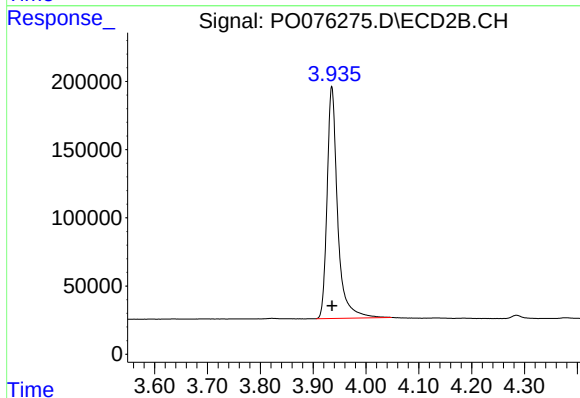


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 2357173
Conc: 56.50 ng/ml

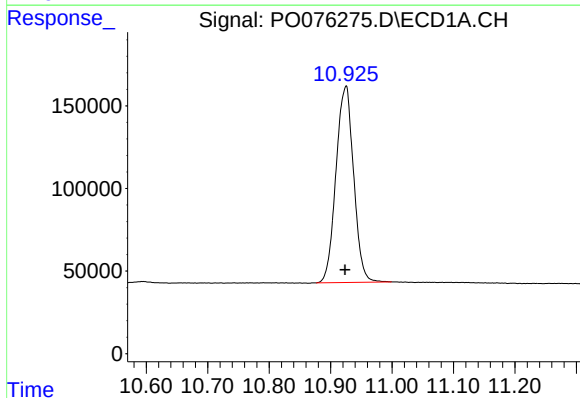


#2 Decachlorobiphenyl

R.T.: 10.925 min
Delta R.T.: 0.002 min
Response: 2372336
Conc: 61.68 ng/ml

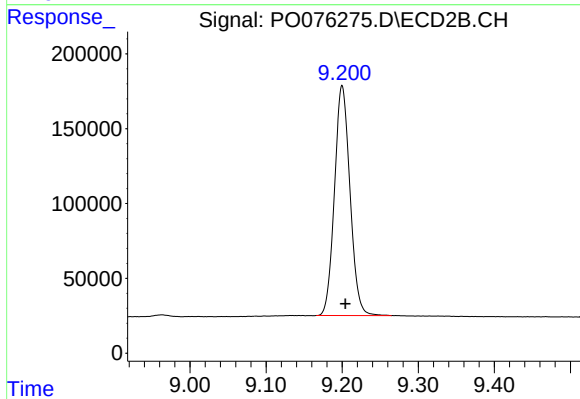

#2 Decachlorobiphenyl

R.T.: 9.200 min
Delta R.T.: -0.004 min
Response: 2176103
Conc: 56.67 ng/ml

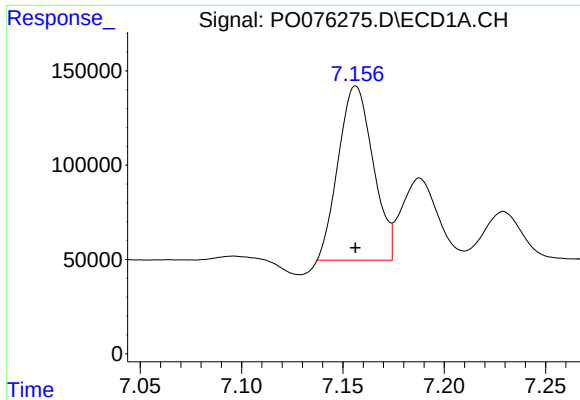


#26 AR-1254-1

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 1105268
Conc: 539.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:32 PM

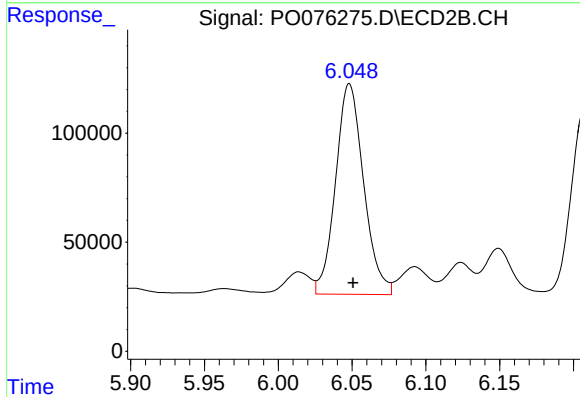


#26 AR-1254-1

R.T.: 6.048 min
Delta R.T.: -0.003 min
Response: 1278327
Conc: 559.32 ng/ml

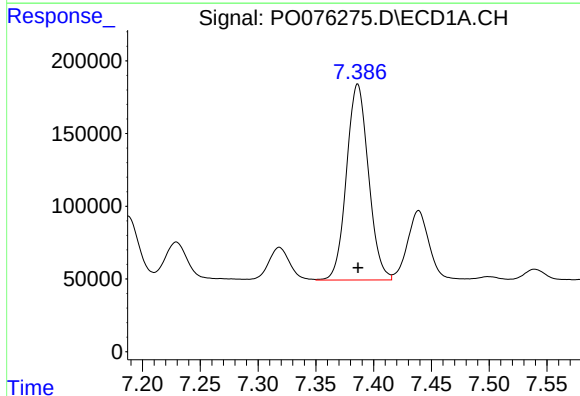


#27 AR-1254-2

R.T.: 7.386 min
Delta R.T.: 0.000 min
Response: 1784759
Conc: 574.33 ng/ml m

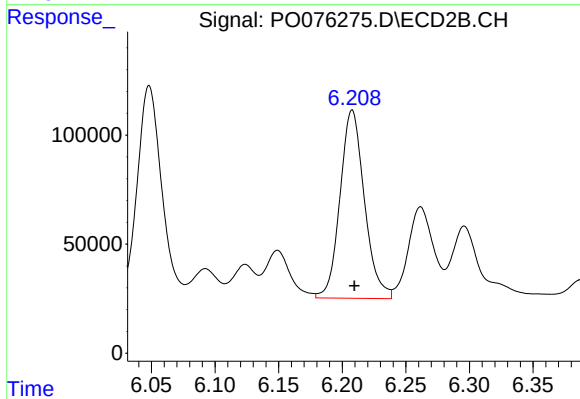

#27 AR-1254-2

R.T.: 6.208 min
Delta R.T.: -0.002 min
Response: 1153139
Conc: 582.23 ng/ml

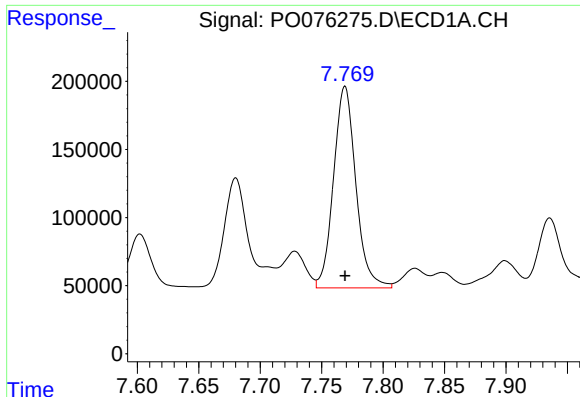


#28 AR-1254-3

R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 1870600
Conc: 587.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:32 PM

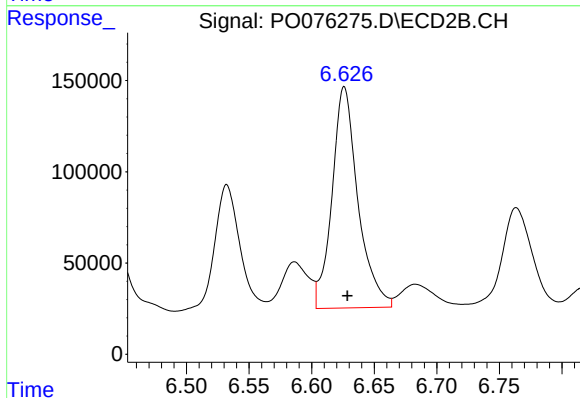


#28 AR-1254-3

R.T.: 6.626 min
Delta R.T.: -0.003 min
Response: 1752666
Conc: 581.89 ng/ml

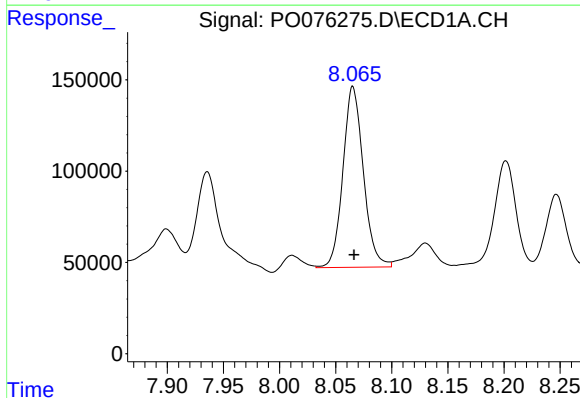


#29 AR-1254-4

R.T.: 8.065 min
Delta R.T.: -0.002 min
Response: 1256433
Conc: 599.69 ng/ml m

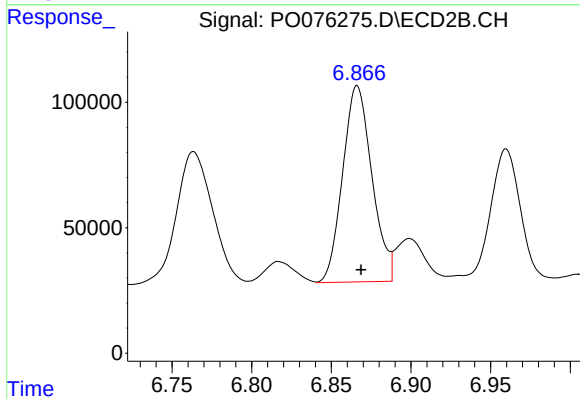

#29 AR-1254-4

R.T.: 6.866 min
Delta R.T.: -0.002 min
Response: 999565
Conc: 566.43 ng/ml

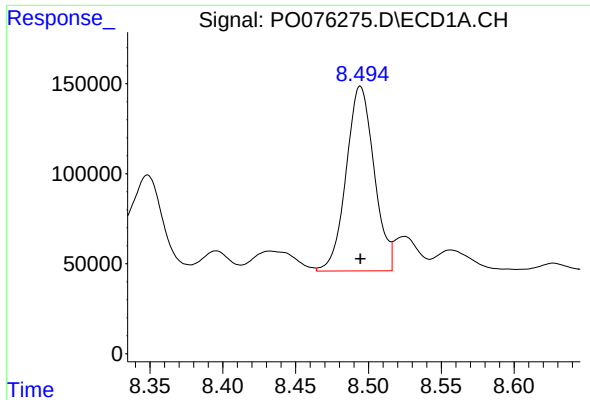


#30 AR-1254-5

R.T.: 8.494 min
Delta R.T.: 0.000 min
Response: 1370860
Conc: 596.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
3/18/2021 4:01:32 PM

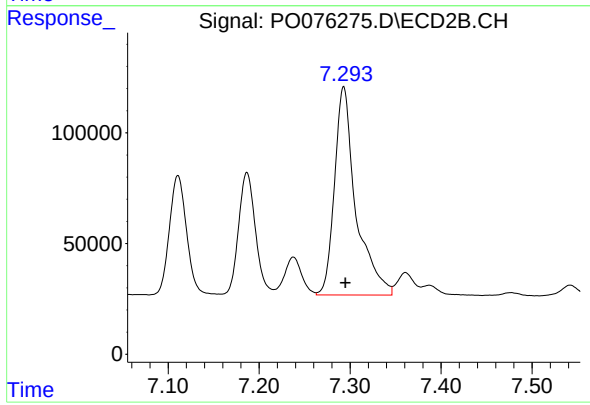

#30 AR-1254-5

R.T.: 7.293 min
Delta R.T.: -0.002 min
Response: 1539050
Conc: 587.86 ng/ml