

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0031821\  
 Data File : P0076319.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 18 Mar 2021 22:43  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 19 02:47:33 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031521.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Mar 16 07:18:57 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1  | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|---------|--------|--------|--------|
| -----                       |                 |        |       |         |        |        |        |
| System Monitoring Compounds |                 |        |       |         |        |        |        |
| 1)                          | SA Tetrachlo... | 4.924  | 3.936 | 1231549 | 906597 | 21.679 | 21.730 |
| 2)                          | SA Decachlor... | 10.927 | 9.202 | 974775  | 926353 | 25.343 | 24.125 |

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0031821\  
Data File : P0076319.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 18 Mar 2021 22:43  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 19 02:47:33 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0031521.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Mar 16 07:18:57 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

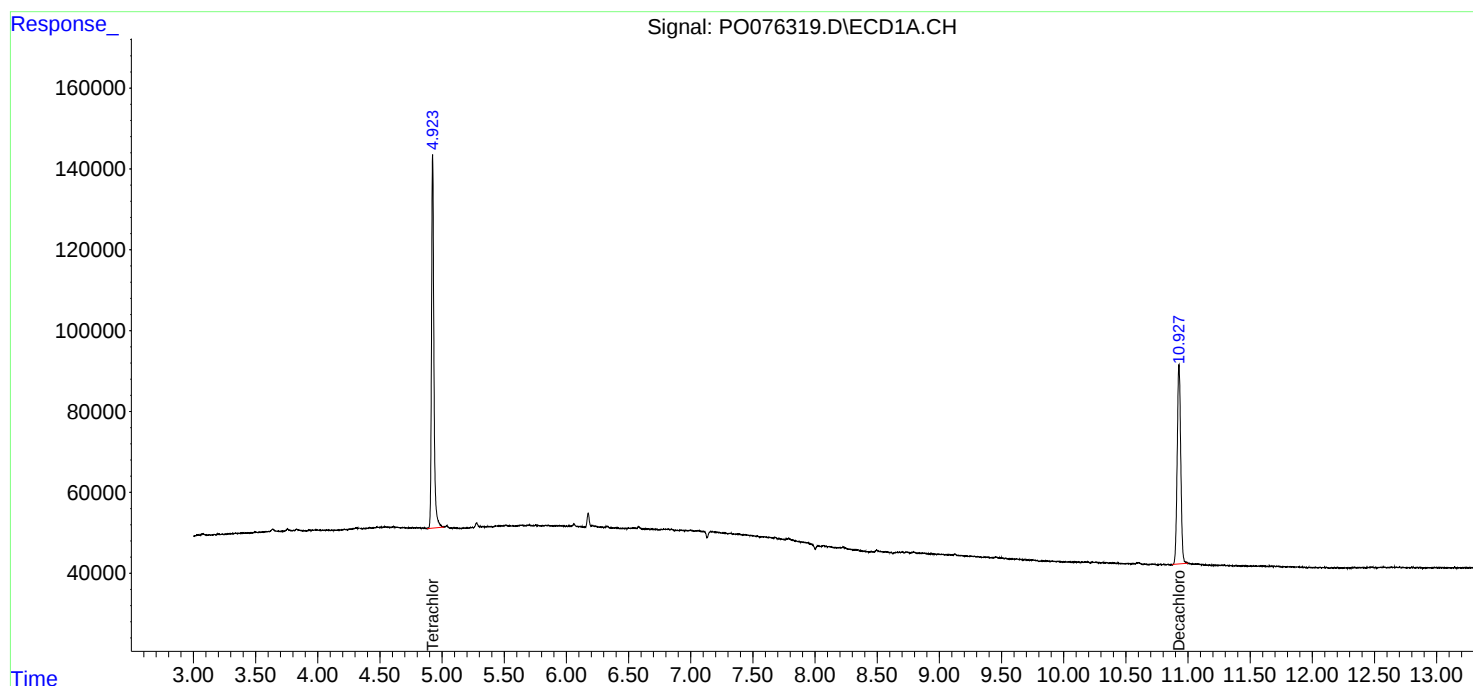


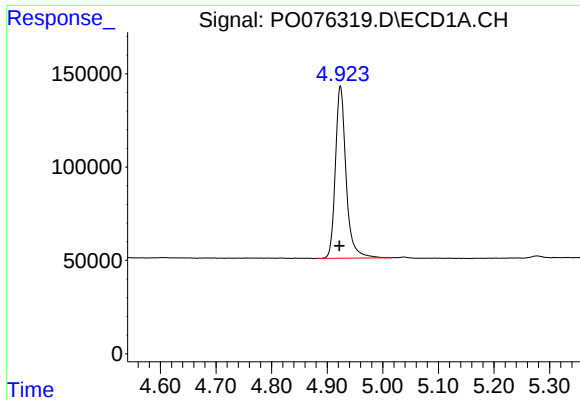

#1 Tetrachloro-m-xylene


R.T.: 4.924 min  
Delta R.T.: 0.002 min  
Response: 1231549  
Conc: 21.68 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
I.BLK

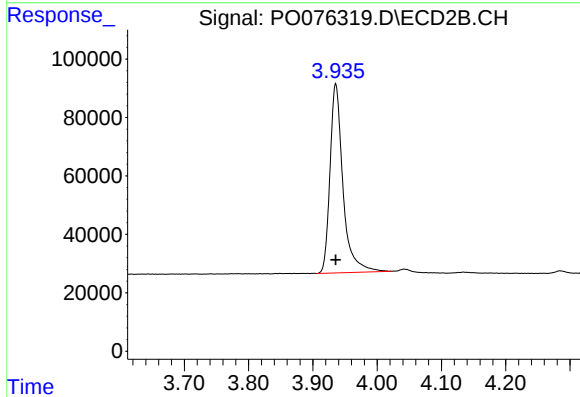


#1 Tetrachloro-m-xylene

R.T.: 3.936 min  
Delta R.T.: 0.000 min  
Response: 906597  
Conc: 21.73 ng/ml

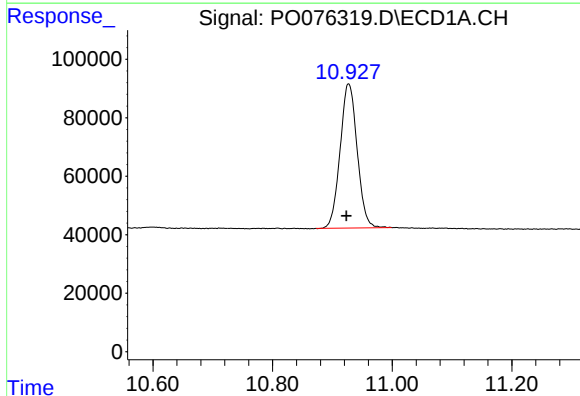

#2 Decachlorobiphenyl

R.T.: 10.927 min  
Delta R.T.: 0.003 min  
Response: 974775  
Conc: 25.34 ng/ml

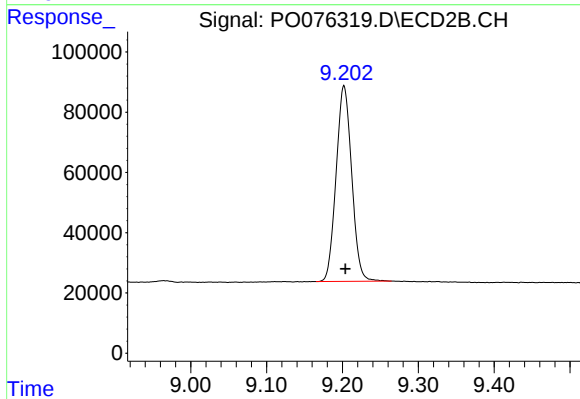

#2 Decachlorobiphenyl

R.T.: 9.202 min  
Delta R.T.: -0.002 min  
Response: 926353  
Conc: 24.13 ng/ml