

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
 Data File : P0076292.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Mar 2021 13:51
 Operator : DD\AJ
 Sample : M1682-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-MANHOLE

Manual Integrations
 APPROVED

Ankita
 3/19/2021 2:35:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 17:01:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 16 07:18:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.922	3.934	1572699	1111472	27.684	26.640
2)	SA Decachlor...	10.922	9.200	1166828	1046930	30.336	27.266
Target Compounds							
31)	L7 AR-1260-1	7.934	6.764	56437	48535	24.273	23.626m
32)	L7 AR-1260-2	8.200	6.961	81819	68754	32.044	28.350
33)	L7 AR-1260-3	8.568	7.111	34413	43509	17.359	19.238
34)	L7 AR-1260-4	8.799	7.594	28807	25169	12.751	13.061
35)	L7 AR-1260-5	9.123	7.842	74005	99213	18.105	22.441

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031821\
Data File : P0076292.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Mar 2021 13:51
Operator : DD\AJ
Sample : M1682-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SP-MANHOLE


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 17:01:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 16 07:18:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

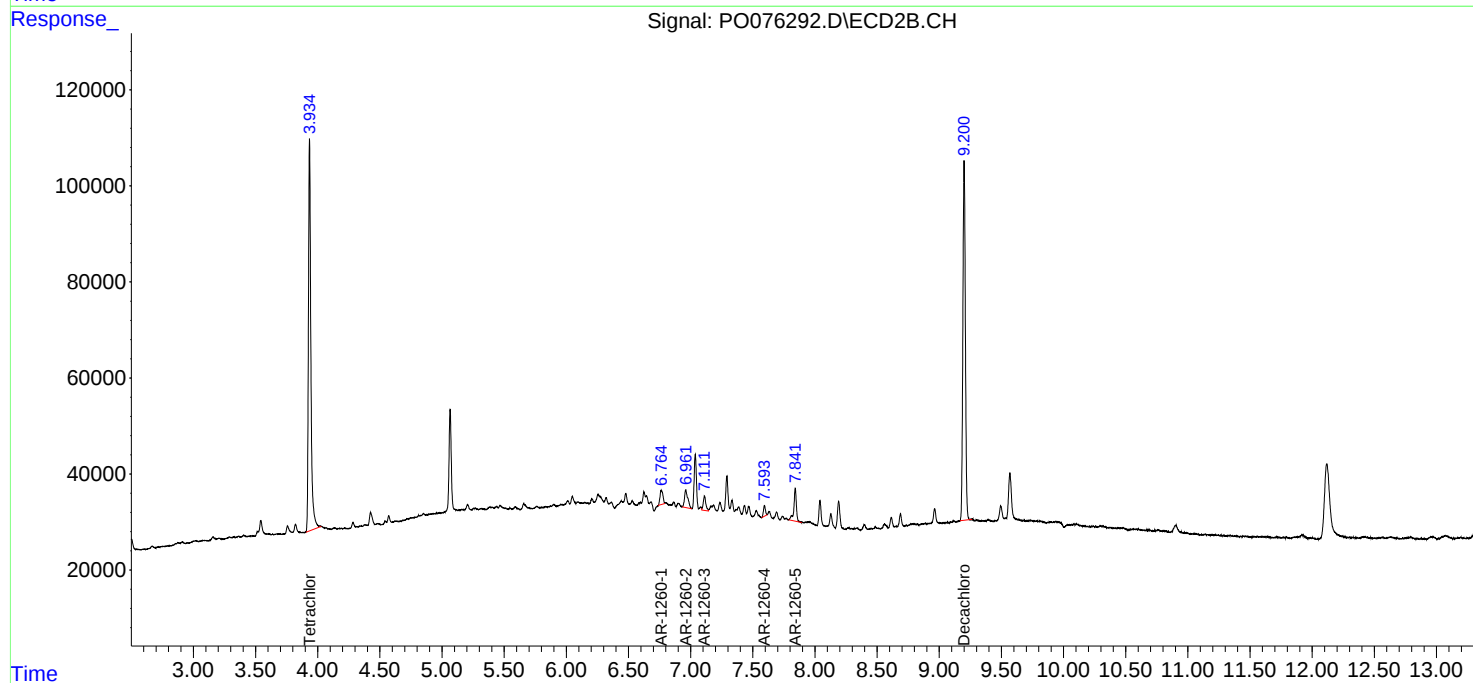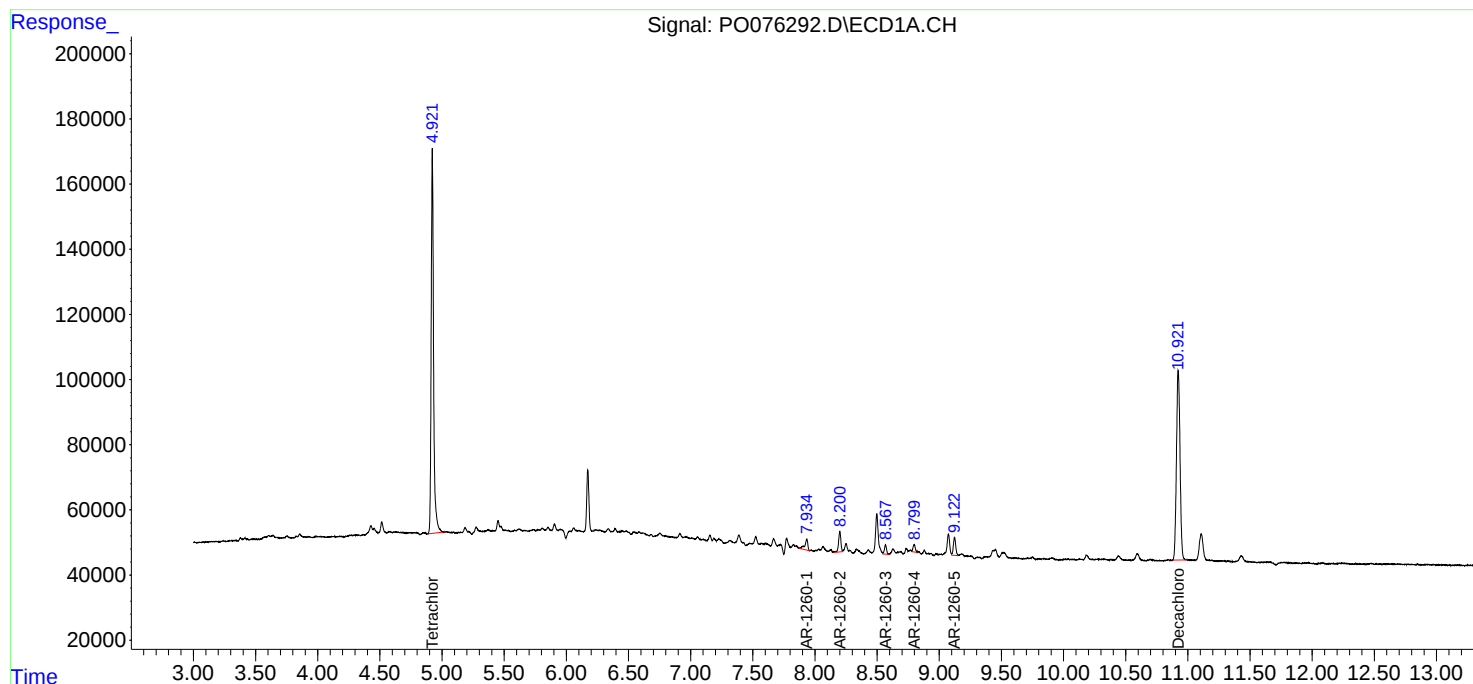

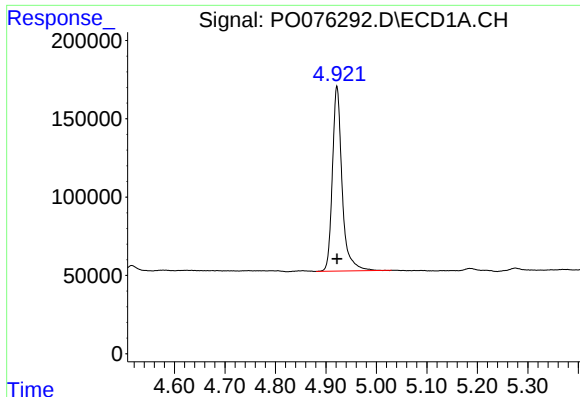


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 1572699
Conc: 27.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-MANHOLE


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:31 PM

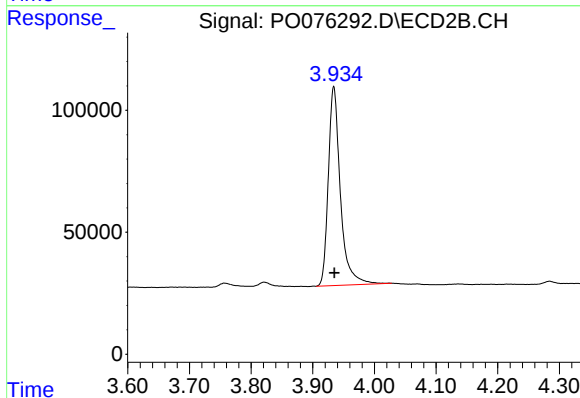


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.001 min
Response: 1111472
Conc: 26.64 ng/ml

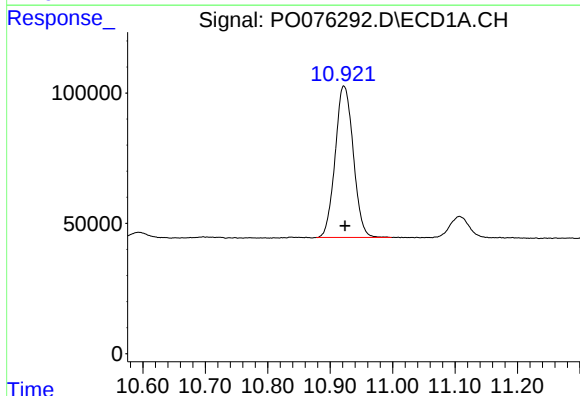


#2 Decachlorobiphenyl

R.T.: 10.922 min
Delta R.T.: -0.002 min
Response: 1166828
Conc: 30.34 ng/ml

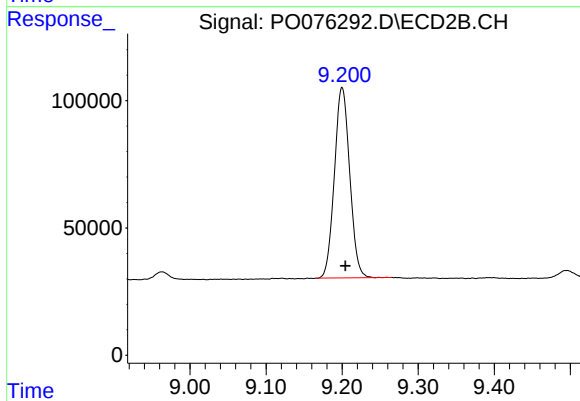

#2 Decachlorobiphenyl

R.T.: 9.200 min
Delta R.T.: -0.004 min
Response: 1046930
Conc: 27.27 ng/ml

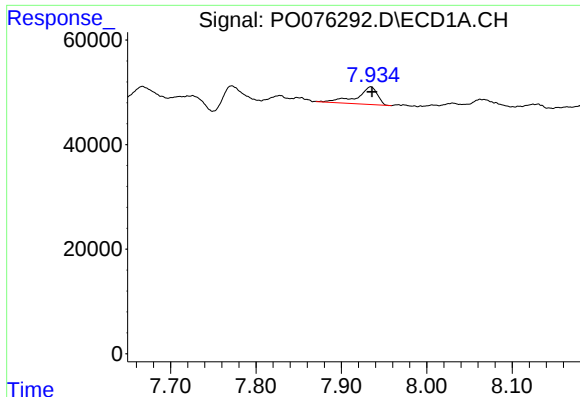


#31 AR-1260-1

R.T.: 7.934 min
Delta R.T.: -0.002 min
Response: 56437
Conc: 24.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-MANHOLE


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:31 PM

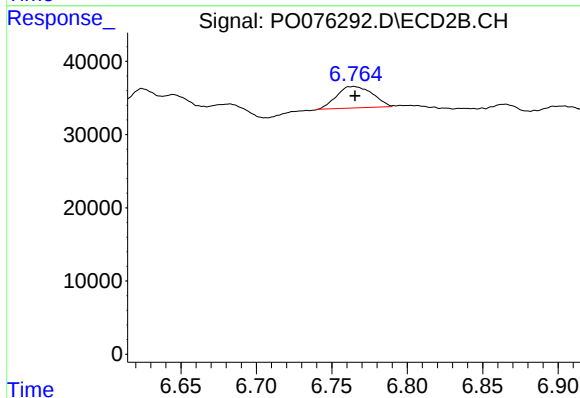


#31 AR-1260-1

R.T.: 6.764 min
Delta R.T.: -0.001 min
Response: 48535
Conc: 23.63 ng/ml m

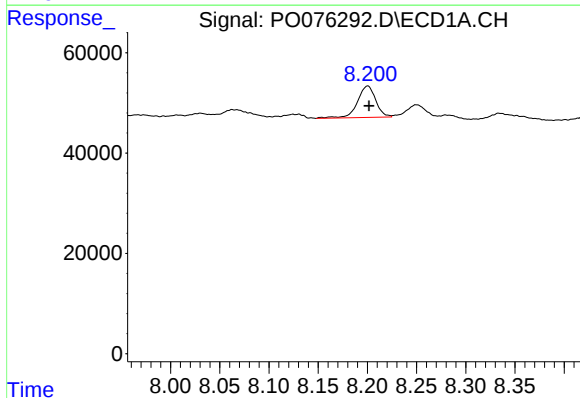


#32 AR-1260-2

R.T.: 8.200 min
Delta R.T.: -0.001 min
Response: 81819
Conc: 32.04 ng/ml

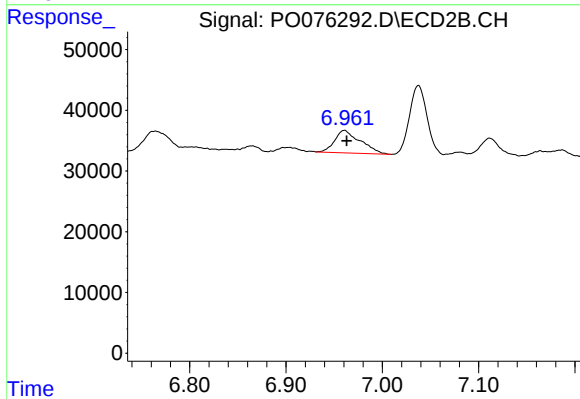

#32 AR-1260-2

R.T.: 6.961 min
Delta R.T.: -0.002 min
Response: 68754
Conc: 28.35 ng/ml

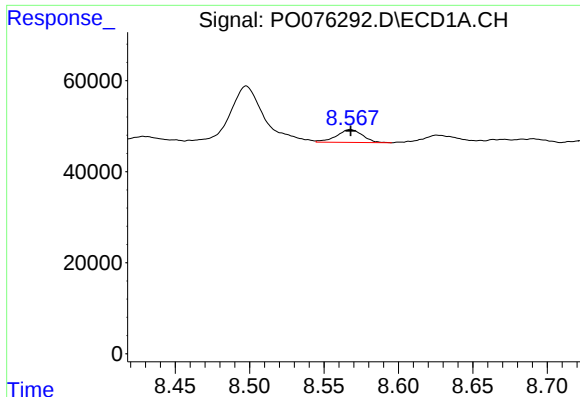


#33 AR-1260-3

R.T.: 8.568 min
Delta R.T.: 0.000 min
Response: 34413
Conc: 17.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-MANHOLE


Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:31 PM

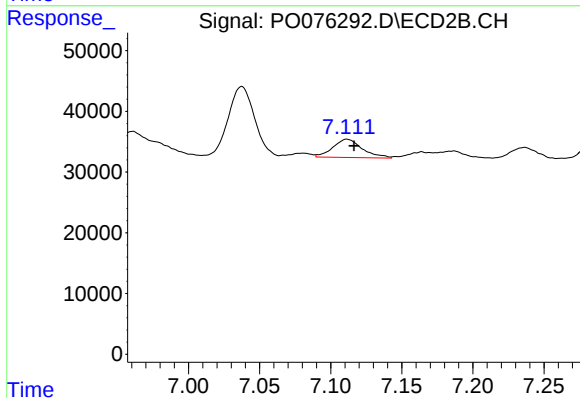


#33 AR-1260-3

R.T.: 7.111 min
Delta R.T.: -0.005 min
Response: 43509
Conc: 19.24 ng/ml

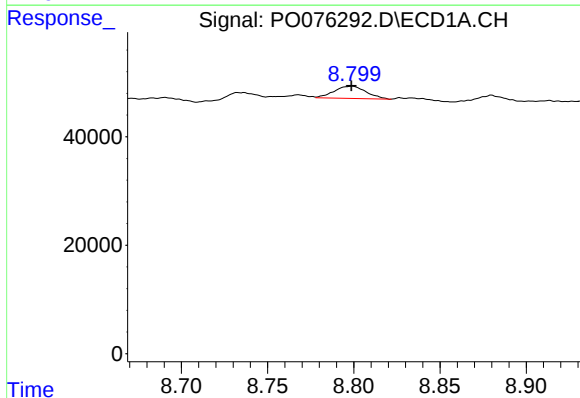


#34 AR-1260-4

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 28807
Conc: 12.75 ng/ml

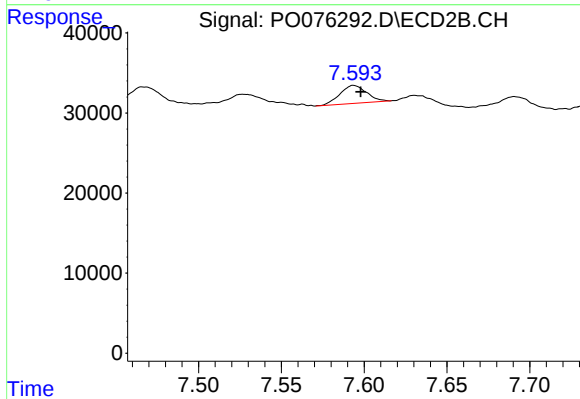

#34 AR-1260-4

R.T.: 7.594 min
Delta R.T.: -0.004 min
Response: 25169
Conc: 13.06 ng/ml

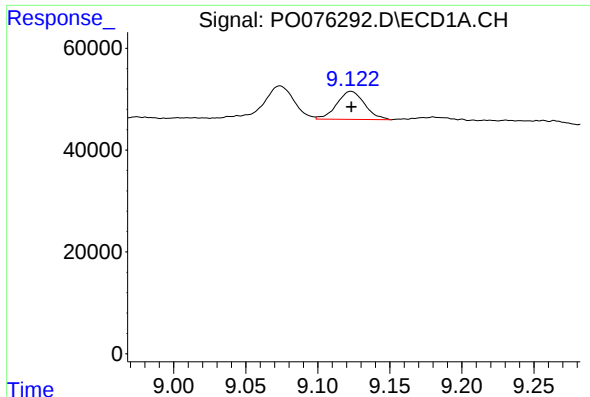


#35 AR-1260-5

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 74005
Conc: 18.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-MANHOLE

Manual Integrations
APPROVED

Ankita
3/19/2021 2:35:31 PM

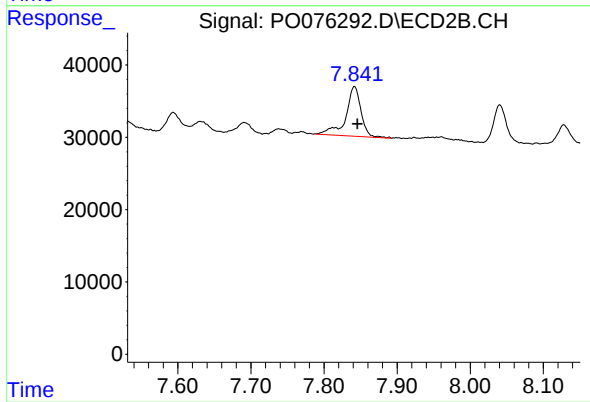

#35 AR-1260-5

R.T.: 7.842 min
Delta R.T.: -0.004 min
Response: 99213
Conc: 22.44 ng/ml